

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
 Data File : BN010516.D
 Acq On : 16 Apr 2020 13:00
 Operator : CG/JU
 Sample : L2191-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7A8

Quant Time: Apr 16 13:56:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	374378	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1648897	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1098103	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	2519143	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	2699482	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2373424	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	42460	5.93	ng/uL	0.00
5) Phenol-d5	6.79	99	973433	32.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	518332	34.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	816775	32.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	850405	34.12	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	416259	32.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	457417	32.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	888164	32.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1021049	32.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3030977	37.20	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	3540423	35.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	531692	33.52	ng/ul	0.00
58) Fluorene-d10	15.22	176	2744009	37.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	408797	31.07	ng/ul	0.00
71) Anthracene-d10	17.07	188	4493996	38.52	ng/ul	0.00
79) Pyrene-d10	19.37	212	5439169	35.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	4850514	39.40	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.69	163	633968	7.495	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010516.D
Acq On : 16 Apr 2020 13:00
Operator : CG/JU
Sample : L2191-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB7A8

Quant Time: Apr 16 13:56:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

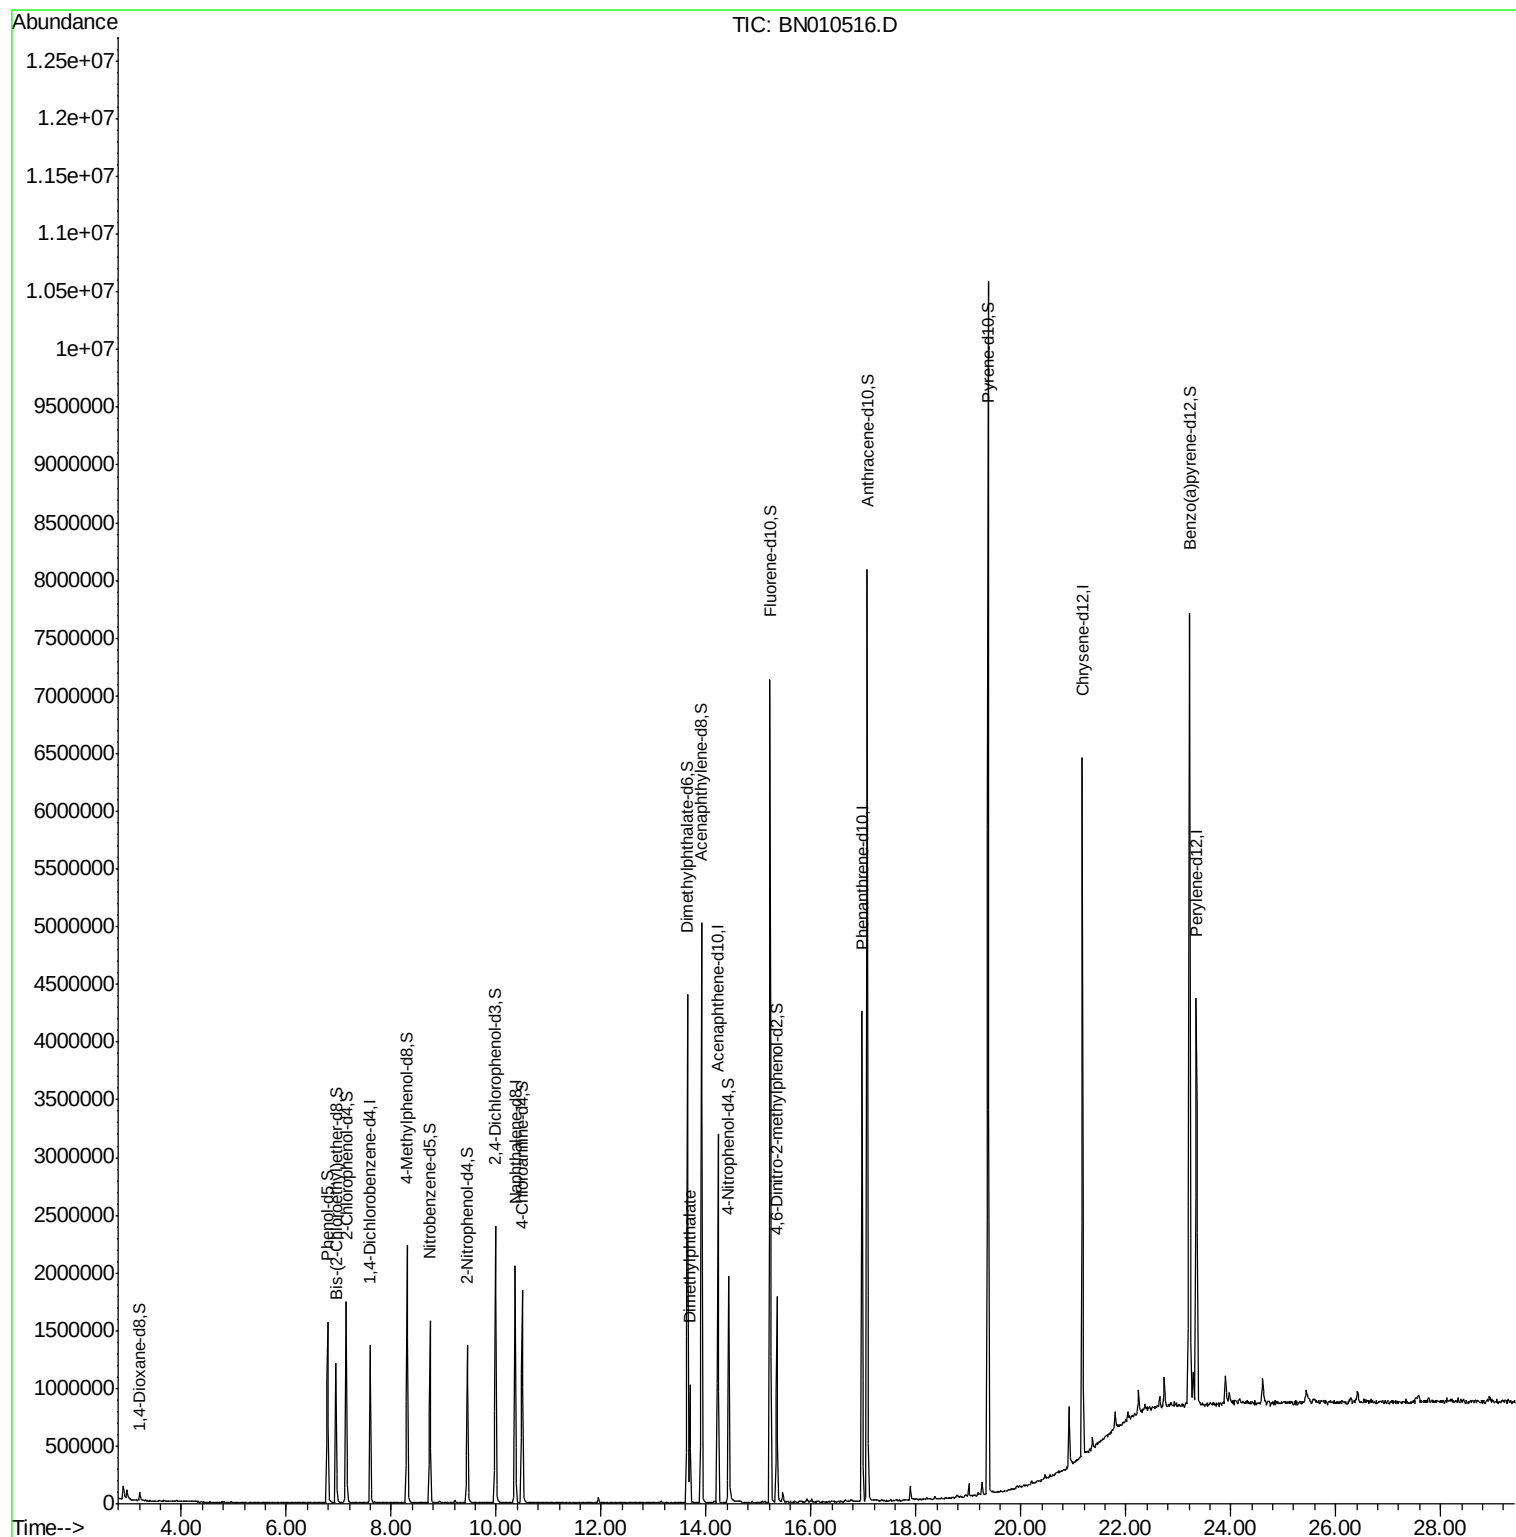

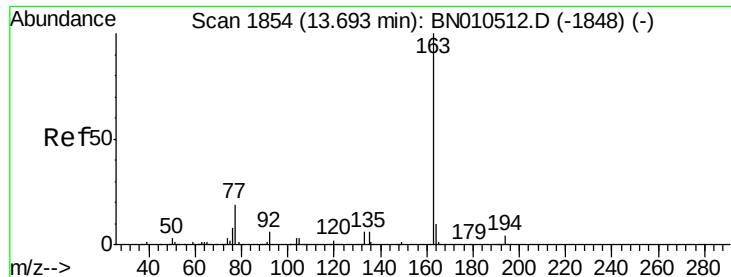

#45

Dimethylphthalate

Concen: 7.495 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010516.D

Acq: 16 Apr 2020 13:00

Instrument :

BNA_N

ClientSampleId :

CB7A8


Tot Ion:163 Resp: 633968

Ion Ratio Lower Upper

163 100

194 4.5 3.3 4.9

164 10.8 8.0 12.0

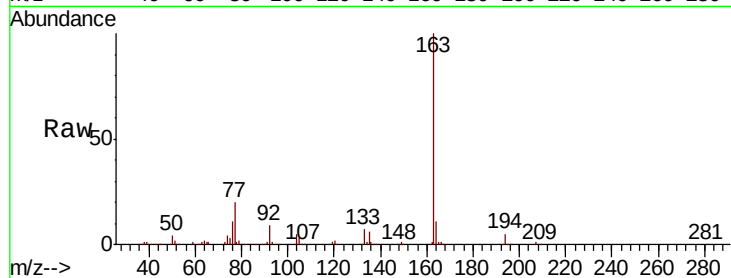

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

