

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041620\
 Data File : BN010531.D
 Acq On : 17 Apr 2020 00:05
 Operator : CG/JU
 Sample : L2191-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB7A2

Manual Integrations
 APPROVED

mohammad
 4/17/2020 1:52:20 PM

Quant Time: Apr 17 02:32:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	554272	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2392190	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1534465	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3339532	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	3235184	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2913424	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	77283	7.30	ng/uL	0.00
5) Phenol-d5	6.78	99	1664904	38.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	892262	40.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	1410633	37.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	1360207	36.86	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	745885	40.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	820416	39.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1482203	36.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1515083	32.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	4612476	40.51	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	5616338	40.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	796808	35.95	ng/ul	0.00
58) Fluorene-d10	15.22	176	4054230	39.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	669059	38.35	ng/ul	0.00
71) Anthracene-d10	17.07	188	6119116	39.56	ng/ul	0.00
79) Pyrene-d10	19.37	212	7084430	38.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	6353110	42.04	ng/ul	0.00

Target Compounds

					Ovalue	
28) Naphthalene	10.40	128	323592	2.517	ng/ul	99
34) 2-Methylnaphthalene	12.02	142	187053	2.059	ng/ul	99
45) Dimethylphthalate	13.69	163	139150	1.177	ng/ul	99
50) Acenaphthene	14.29	153	461685	4.571	ng/ul	98
54) Dibenzofuran	14.62	168	627599	4.438	ng/ul	99
59) Fluorene	15.27	166	703908	6.071	ng/ul	98
70) Phenanthrene	17.02	178	8100617	43.680	ng/ul	99
72) Anthracene	17.10	178	1795120	9.549	ng/ul	99
75) Carbazole	17.37	167	603286	3.907	ng/ul	98
77) Fluoranthene	19.04	202	8429441	41.833	ng/ul	97
80) Pyrene	19.40	202	7311109	31.277	ng/ul	98
83) Benzo(a)anthracene	21.16	228	3991327	17.784	ng/ul	99
85) Chrysene	21.21	228	3481652	16.499	ng/ul	98
88) Benzo(b)fluoranthene	22.70	252	3498286	18.401	ng/ul	98
89) Benzo(k)fluoranthene	22.74	252	1380031m	7.317	ng/ul	
91) Benzo(a)pyrene	23.25	252	2343523	13.875	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.49	276	1365551	7.183	ng/ul	96
93) Dibenzo(a,h)anthracene	25.49	278	399124	2.500	ng/ul#	86
94) Benzo(g,h,i)perylene	26.14	276	884529	5.622	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041620\
Data File : BN010531.D
Acq On : 17 Apr 2020 00:05
Operator : CG/JU
Sample : L2191-09
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
CB7A2

Manual Integrations
APPROVED

mohammad
4/17/2020 1:52:20 PM

Quant Time: Apr 17 02:32:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

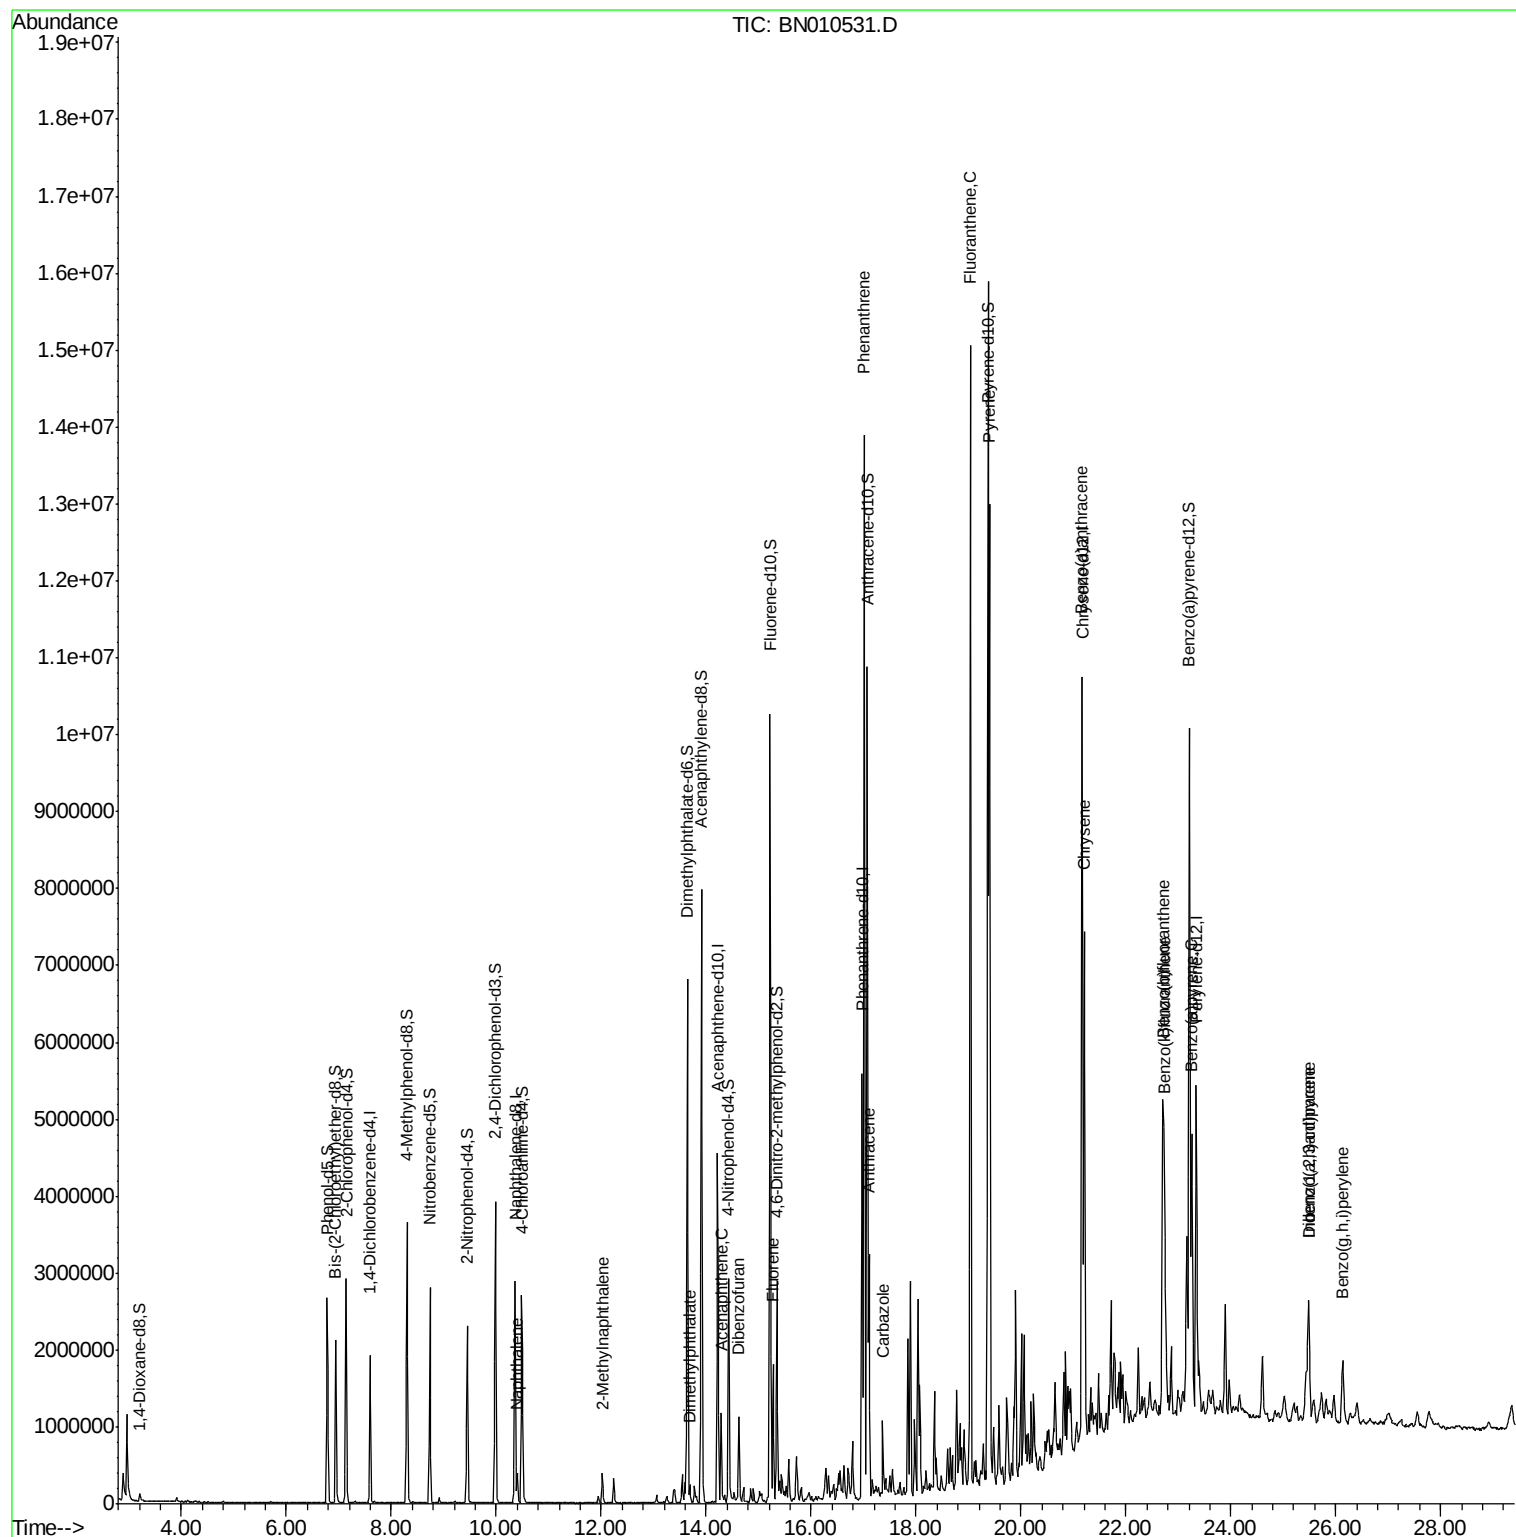

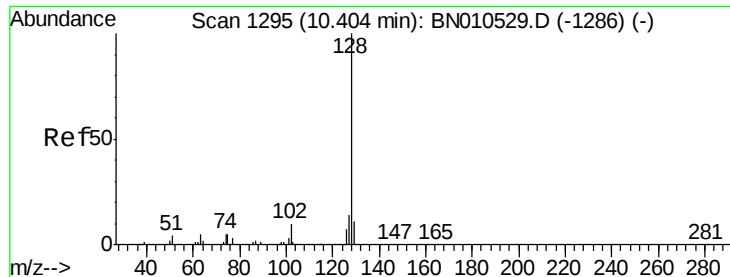





#28
Naphthalene
Concen: 2.517 ng/ul
RT: 10.40 min Scan# 1295
Delta R.T. 0.00 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Instrument :
BNA_N
ClientSampled :
CB7A2

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.2	8.6	13.0
127	13.1	10.7	16.1




Manual Integrations
APPROVED


mohammad
4/17/2020 1:52:20 PM

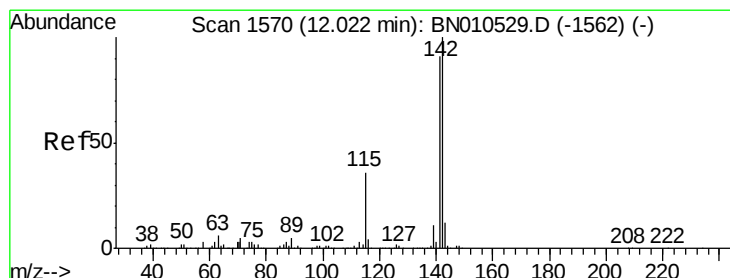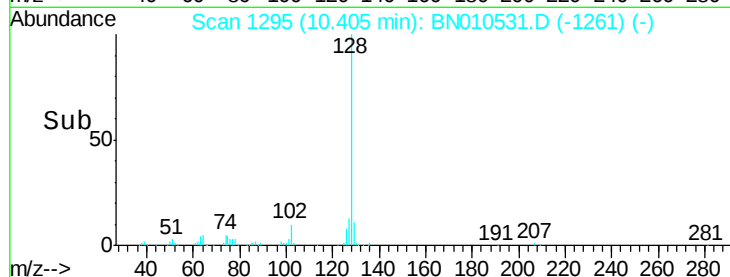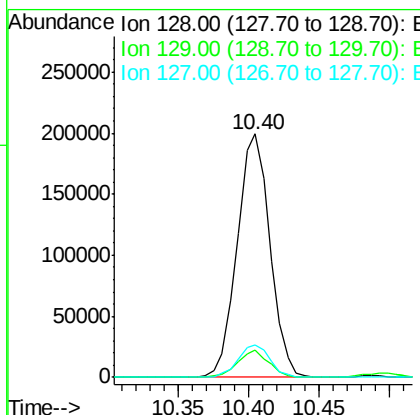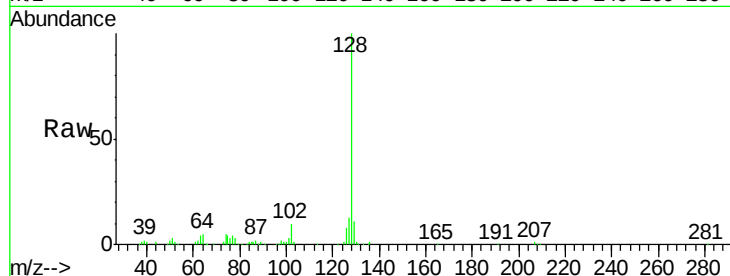

#34
2-Methylnaphthalene
Concen: 2.059 ng/ul
RT: 12.02 min Scan# 1570
Delta R.T. 0.00 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.3	71.8	107.8

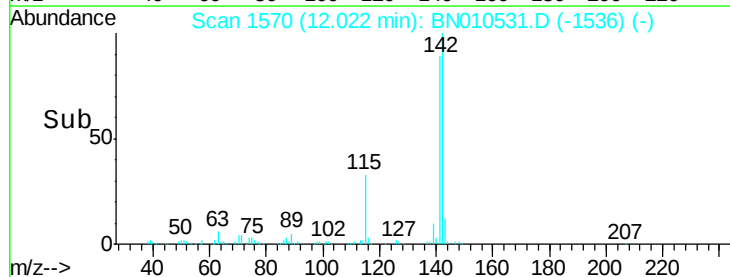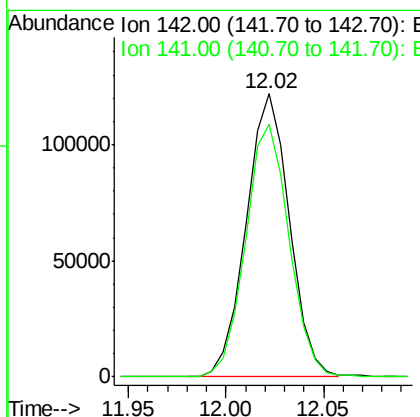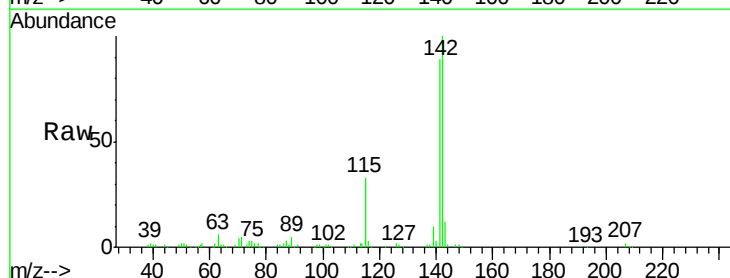

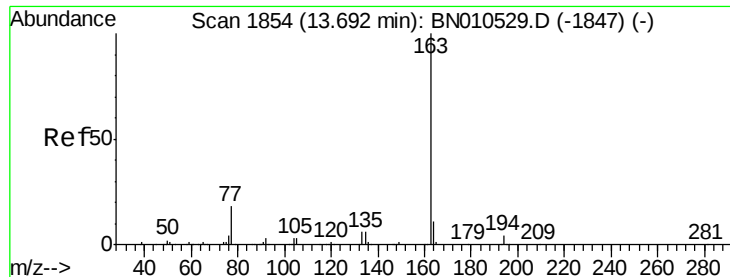


#45
Dimethylphthalate
Concen: 1.177 ng/ul
RT: 13.69 min Scan# 1853
Delta R.T. -0.01 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Instrument :
BNA_N
ClientSampleId :
CB7A2




Tot Ion	Ratio	Resp	Lower	Upper
163	100	139150		
194	4.4	3.3	4.9	
164	9.9	8.0	12.0	

Manual Integrations
APPROVED

mohammad
4/17/2020 1:52:20 PM

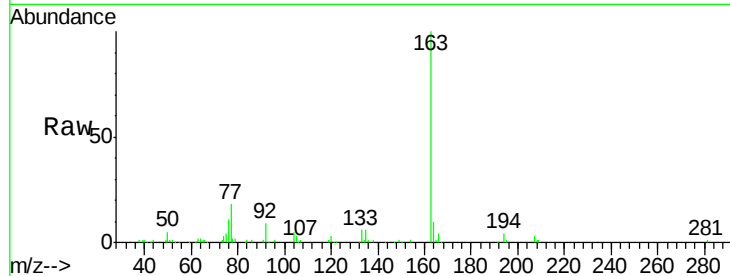


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

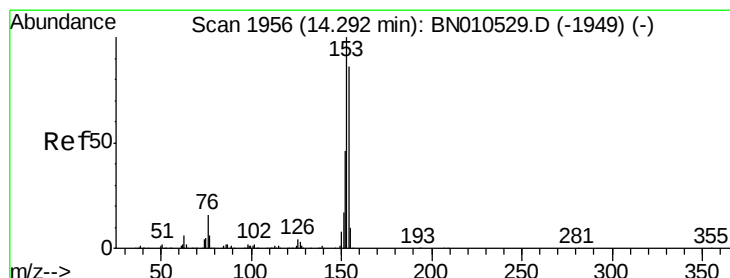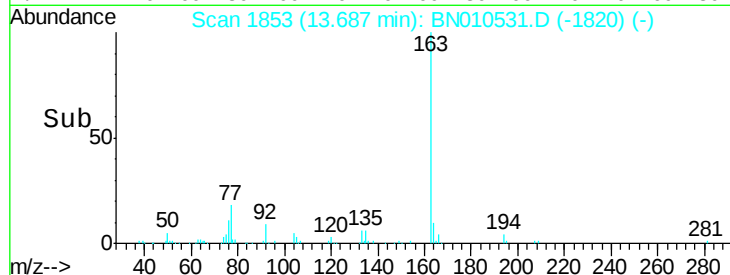
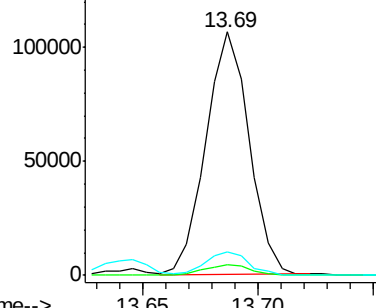



#50
Acenaphthene
Concen: 4.571 ng/ul
RT: 14.29 min Scan# 1955
Delta R.T. -0.01 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	461685		
152	47.0	36.8	55.2	
154	87.5	68.2	102.2	

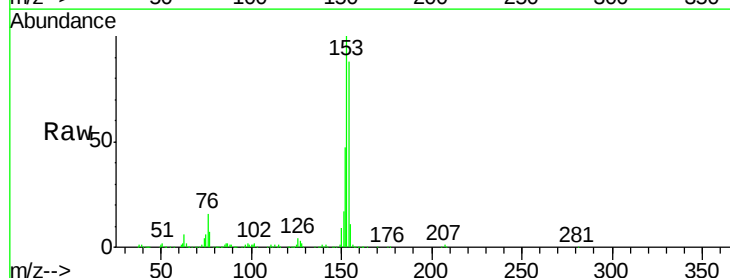

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

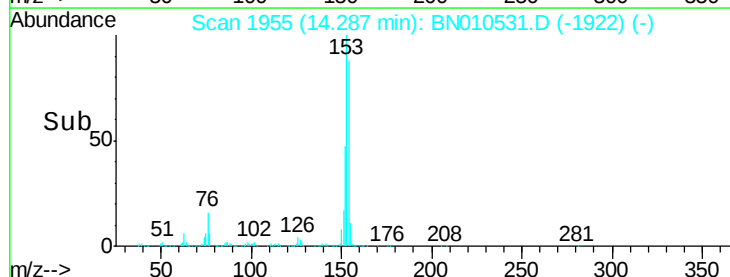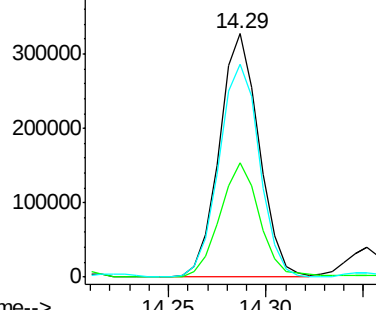

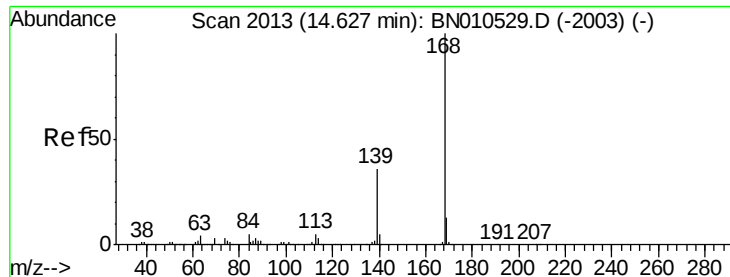

#54

Dibenzenofuran

Concen: 4.438 ng/ul

RT: 14.62 min Scan# 2012

Delta R.T. -0.01 min

Lab File: BN010531.D

Acq: 17 Apr 2020 00:05

Instrument :

BNA_N

ClientSampled :

CB7A2

Tot Ion:168 Resp: 627599





Ion Ratio Lower Upper

168 100

139 37.2 30.2 45.4

Manual Integrations
APPROVED

mohammad
4/17/2020 1:52:20 PM

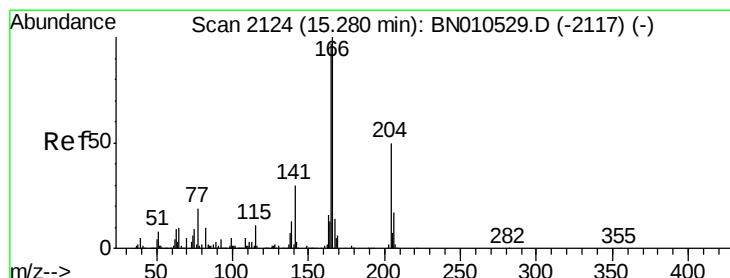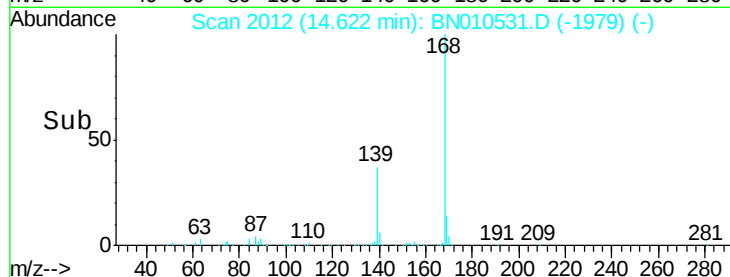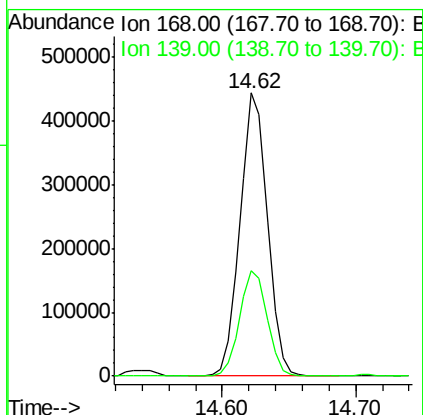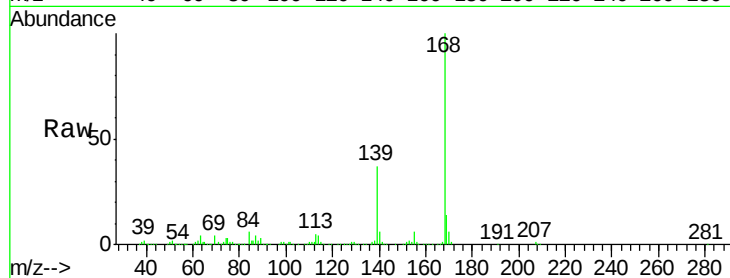

#59

Fluorene

Concen: 6.071 ng/ul

RT: 15.27 min Scan# 2123

Delta R.T. -0.01 min

Lab File: BN010531.D

Acq: 17 Apr 2020 00:05




Tgt Ion:166 Resp: 703908


Ion Ratio Lower Upper

166 100

165 97.1 75.9 113.9

167 13.9 11.2 16.8

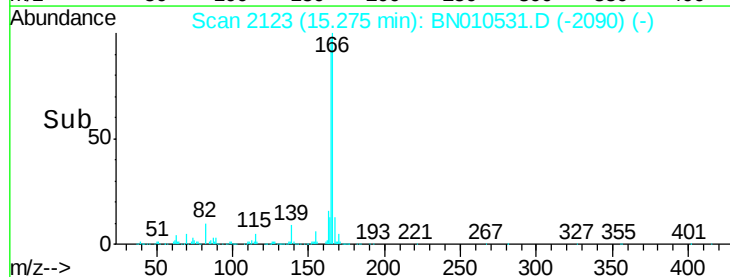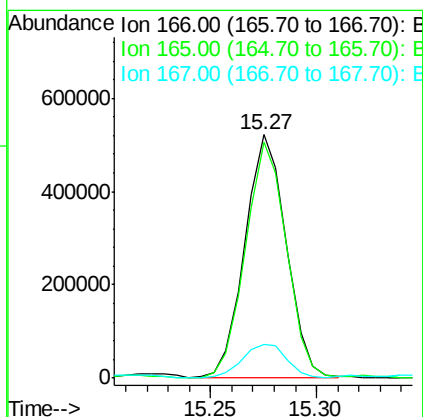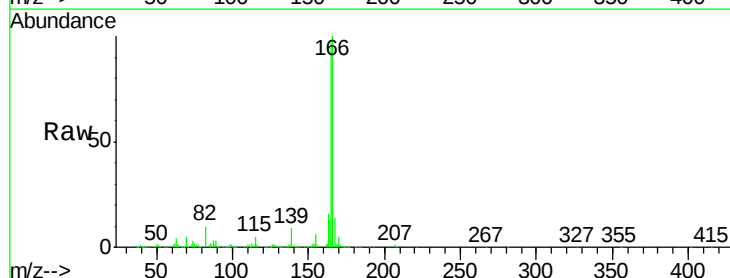

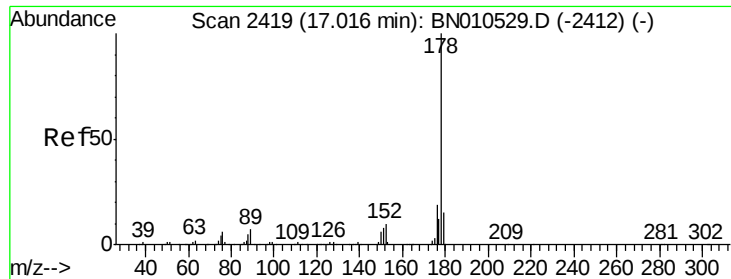

#70

Phenanthrene

Concen: 43.680 ng/ul

RT: 17.02 min Scan# 2419

Delta R.T. 0.00 min

Lab File: BN010531.D

Acq: 17 Apr 2020 00:05

Instrument :

BNA_N

ClientSampleId :

CB7A2

Tot Ion:178 Resp: 8100617

Ion Ratio Lower Upper


178 100

179 15.3 11.4 17.2




176 19.3 15.3 22.9

Manual Integrations
APPROVED

mohammad
4/17/2020 1:52:20 PM

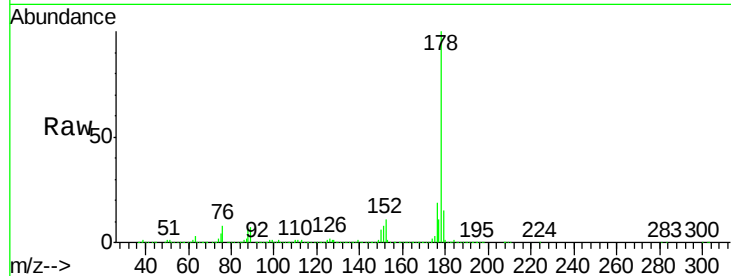

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

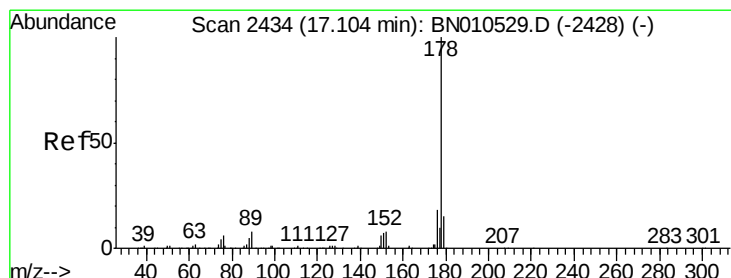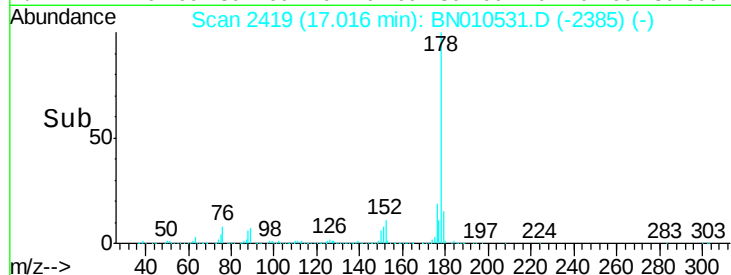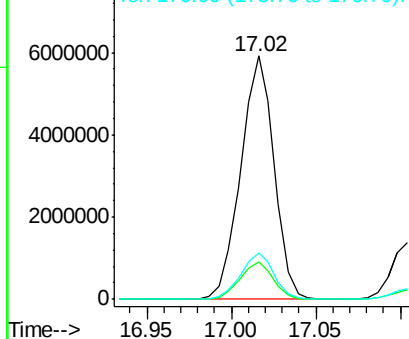

#72

Anthracene

Concen: 9.549 ng/ul

RT: 17.10 min Scan# 2434

Delta R.T. 0.00 min

Lab File: BN010531.D

Acq: 17 Apr 2020 00:05


Tgt Ion:178 Resp: 1795120

Ion Ratio Lower Upper



178 100


179 16.1 12.3 18.5

176 18.3 14.2 21.4

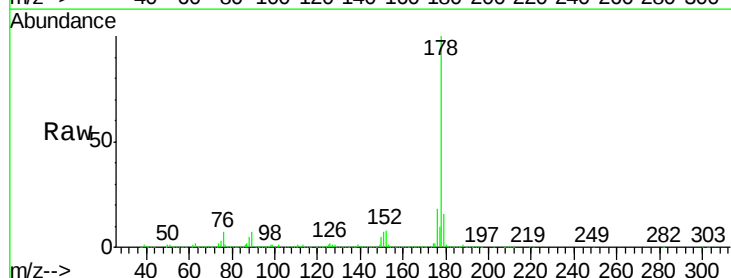

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

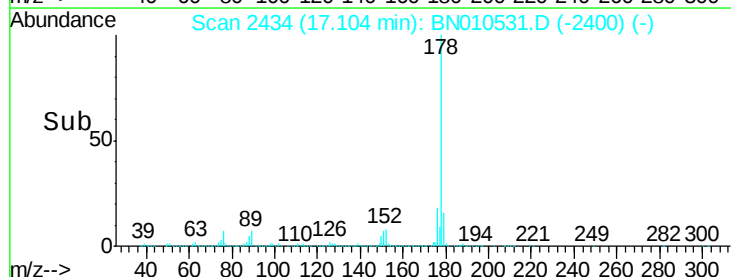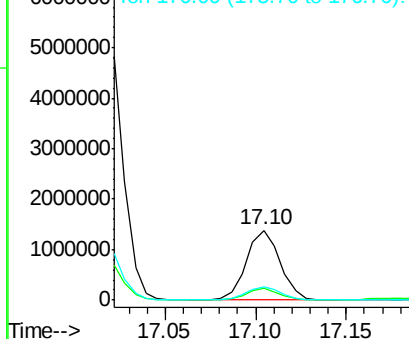

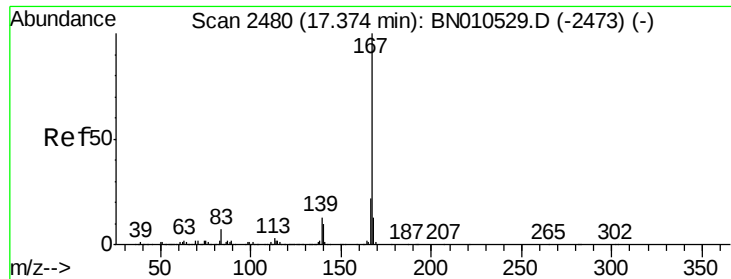





#75
 Carbazole
 Concen: 3.907 ng/ul
 RT: 17.37 min Scan# 2479
 Delta R.T. -0.01 min
 Lab File: BN010531.D
 Acq: 17 Apr 2020 00:05

Instrument :
 BNA_N
 ClientSampled :
 CB7A2

Tot Ion	Ratio	Lower	Upper
167	100		
166	22.4	16.8	25.2
139	12.7	10.1	15.1




Manual Integrations
 APPROVED


mohammad
 4/17/2020 1:52:20 PM

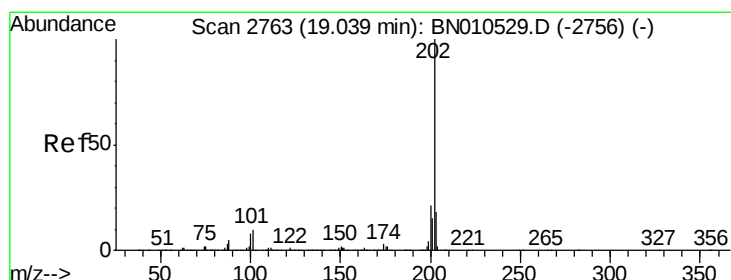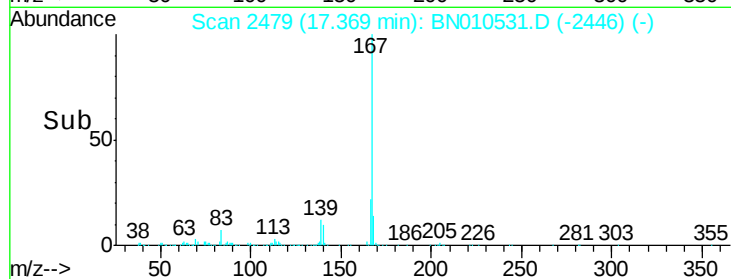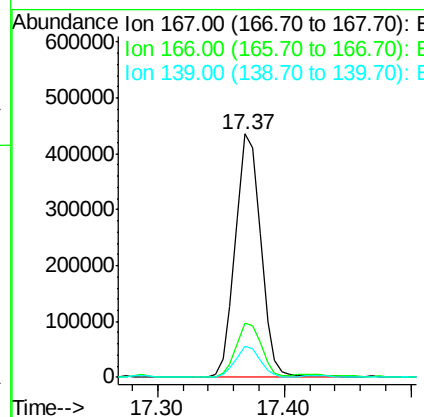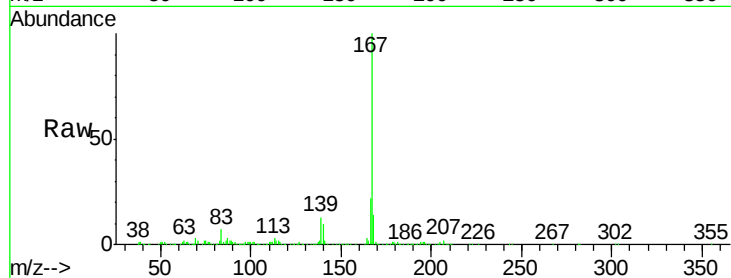

#77
 Fluoranthene
 Concen: 41.833 ng/ul
 RT: 19.04 min Scan# 2763
 Delta R.T. 0.00 min
 Lab File: BN010531.D
 Acq: 17 Apr 2020 00:05

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.2	7.1	10.7
100	7.9	5.5	8.3

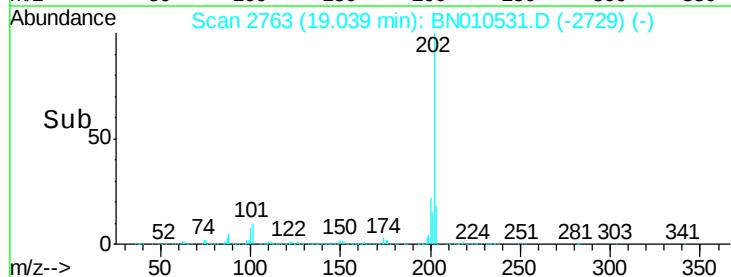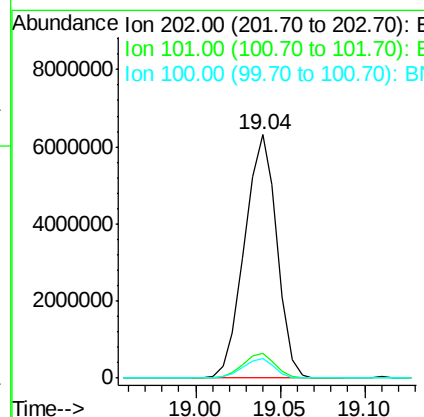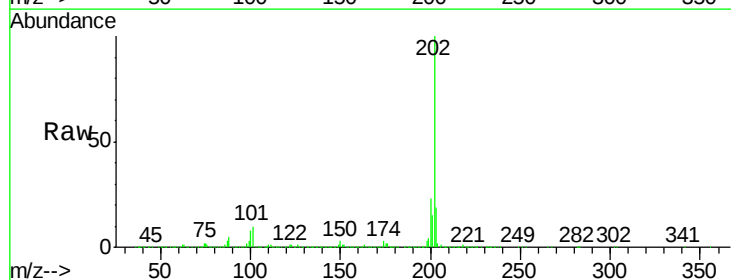

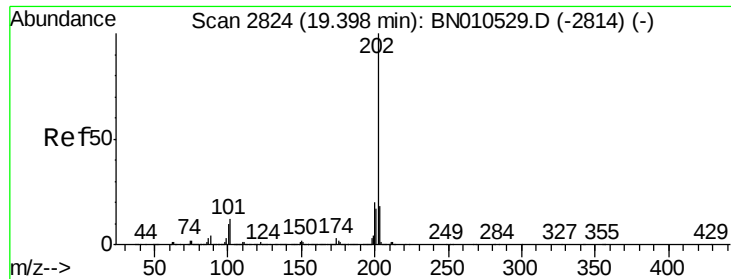





#80
Pvrene
Concen: 31.277 ng/ul
RT: 19.40 min Scan# 2825
Delta R.T. 0.00 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Instrument :
BNA_N
ClientSampleId :
CB7A2

Tot Ion	Ratio	Lower	Upper
202	100		
101	11.5	8.6	13.0
100	9.3	7.0	10.6




Manual Integrations
APPROVED


mohammad
4/17/2020 1:52:20 PM

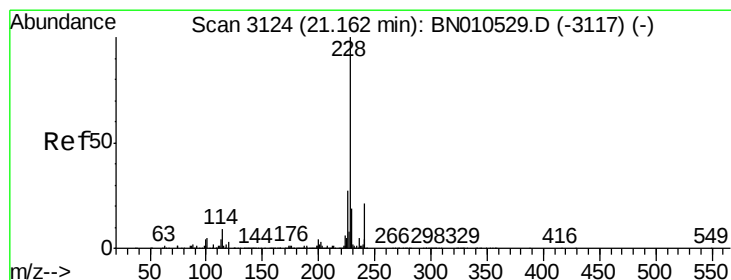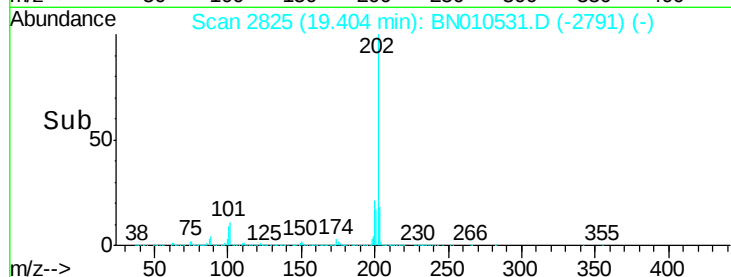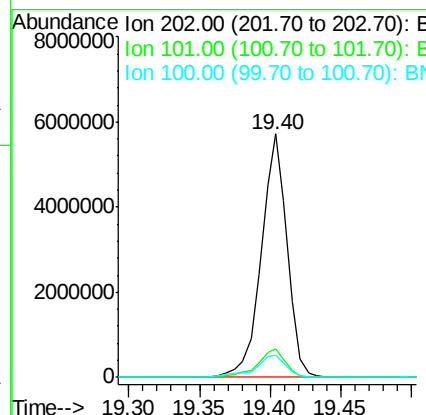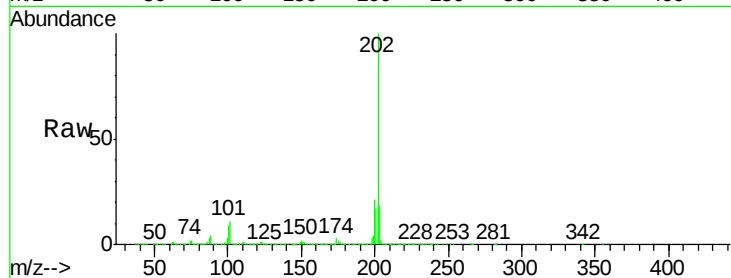

#83
Benzo(a)anthracene
Concen: 17.784 ng/ul
RT: 21.16 min Scan# 3123
Delta R.T. -0.01 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.3	16.0	24.0
226	26.0	21.4	32.2

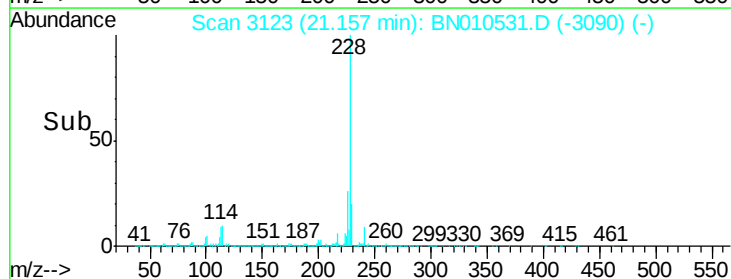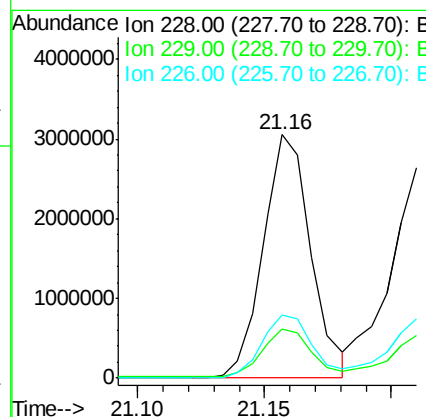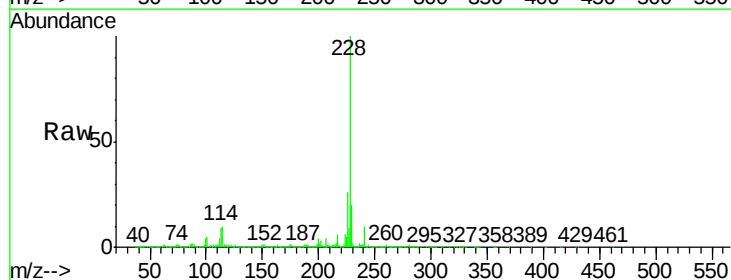

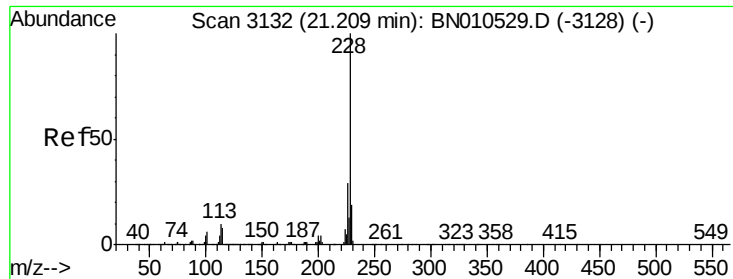





#85
Chrysene
Concen: 16.499 ng/ul
RT: 21.21 min Scan# 3132
Delta R.T. -0.01 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Instrument :
BNA_N
ClientSampleId :
CB7A2

Tot Ion	Ratio	Lower	Upper
228	100		
226	28.3	23.0	34.6
229	20.0	15.0	22.4




Manual Integrations
APPROVED


mohammad
4/17/2020 1:52:20 PM

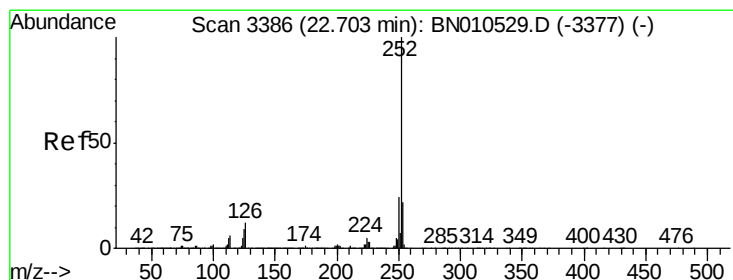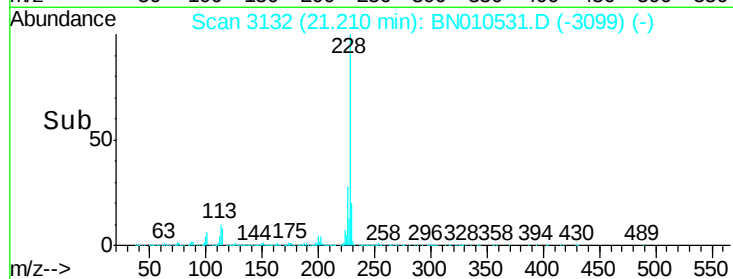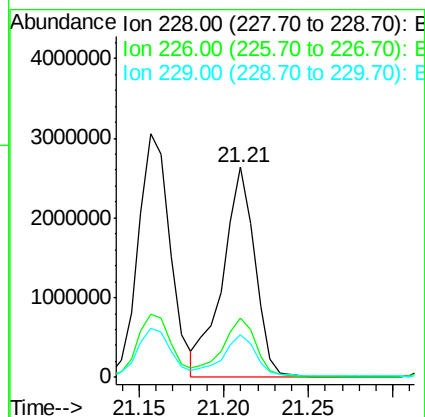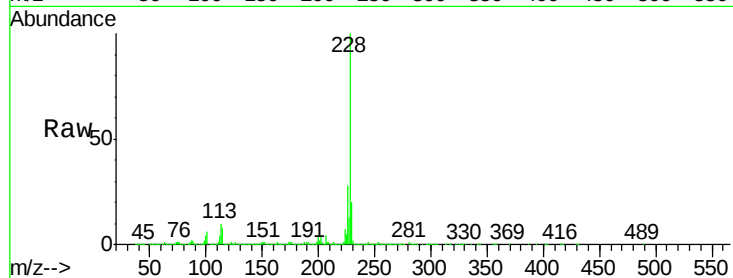

#88
Benzo(b)fluoranthene
Concen: 18.401 ng/ul
RT: 22.70 min Scan# 3386
Delta R.T. 0.00 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.8	16.7	25.1
125	9.9	7.2	10.8

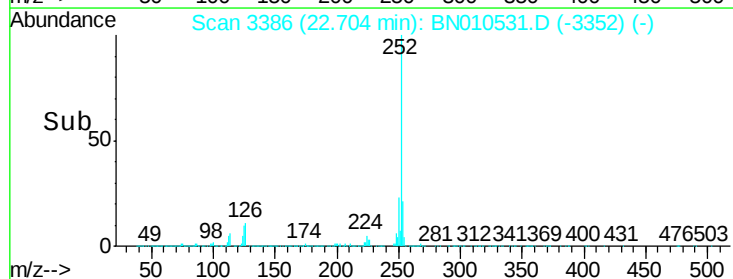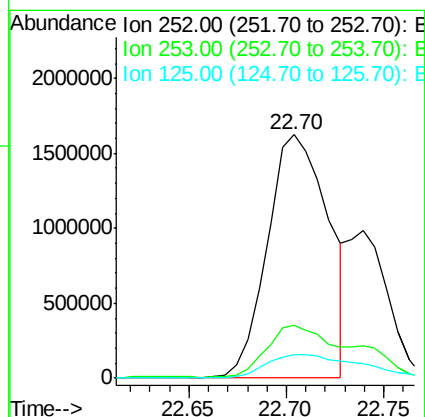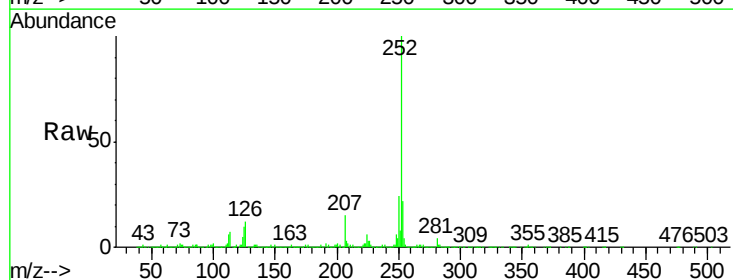

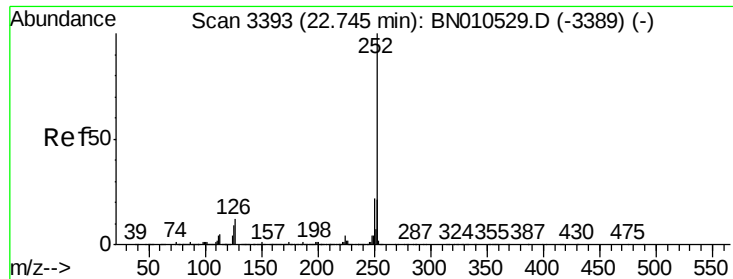

#89

Benzo(k)fluoranthene

Concen: 7.317 ng/ul m

RT: 22.74 min Scan# 3392

Delta R.T. -0.01 min

Lab File: BN010531.D

Acq: 17 Apr 2020 00:05

Instrument :

BNA_N

ClientSampled :

CB7A2

Tot Ion:252 Resp: 1380031

Ion Ratio Lower Upper


252 100

253 21.6 17.4 26.2




125 9.9 6.9 10.3

Manual Integrations
APPROVED

mohammad
4/17/2020 1:52:20 PM

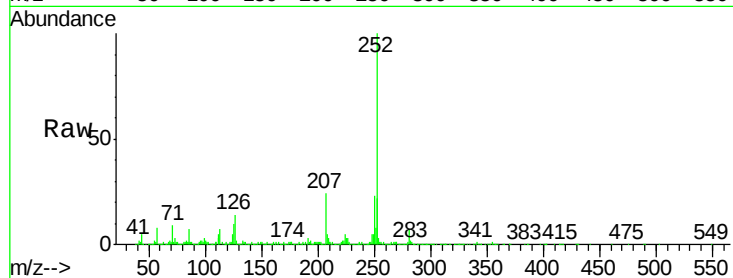

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

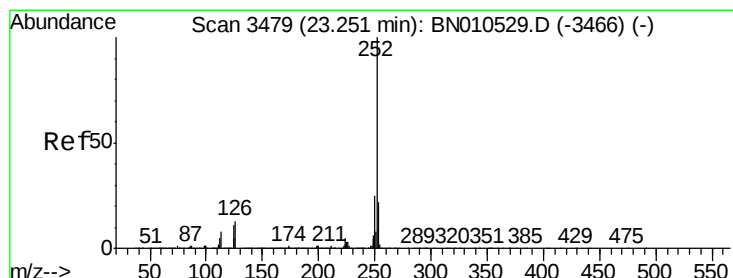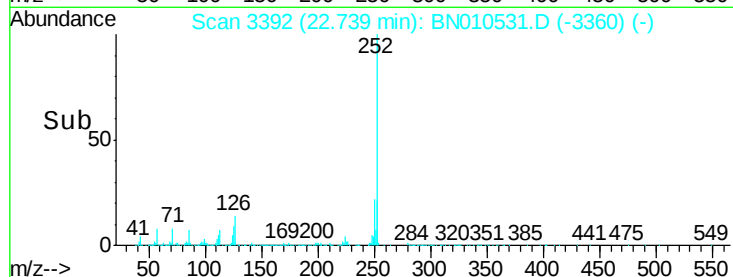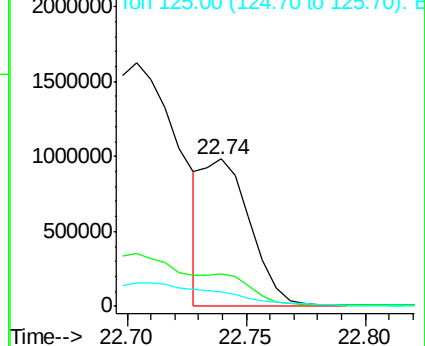

#91

Benzo(a)pyrene

Concen: 13.875 ng/ul

RT: 23.25 min Scan# 3479

Delta R.T. -0.01 min

Lab File: BN010531.D

Acq: 17 Apr 2020 00:05


Tgt Ion:252 Resp: 2343523

Ion Ratio Lower Upper



252 100


253 22.5 17.8 26.8

125 10.5 7.8 11.6

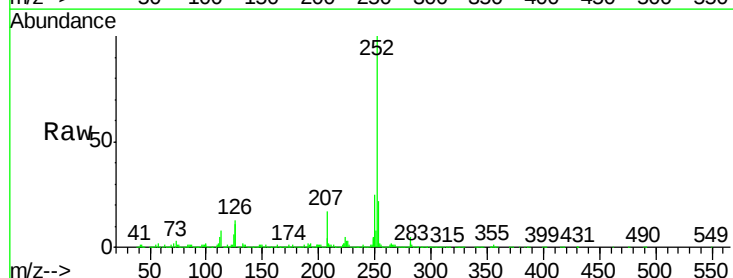

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

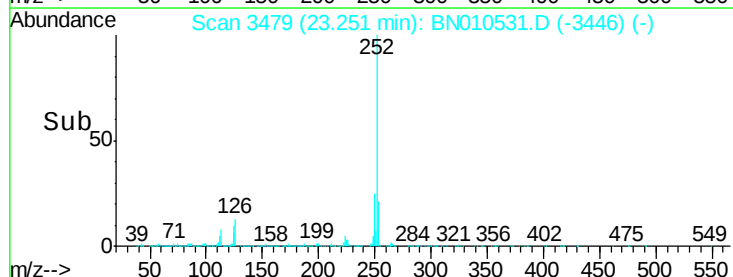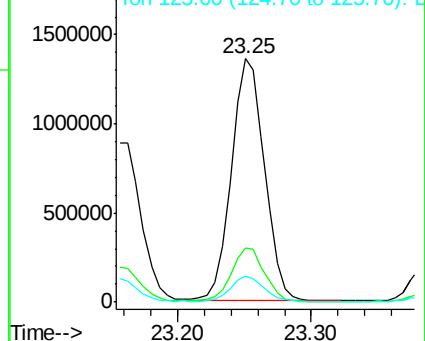

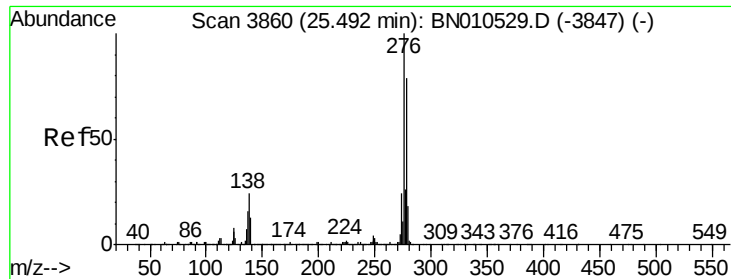

#92





Indeno(1,2,3-cd)pyrene
Concen: 7.183 ng/ul
RT: 25.49 min Scan# 3859
Delta R.T. -0.01 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Instrument :
BNA_N
ClientSampleId :
CB7A2

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.8	18.3	27.5
277	24.0	19.8	29.8

Manual Integrations
APPROVED




mohammad
4/17/2020 1:52:20 PM

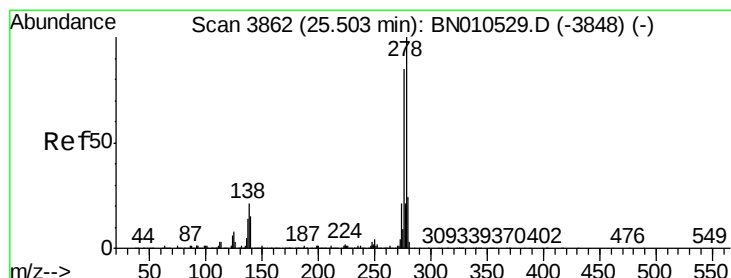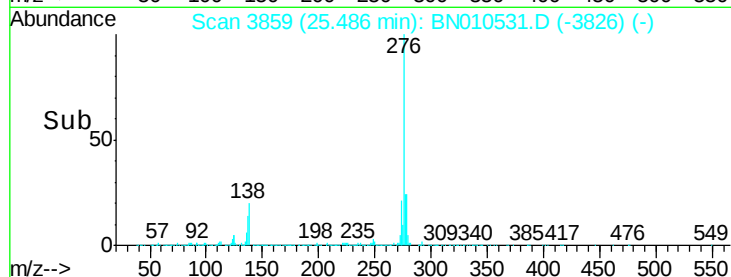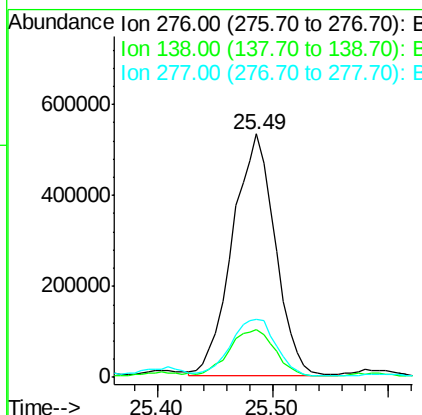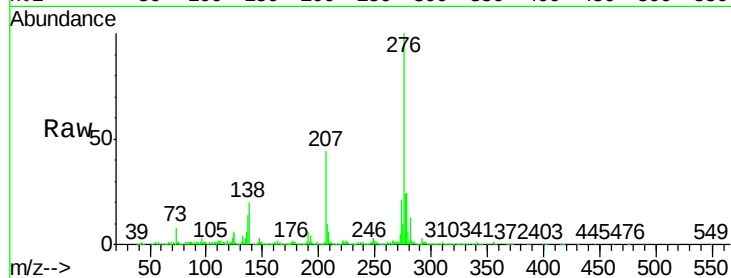


#93

Dibenzo(a,h)anthracene
Concen: 2.500 ng/ul
RT: 25.49 min Scan# 3859
Delta R.T. -0.02 min
Lab File: BN010531.D
Acq: 17 Apr 2020 00:05

Tgt Ion	Ratio	Lower	Upper
278	100		
139	0.0	11.5	17.3#
279	24.4	19.2	28.8

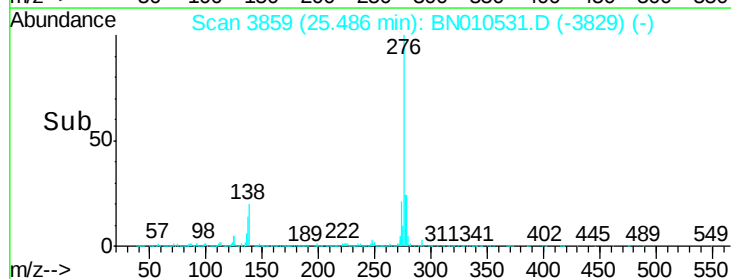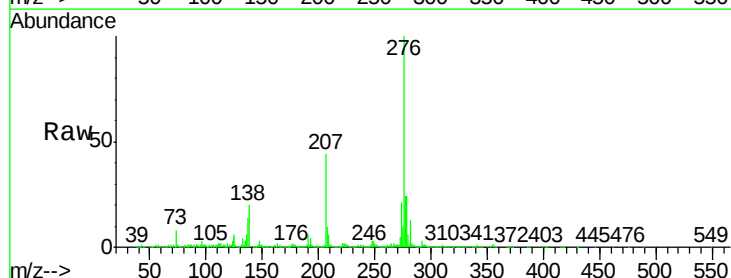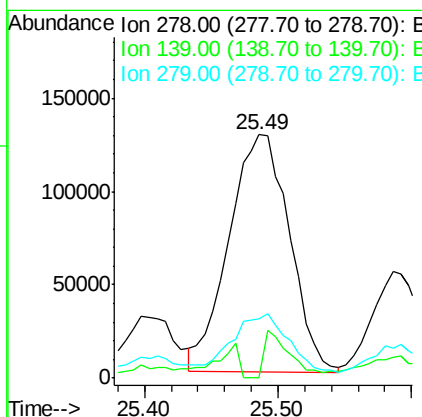

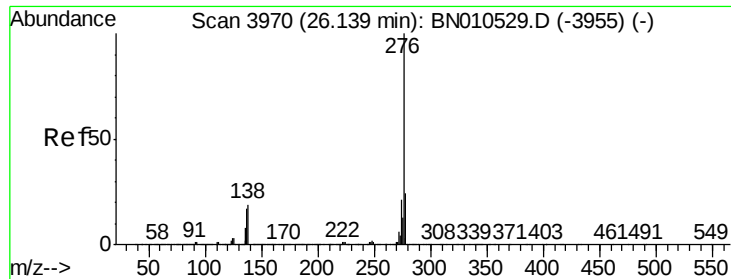

#94
 Benzo(a,h,i)perylene
 Concen: 5.622 ng/ul
 RT: 26.14 min Scan# 3970
 Delta R.T. -0.01 min
 Lab File: BN010531.D
 Acq: 17 Apr 2020 00:05

Instrument :
 BNA_N
 ClientSampleId :
 CB7A2

Tot Ion	Ratio	Lower	Upper
276	100		
138	20.3	14.7	22.1
277	24.4	18.4	27.6

Manual Integrations
 APPROVED

mohammad
 4/17/2020 1:52:20 PM

