

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
 Data File : BN010537.D
 Acq On : 17 Apr 2020 03:40
 Operator : CG/JU
 Sample : L2176-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG2H8

Quant Time: Apr 17 05:00:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	470460	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2091936	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1352926	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3027162	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	2898934	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2623934	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	41000	4.56	ng/uL	0.00
5) Phenol-d5	6.78	99	951209	25.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	517072	27.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	808136	25.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	844749	26.97	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	422774	26.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	467758	26.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	884625	25.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1279972	31.70	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	2915432	29.04	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	3403403	27.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	478948	24.51	ng/ul	0.00
58) Fluorene-d10	15.22	176	2562819	28.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	372712	23.57	ng/ul	0.00
71) Anthracene-d10	17.07	188	4139581	29.52	ng/ul	0.00
79) Pyrene-d10	19.37	212	4680245	28.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	3930880	28.88	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.69	163	1028557	9.869	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010537.D
Acq On : 17 Apr 2020 03:40
Operator : CG/JU
Sample : L2176-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG2H8

Quant Time: Apr 17 05:00:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

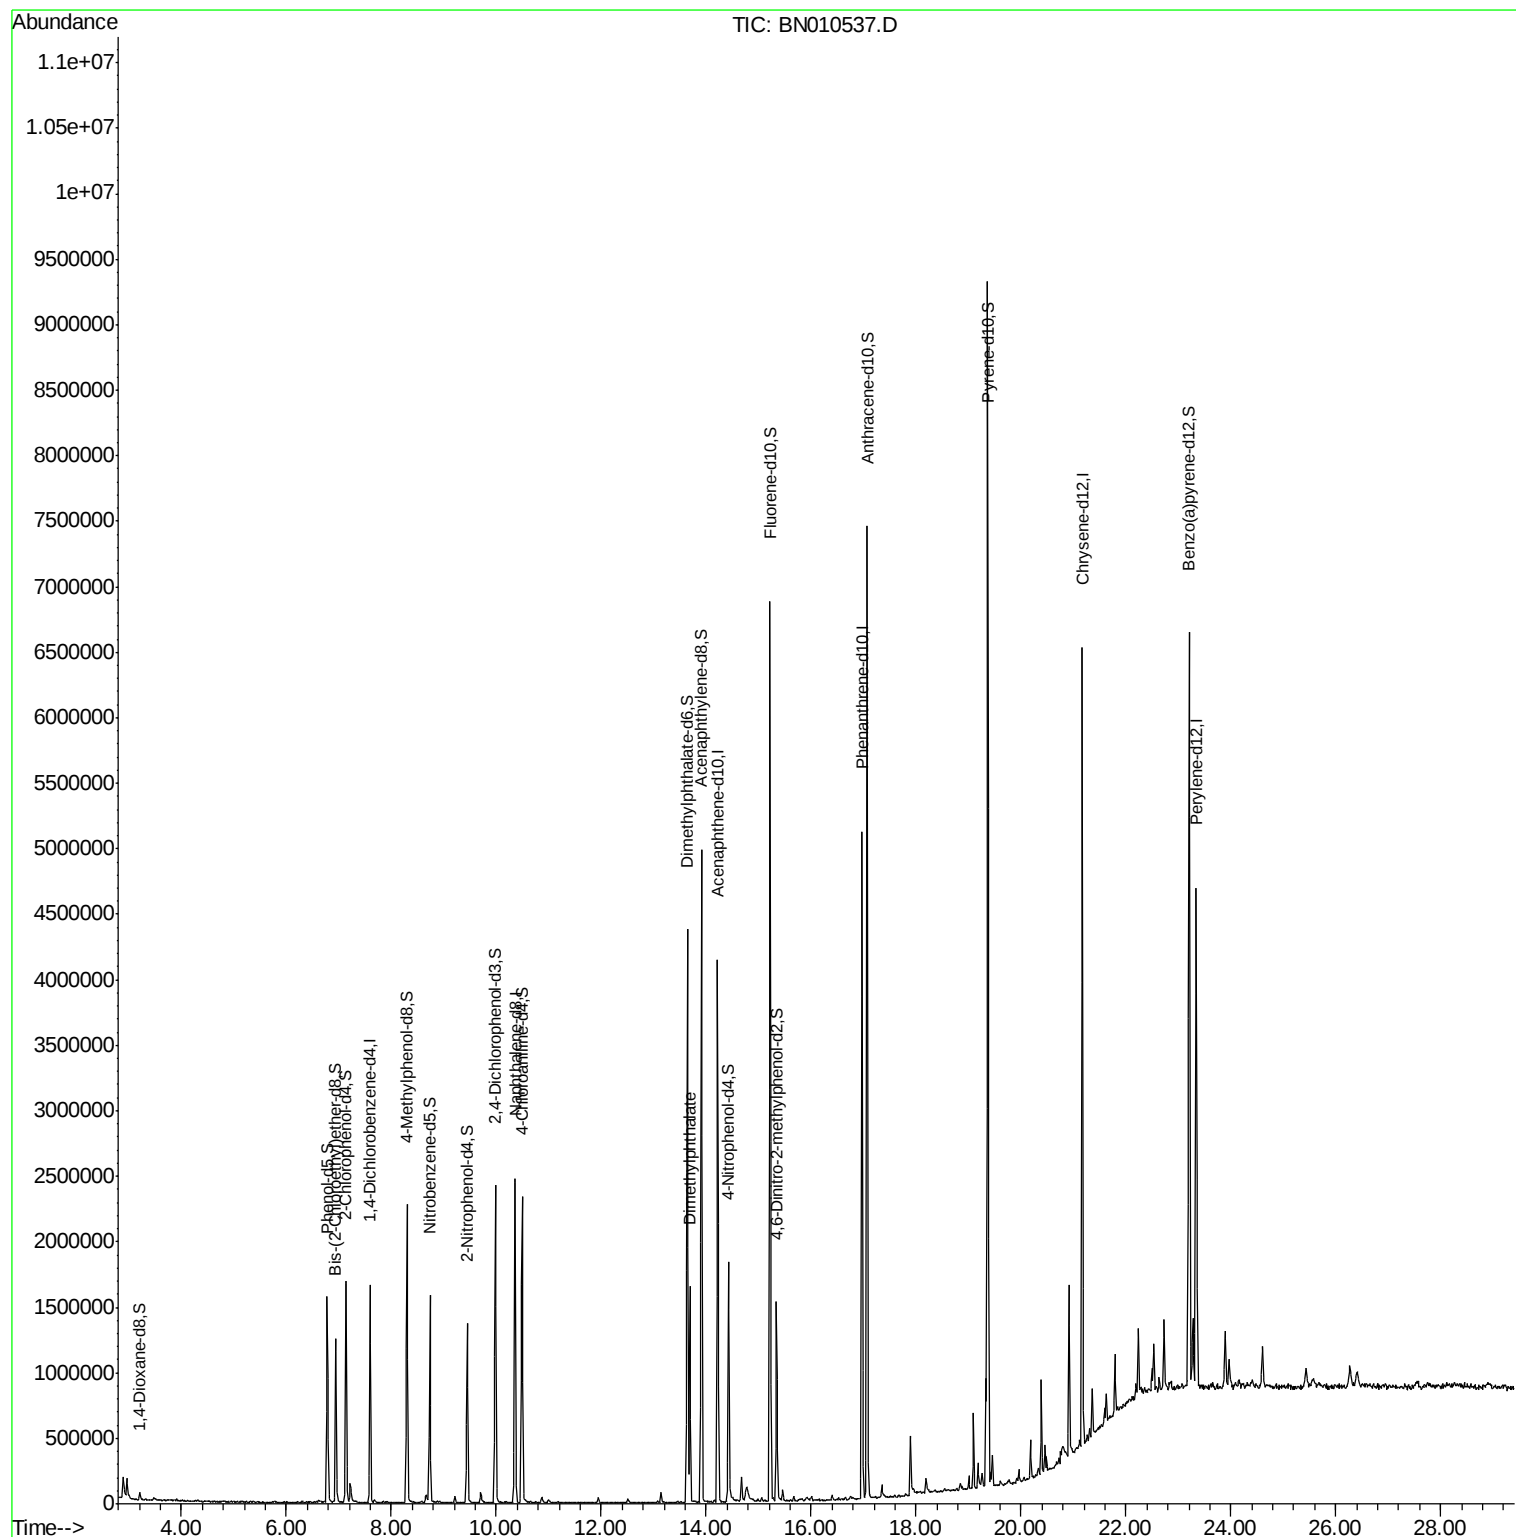

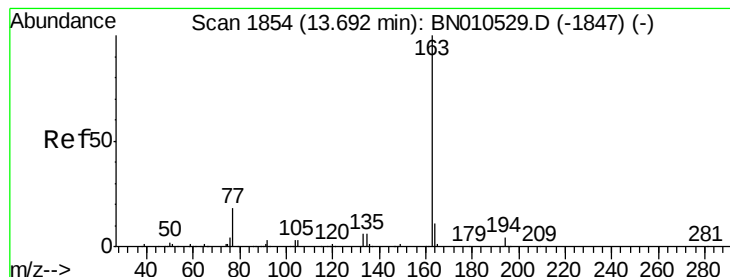

#45

Dimethylphthalate

Concen: 9.869 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010537.D

Acq: 17 Apr 2020 03:40

Instrument :

BNA_N

ClientSampleId :

BG2H8


Tot Ion:163 Resp: 1028557

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 10.9 8.0 12.0

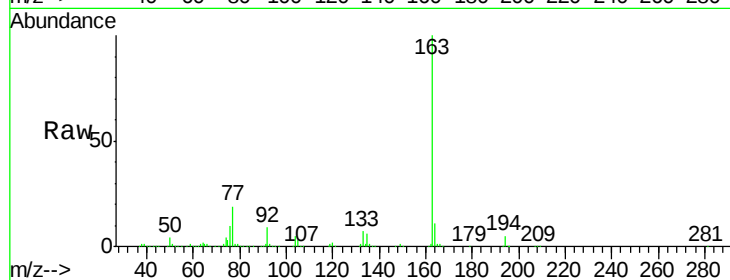

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

