

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
 Data File : BN010540.D
 Acq On : 17 Apr 2020 05:28
 Operator : CG/JU
 Sample : L2176-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG2J2

Quant Time: Apr 17 07:03:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	504455	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2218112	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1477476	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3350206	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	3358224	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	3002947	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	28841	2.99	ng/uL	0.00
5) Phenol-d5	6.78	99	779943	19.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	414332	20.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	672664	19.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	696548	20.74	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	346312	20.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	390088	20.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	745069	19.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	765647	17.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	2411217	22.00	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	2854470	21.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	396714	18.59	ng/ul	0.00
58) Fluorene-d10	15.22	176	2132425	21.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	302136	17.26	ng/ul	0.00
71) Anthracene-d10	17.07	188	3489536	22.49	ng/ul	0.00
79) Pyrene-d10	19.37	212	4083243	21.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	3529129	22.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.69	163	860756	7.563	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010540.D
Acq On : 17 Apr 2020 05:28
Operator : CG/JU
Sample : L2176-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG2J2

Quant Time: Apr 17 07:03:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

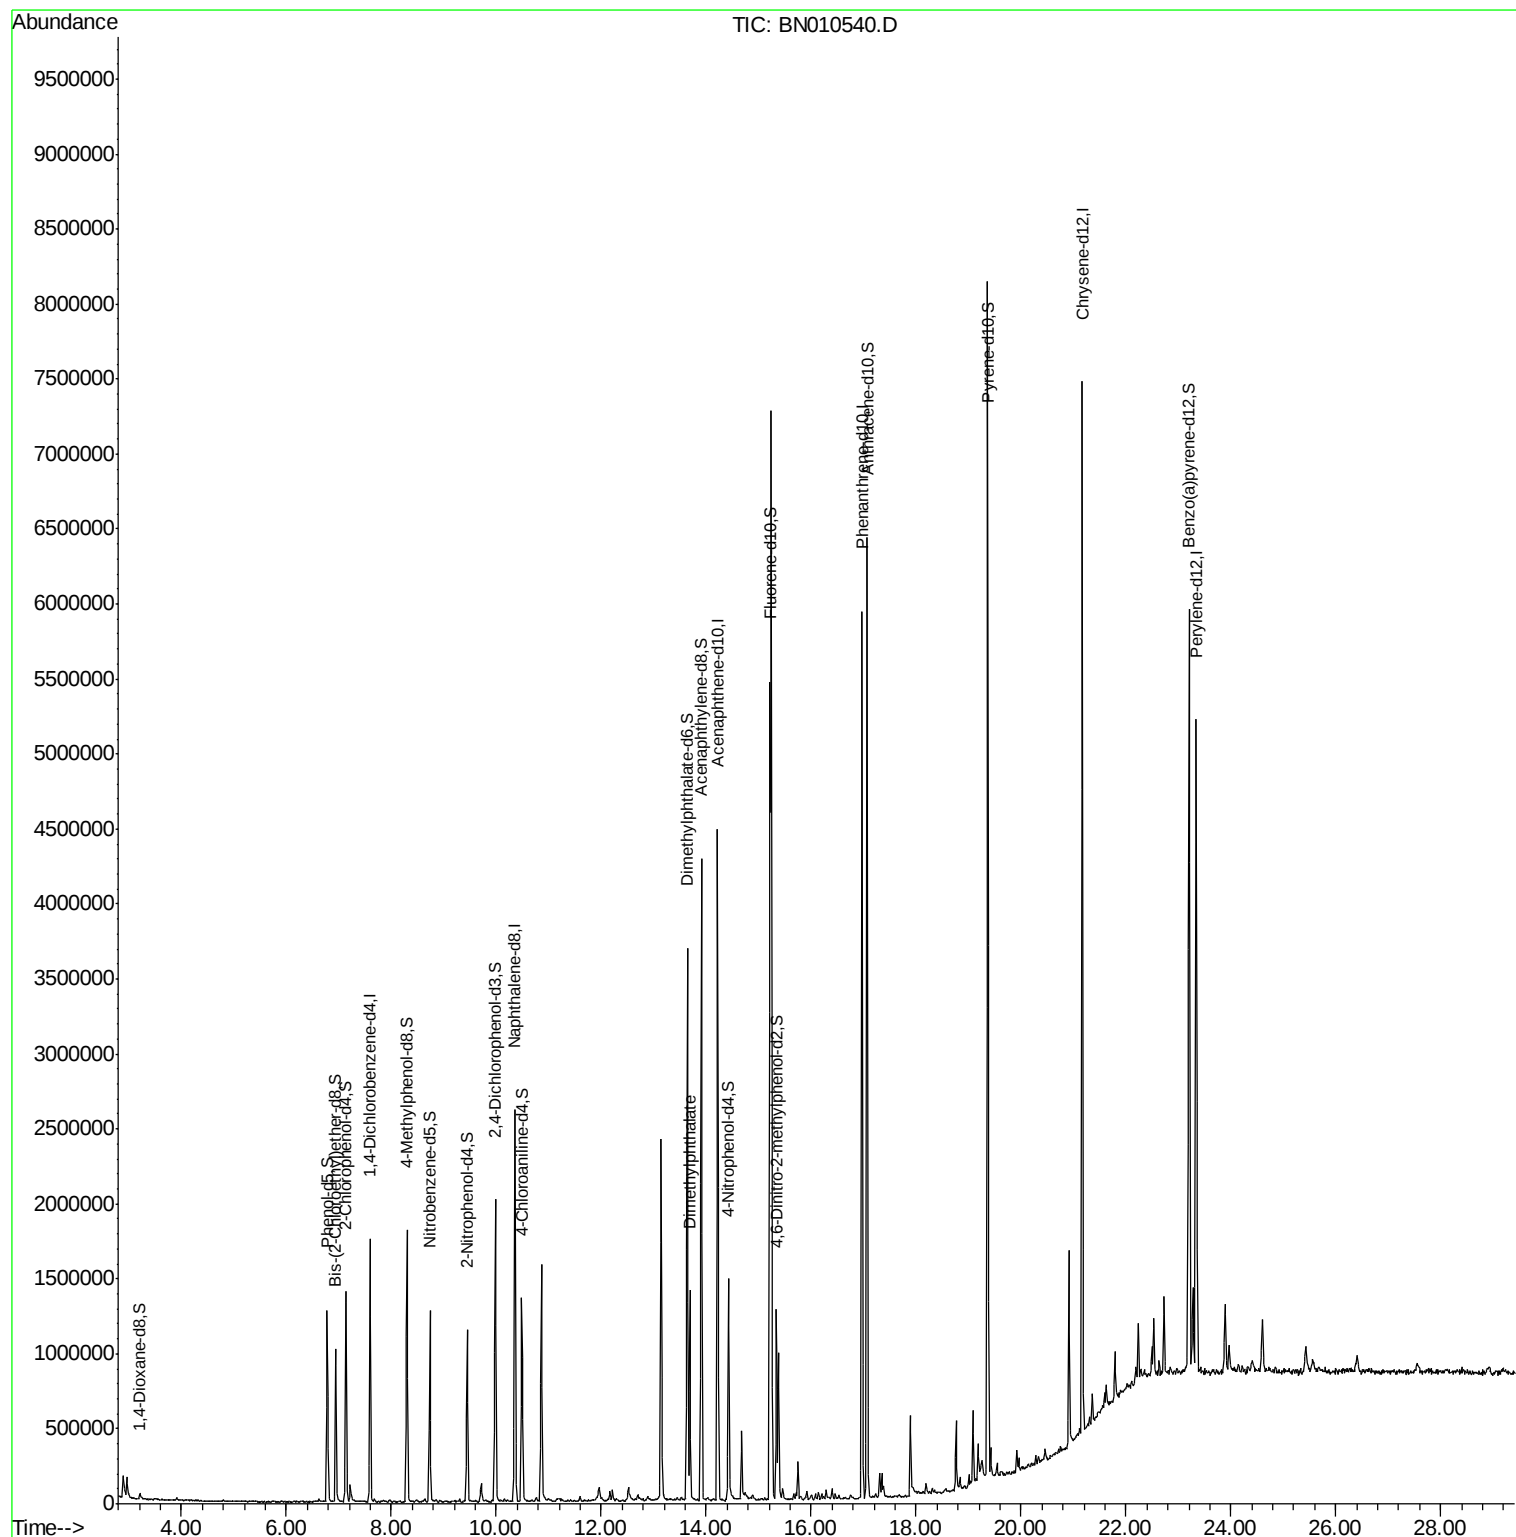

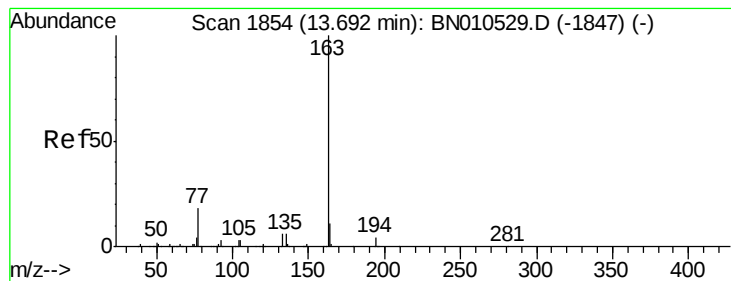

#45

Dimethylphthalate

Concen: 7.563 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010540.D

Acq: 17 Apr 2020 05:28

Instrument :

BNA_N

ClientSampleId :

BG2J2


Tot Ion:163 Resp: 860756

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 10.1 8.0 12.0

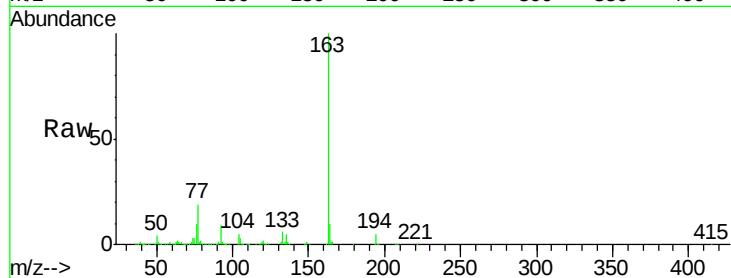

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

