

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
 Data File : BN010542.D
 Acq On : 17 Apr 2020 06:40
 Operator : CG/JU
 Sample : L2176-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG2J5

Quant Time: Apr 17 08:00:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	524772	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2311346	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1523928	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3352646	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	3496023	20.00	ng/ul	-0.01
86) Perylene-d12	23.34	264	3001839	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	29424	2.93	ng/uL	0.00
5) Phenol-d5	6.78	99	679256	16.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	339968	16.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	556561	15.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	597816	17.11	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	272844	15.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	304970	15.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	627156	16.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	396770	8.89	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	1946579	17.22	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	2276741	16.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	313487	14.24	ng/ul	0.00
58) Fluorene-d10	15.22	176	1720138	16.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.34	200	182330	10.41	ng/ul	-0.01
71) Anthracene-d10	17.07	188	2672237	17.21	ng/ul	0.00
79) Pyrene-d10	19.37	212	3201377	16.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	2723391	17.49	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.69	163	809792	6.898	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010542.D
Acq On : 17 Apr 2020 06:40
Operator : CG/JU
Sample : L2176-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG2J5

Quant Time: Apr 17 08:00:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

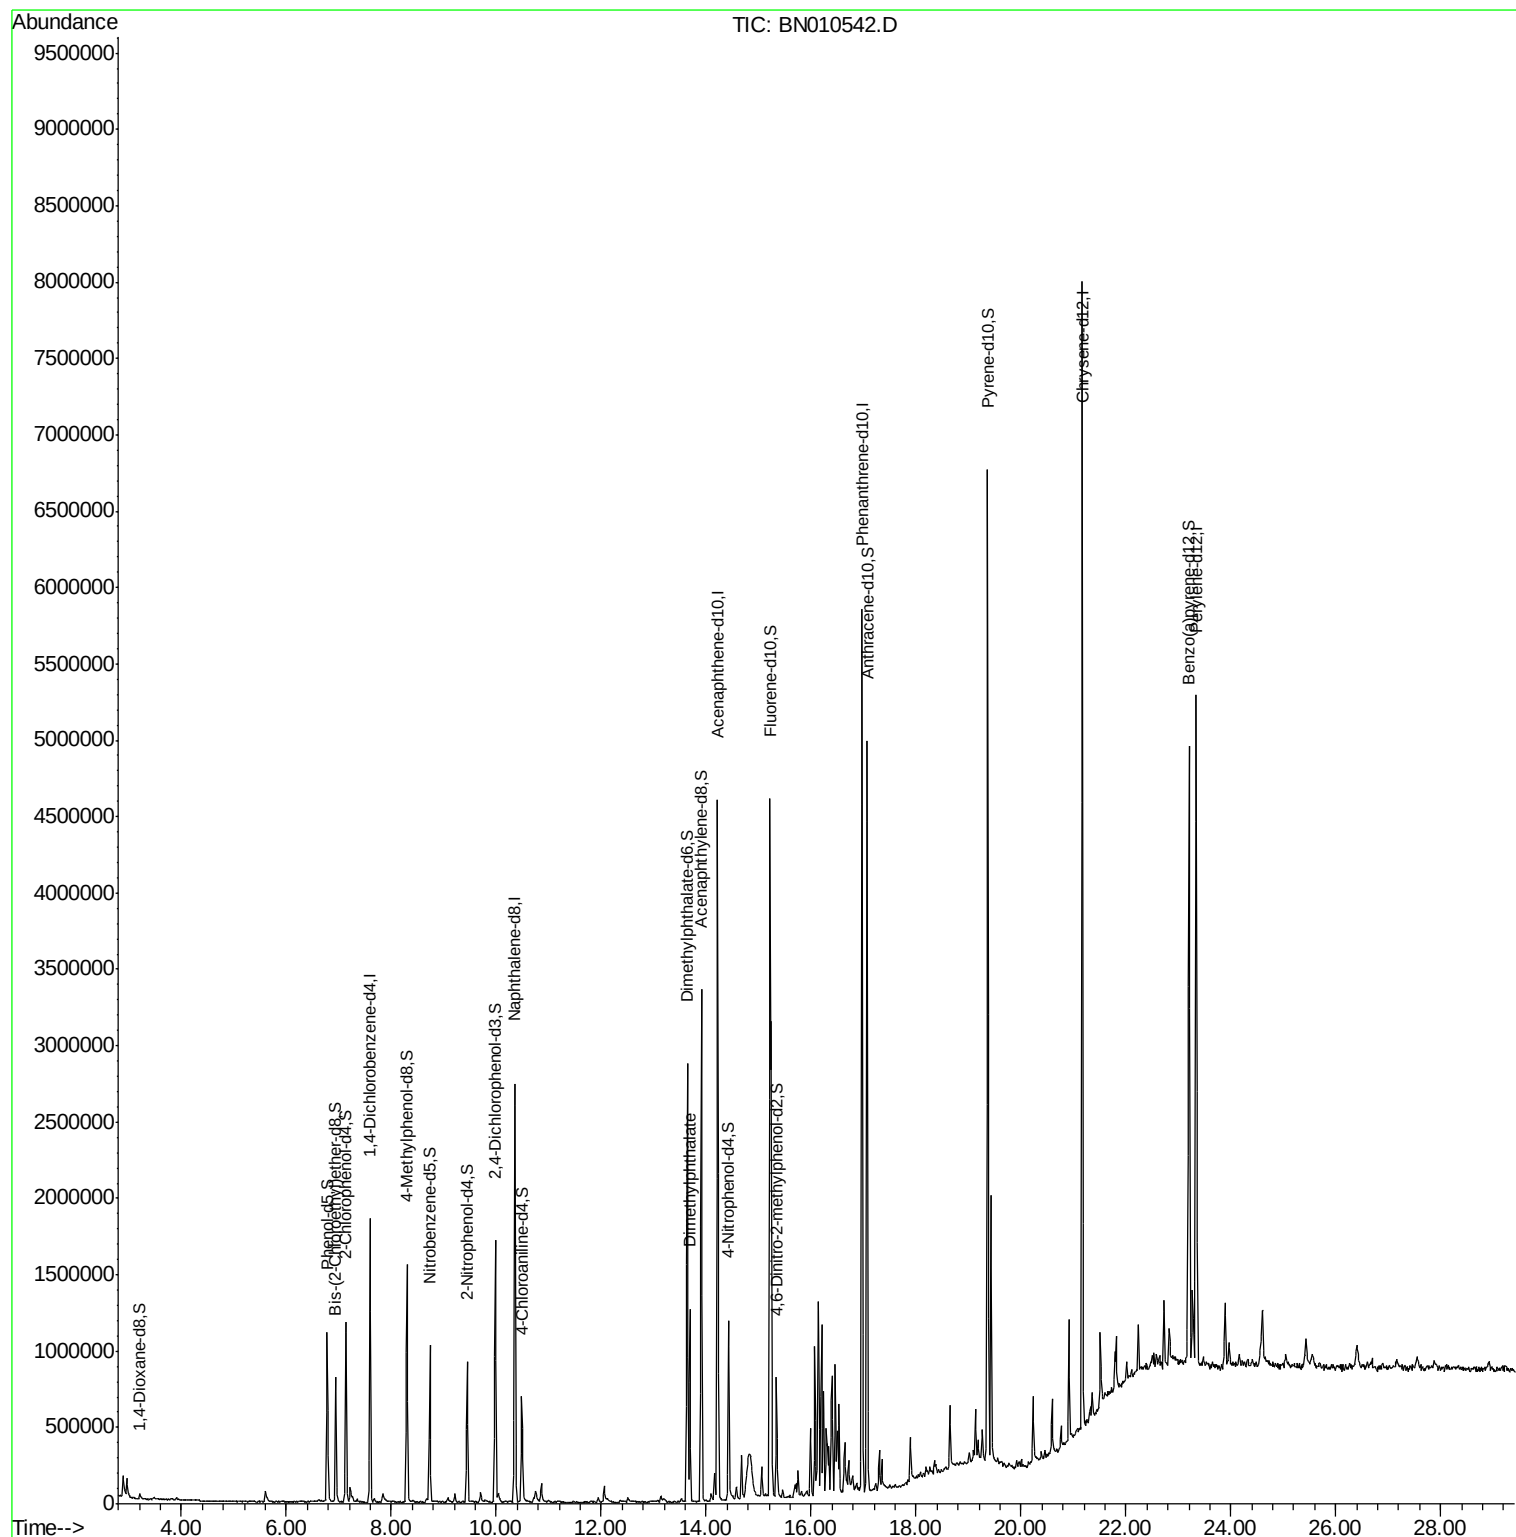

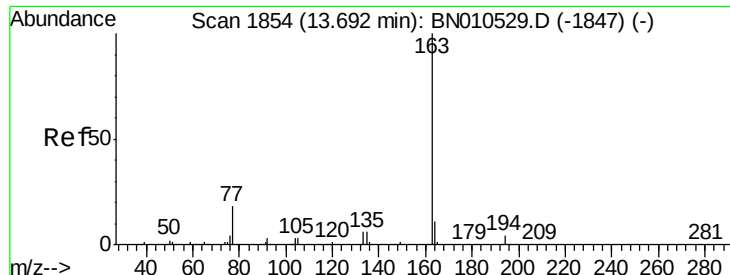

#45

Dimethylphthalate

Concen: 6.898 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010542.D

Acq: 17 Apr 2020 06:40

Instrument :

BNA_N

ClientSampleId :

BG2J5



Tot Ion:163 Resp: 809792

Ion Ratio Lower Upper

163 100

194 4.4 3.3 4.9

164 9.4 8.0 12.0

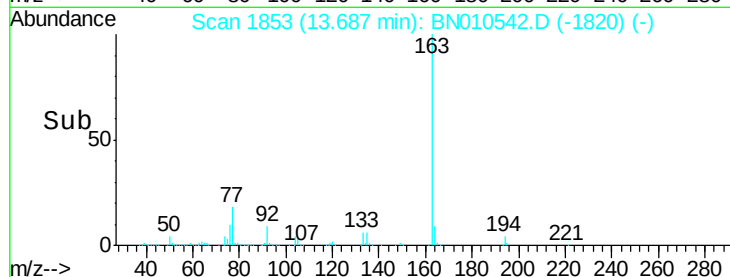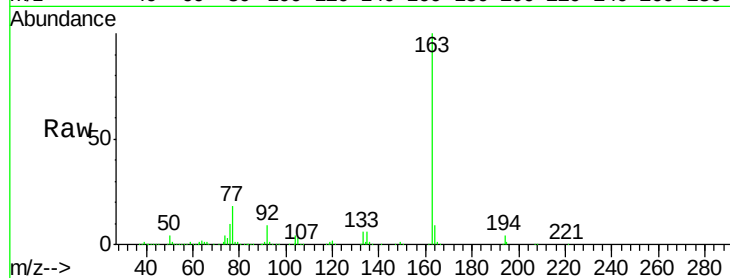

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

