

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
 Data File : BN010543.D
 Acq On : 17 Apr 2020 07:15
 Operator : CG/JU
 Sample : L2207-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFS84

Quant Time: Apr 17 08:00:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	576760	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2504912	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1606882	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3647405	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	3522847	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	3046747	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	19434	1.76	ng/uL	0.00
5) Phenol-d5	6.78	99	352914	7.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	835310	36.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	1095839	28.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	686944	17.89	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	689485	35.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	776123	36.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1349190	32.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	31956	0.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	4401089	36.92	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	5244244	35.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	150047	6.46	ng/ul	0.00
58) Fluorene-d10	15.22	176	3833804	35.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.34	200	608393	31.93	ng/ul	-0.01
71) Anthracene-d10	17.07	188	5897362	34.91	ng/ul	0.00
79) Pyrene-d10	19.37	212	6933197	34.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5750748	36.39	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.69	163	536023	4.330	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010543.D
Acq On : 17 Apr 2020 07:15
Operator : CG/JU
Sample : L2207-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFS84

Quant Time: Apr 17 08:00:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

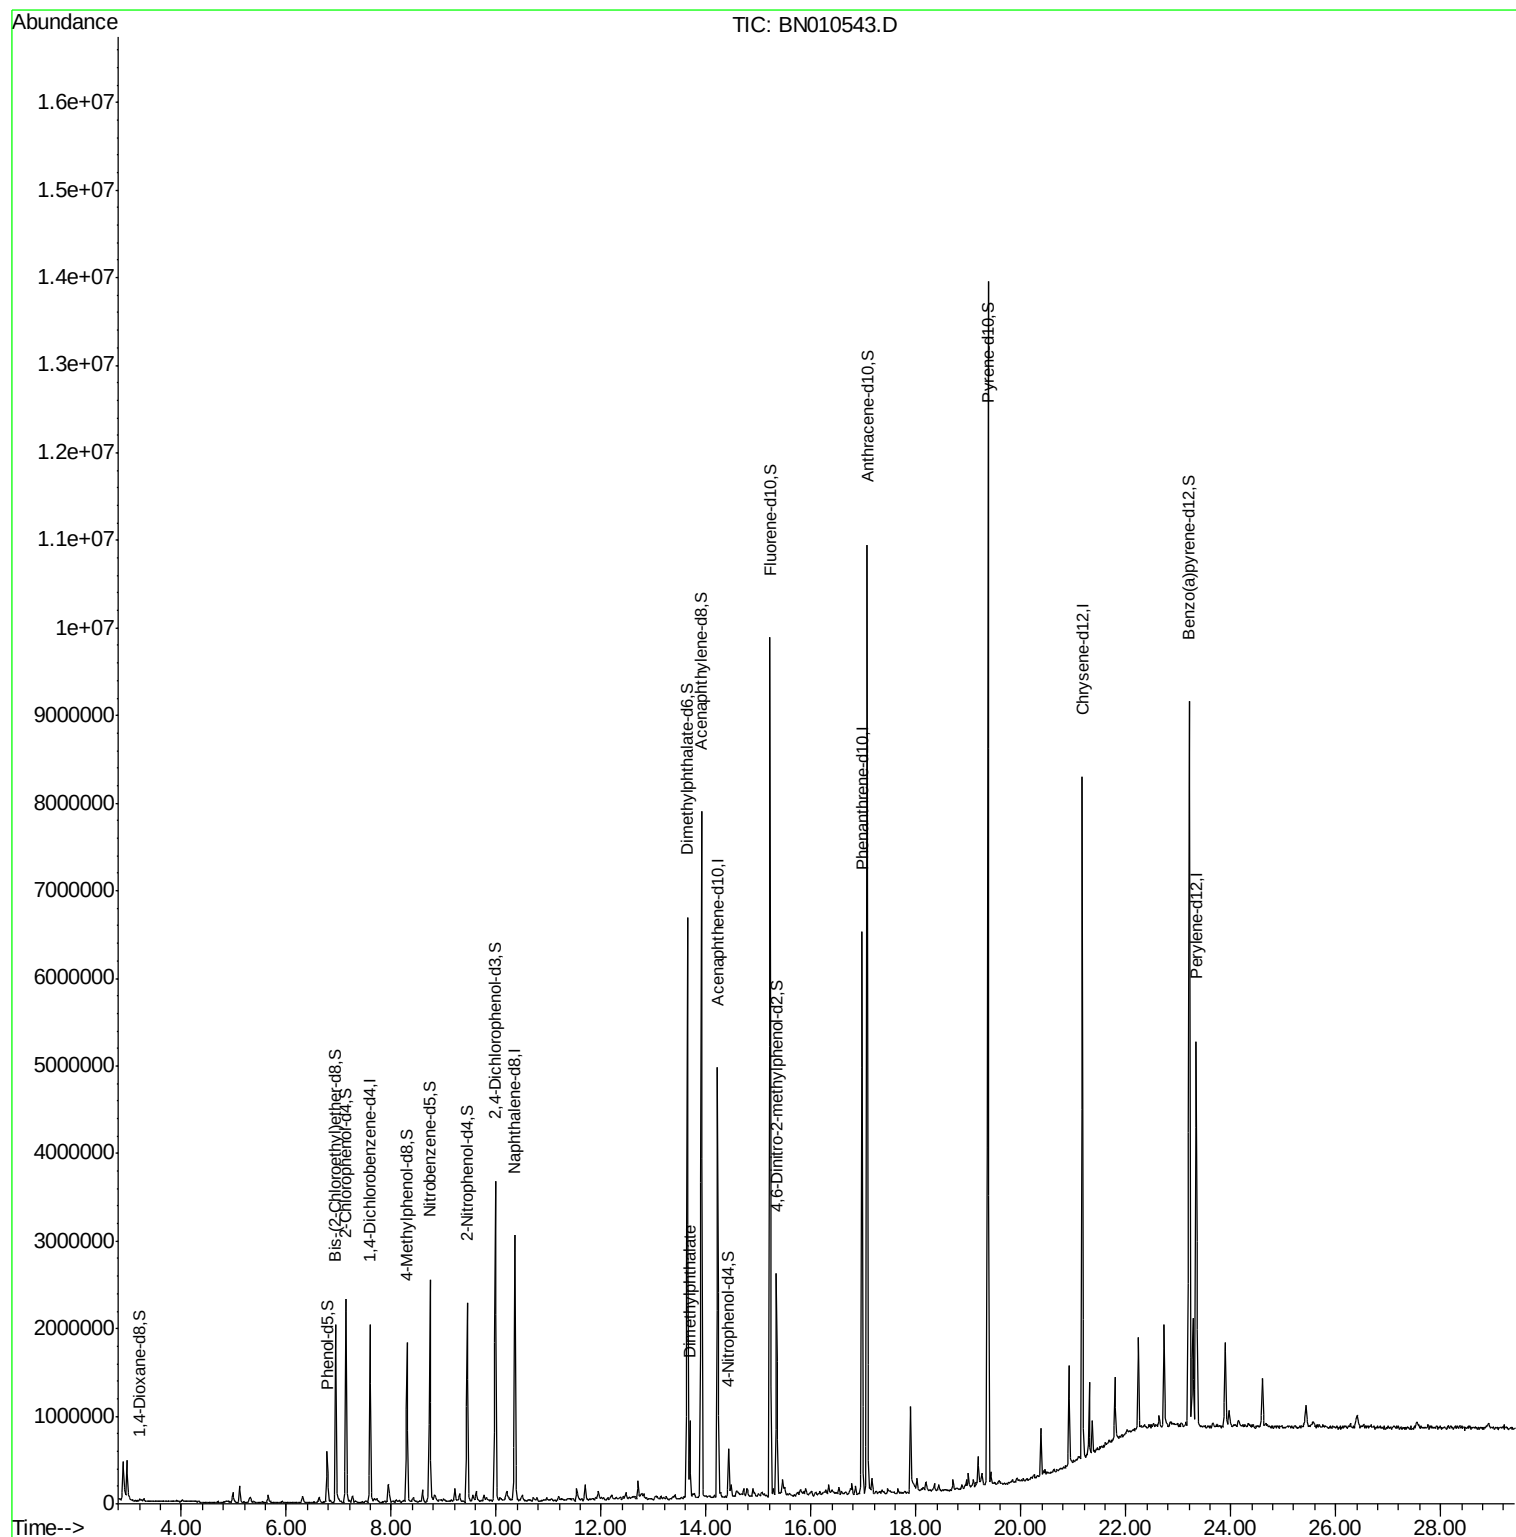

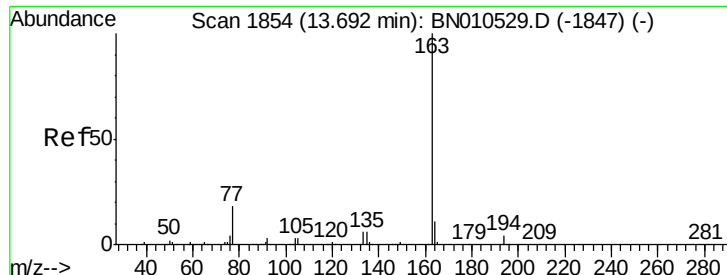

#45

Dimethylphthalate

Concen: 4.330 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010543.D

Acq: 17 Apr 2020 07:15

Instrument :

BNA_N

ClientSampleId :

BFS84

Tot Ion:163 Resp: 536023

Ion Ratio Lower Upper

163 100

194 4.7 3.3 4.9

164 10.6 8.0 12.0

