

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041620\
 Data File : BN010550.D
 Acq On : 17 Apr 2020 14:34
 Operator : CG/JU
 Sample : L2317-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0F12

Quant Time: Apr 17 15:12:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 10:21:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	442557	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1990072	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	1298628	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	2970175	20.00	ng/ul	0.00
78) Chrysene-d12	21.17	240	3176831	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2806705	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.21	96	7675	0.91	ng/uL	0.00
5) Phenol-d5	6.78	99	273941	7.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	616776	34.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	824412	27.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	502493	17.06	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	524321	34.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	583449	34.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1028791	30.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	70540	1.84	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	3404427	35.33	ng/ul	0.00
47) Acenaphthylene-d8	13.91	160	4197976	35.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	107542	5.73	ng/ul	0.00
58) Fluorene-d10	15.22	176	3150153	36.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.34	200	416784	26.86	ng/ul	-0.01
71) Anthracene-d10	17.07	188	4966306	36.10	ng/ul	0.00
79) Pyrene-d10	19.37	212	5818256	32.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5292257	36.35	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.69	163	446854	4.467	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041620\
Data File : BN010550.D
Acq On : 17 Apr 2020 14:34
Operator : CG/JU
Sample : L2317-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0F12

Quant Time: Apr 17 15:12:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 10:21:51 2020
Response via : Initial Calibration

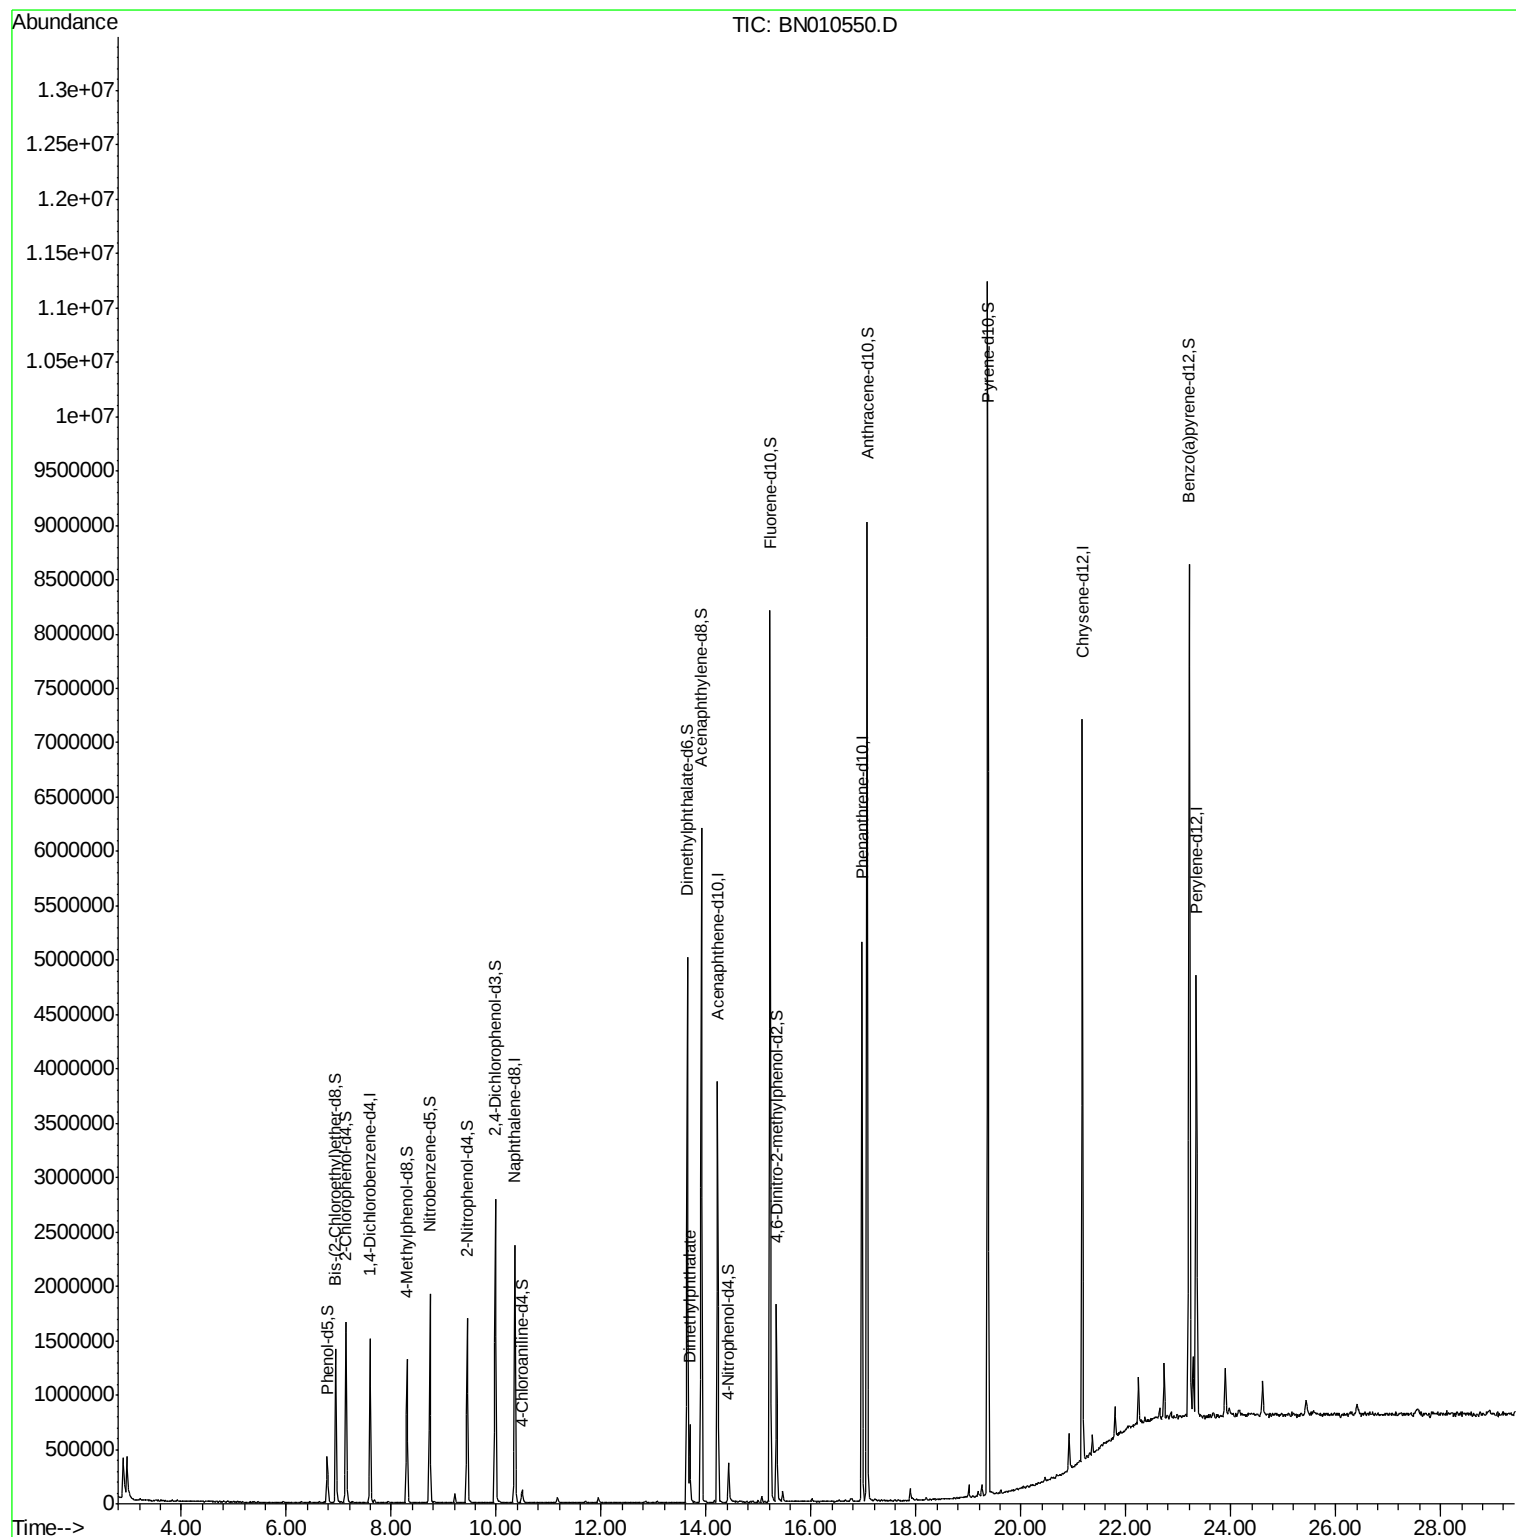

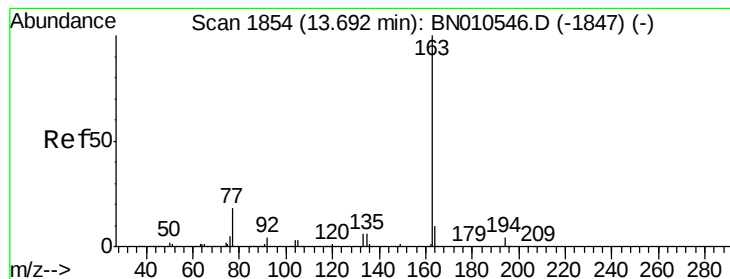

#45

Dimethylphthalate

Concen: 4.467 ng/ul

RT: 13.69 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BN010550.D

Acq: 17 Apr 2020 14:34

Instrument :

BNA_N

ClientSampleId :

C0F12


Tot Ion:163 Resp: 446854

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 10.1 8.0 12.0

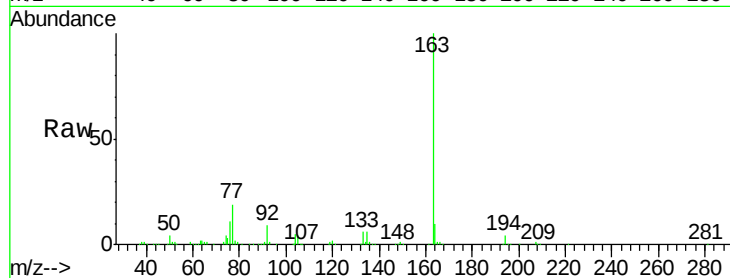

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

