
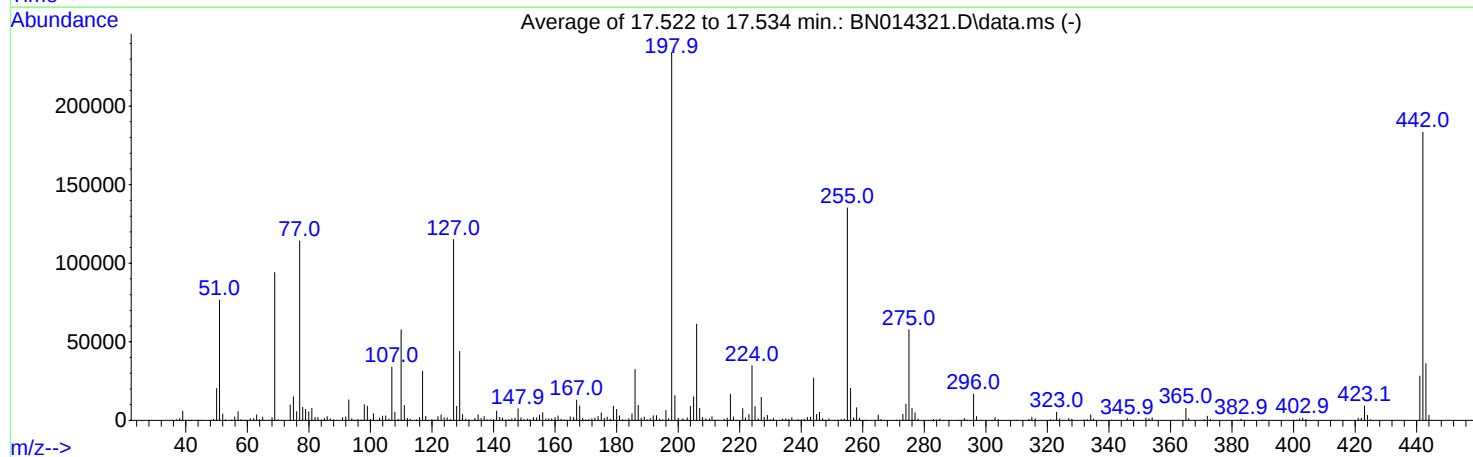


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041921\
 Data File : BN014321.D
 Acq On : 19 Apr 2021 08:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 19 10:42:58 2021

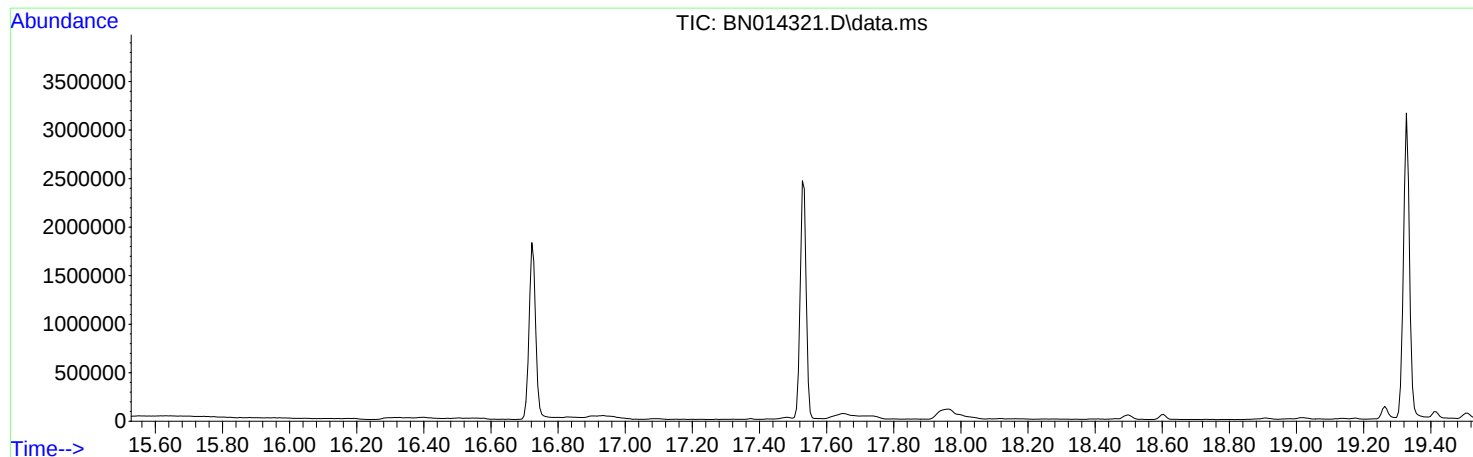




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	76568	PASS
68	69	0.00	2	1.9	1747	PASS
69	198	0.00	100	40.2	94102	PASS
70	69	0.00	2	0.6	542	PASS
127	198	10	80	49.2	115109	PASS
197	198	0.00	2	0.5	1128	PASS
198	198	100	100	100.0	234155	PASS
199	198	5	9	6.7	15746	PASS
275	198	10	60	24.6	57709	PASS
365	198	1	100	3.3	7680	PASS
441	198	0.01	100	12.1	28239	PASS
442	442	50	100	100.0	183451	PASS
443	442	15	24	19.7	36104	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041921\
Data File : BN014321.D
Acq On : 19 Apr 2021 08:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 19 10:51:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

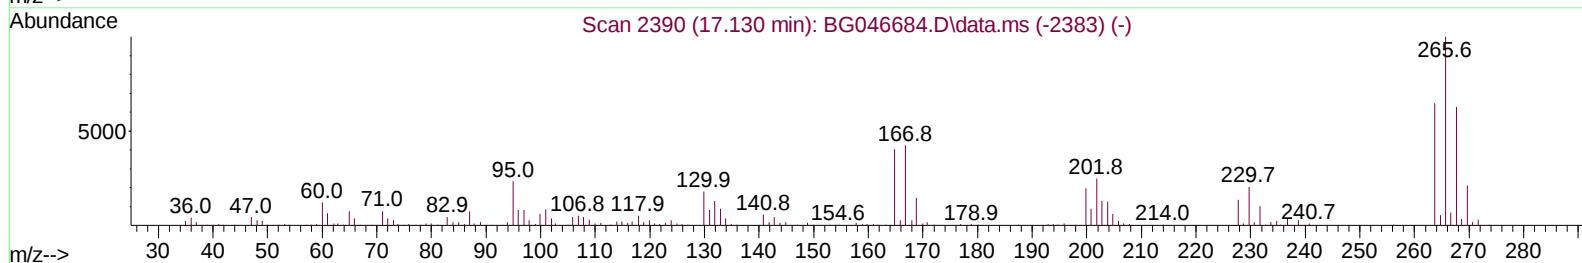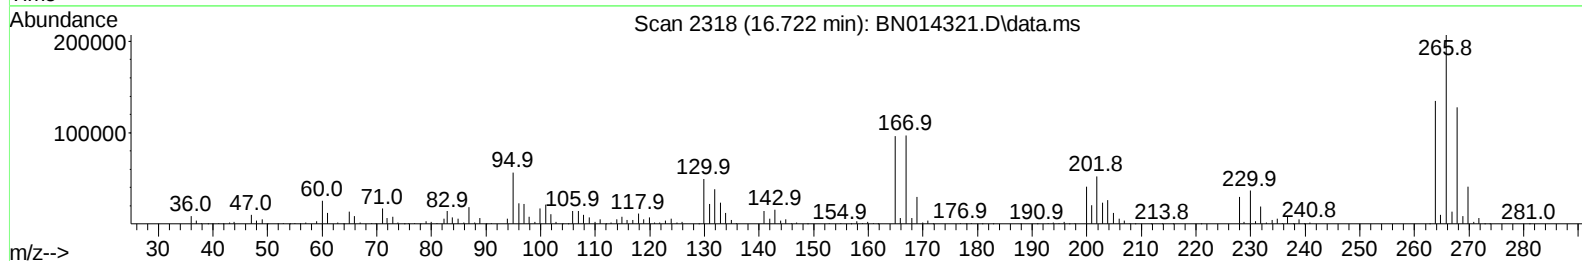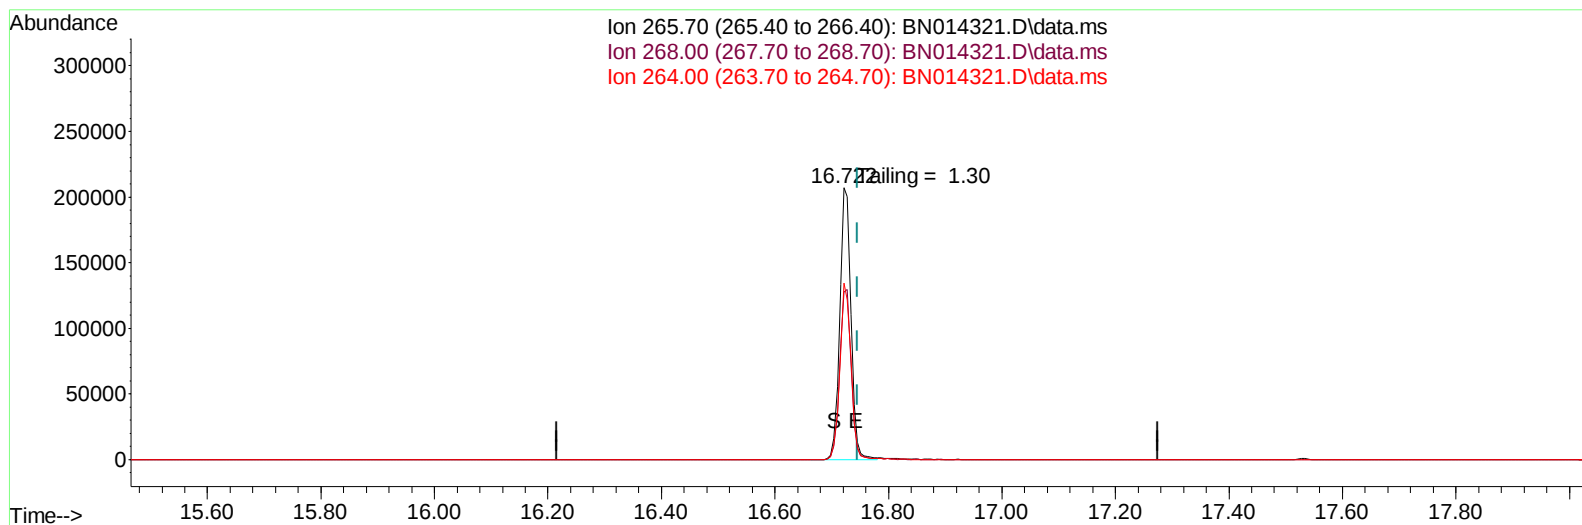

TIC: BN014321.D\data.ms

(70) Pentachloropheno1 (C)

16.722min (-0.023) 20455.69 ng




response 283498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.69
264.00	61.60	64.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041921\
Data File : BN014321.D
Acq On : 19 Apr 2021 08:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 19 10:51:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

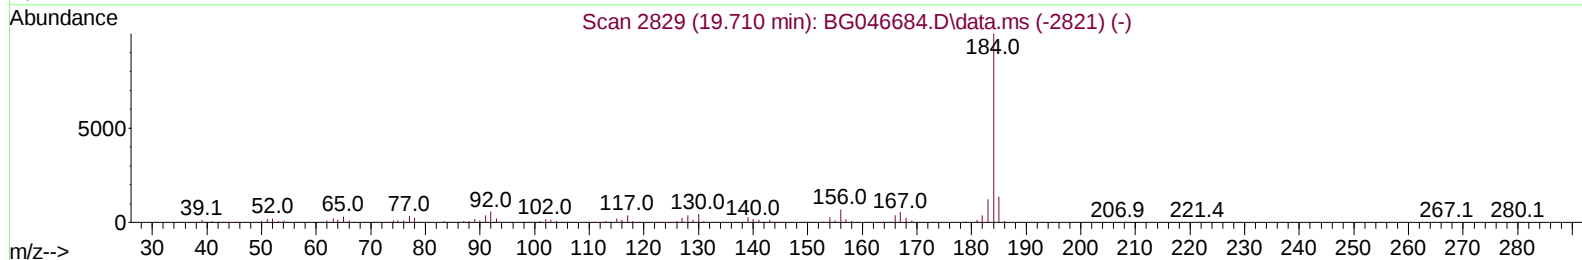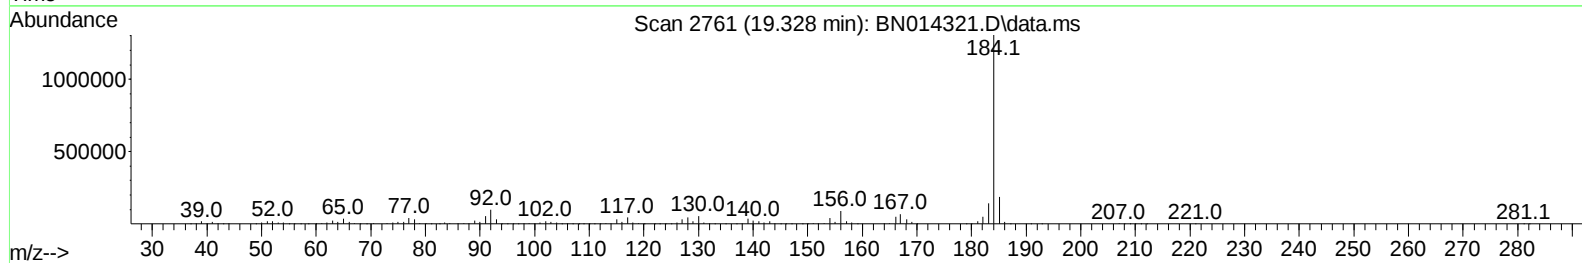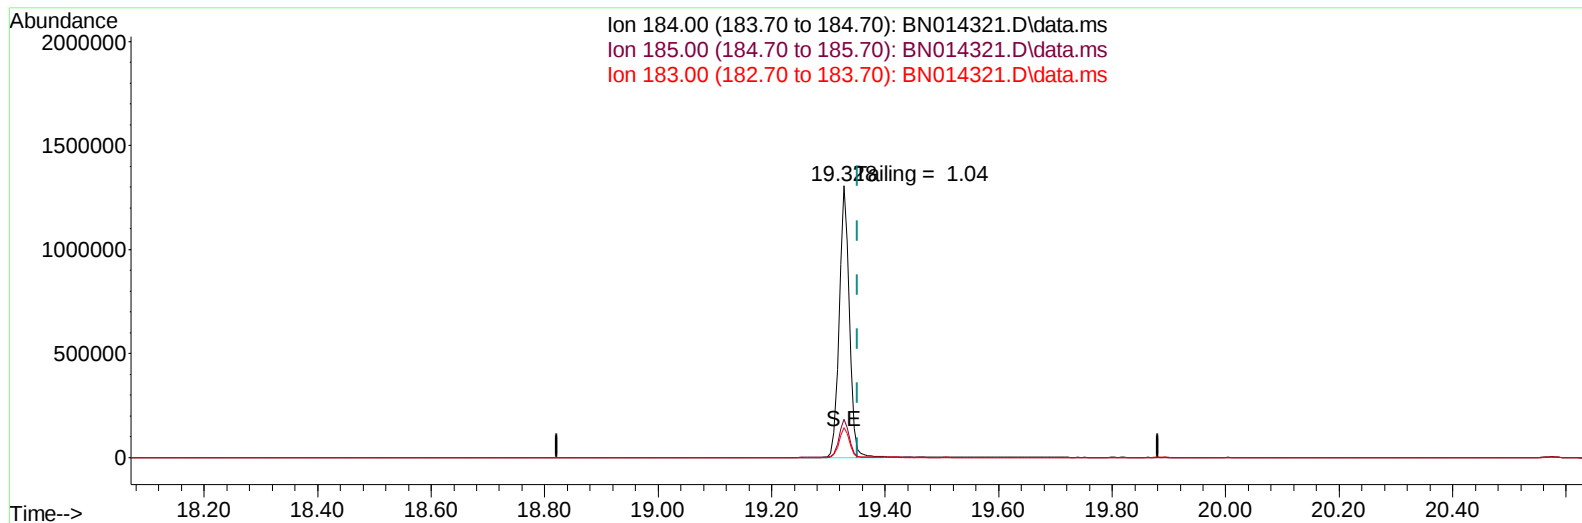

TIC: BN014321.D\data.ms

(77) Benzidine

19.328min (-0.023) 2372.97 ng

response 1601858

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.11
183.00	13.20	10.93
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_N	<u>BN014321.D</u>
Compound Name	Response	Retention Time
DDT	836728	20.575
DDD	5296	20.133
DDE	1139	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6435	843163	0.76