
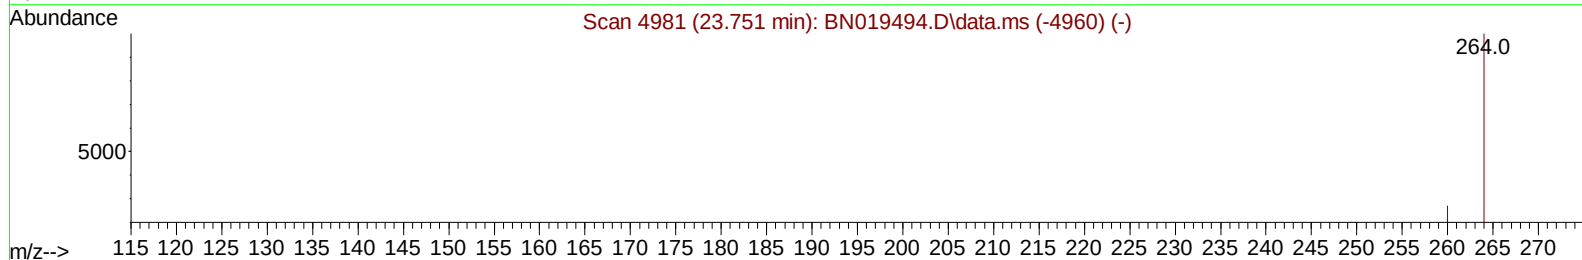
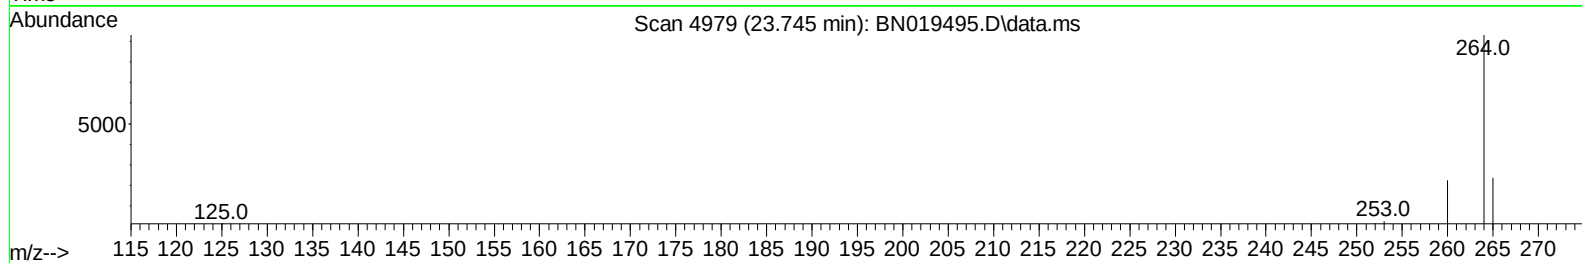


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
Data File : BN019495.D
Acq On : 19 Apr 2022 12:00
Operator : CG/JU
Sample : PB144173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 20 02:53:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

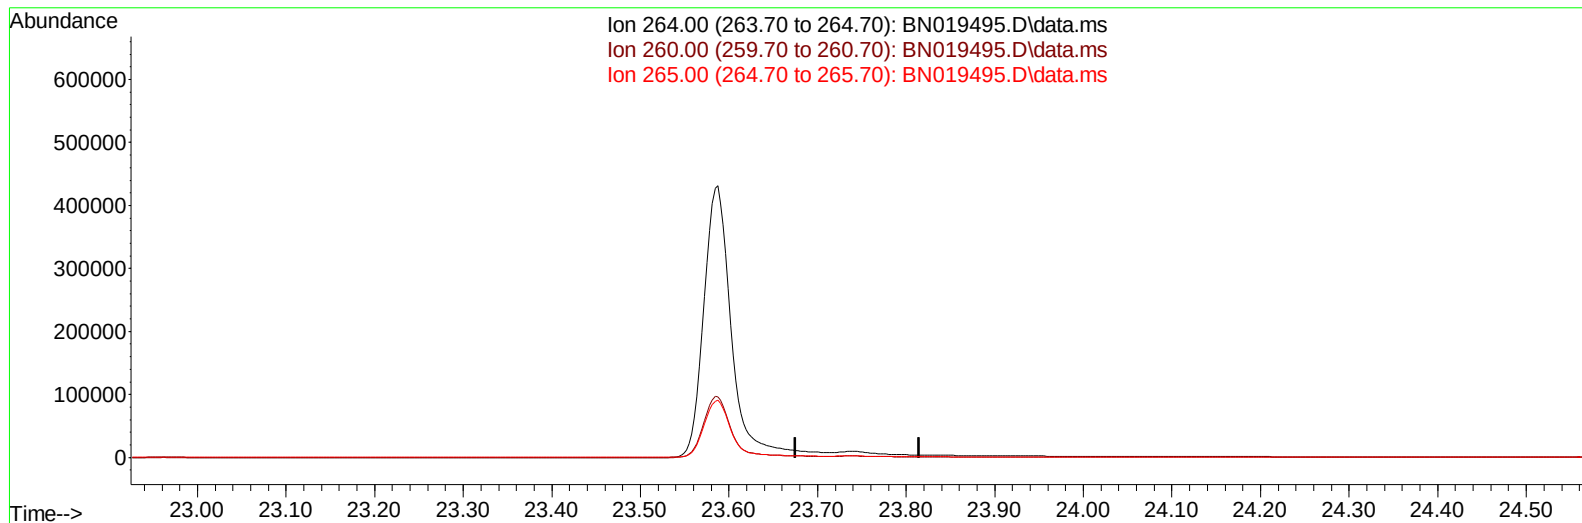

TIC: BN019495.D\data.ms

(23) Perylene-d12 (I)




23.745min (-23.745) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
Data File : BN019495.D
Acq On : 19 Apr 2022 12:00
Operator : CG/JU
Sample : PB144173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 20 02:53:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

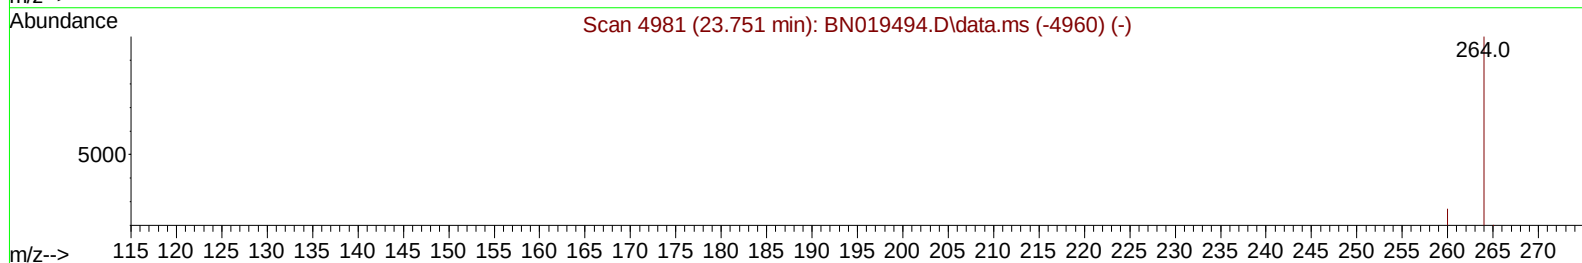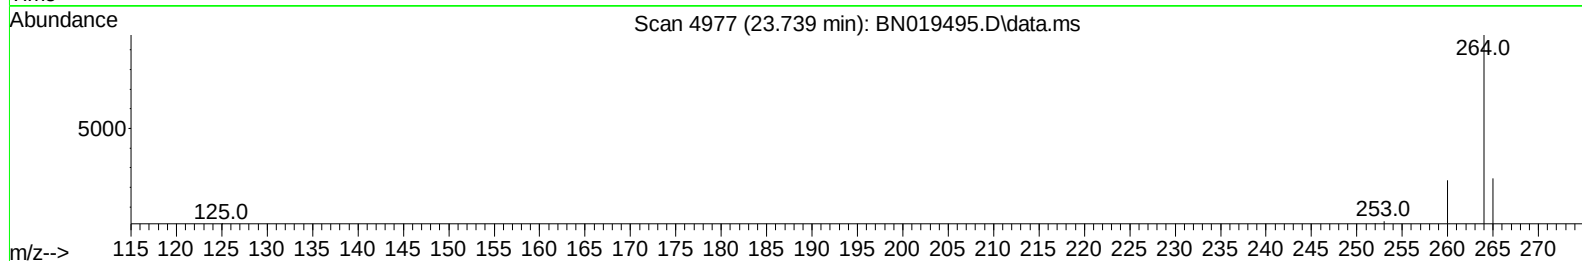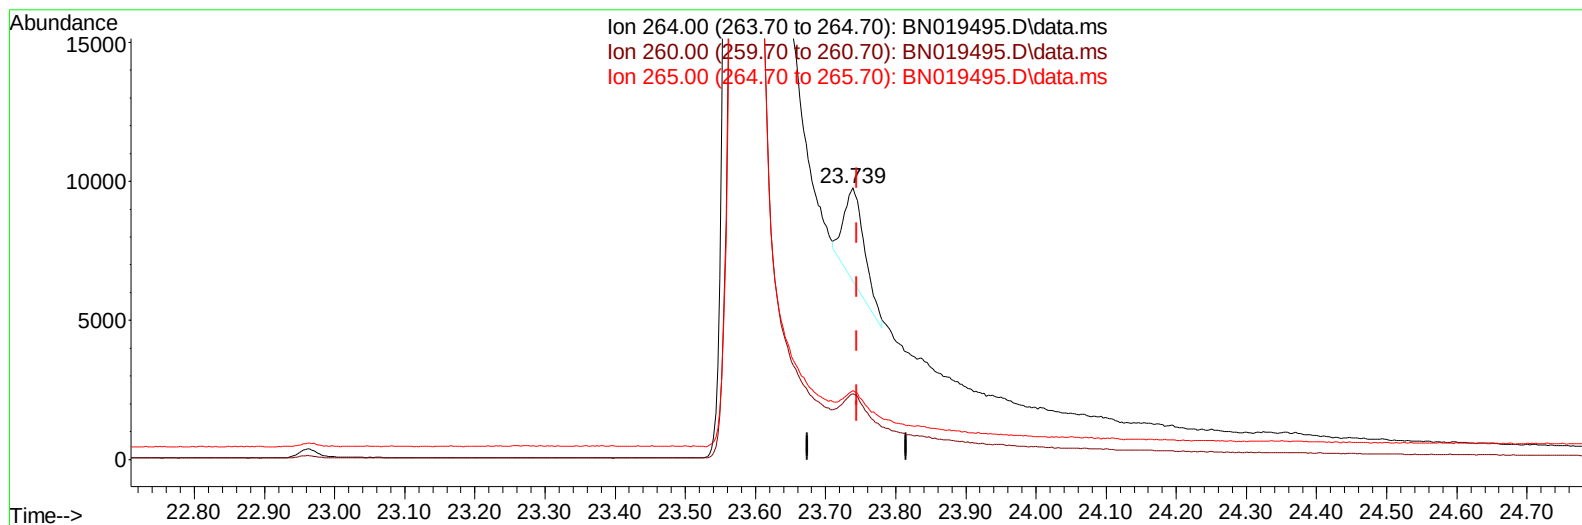

TIC: BN019495.D\data.ms

(23) Perylene-d12 (I)

23.739min (-0.006) 0.40 ng/ul m

response 6651

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.18
265.00	45.70	25.31#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
 Data File : BN019495.D
 Acq On : 19 Apr 2022 12:00
 Operator : CG/JU
 Sample : PB144173BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 20 02:53:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.814	152	5327	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136	16407	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.455	164	10035	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.196	188	19417	0.400	ng/ul	0.00
17) Chrysene-d12	21.407	240	9803	0.400	ng/ul	0.01
23) Perylene-d12	23.739	264	6651m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.173	96	39518	6.121	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152	8439	0.383	ng/ul	0.00
18) Fluoranthene-d10	19.229	212	17958	0.449	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
Data File : BN019495.D
Acq On : 19 Apr 2022 12:00
Operator : CG/JU
Sample : PB144173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Apr 20 02:53:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

