
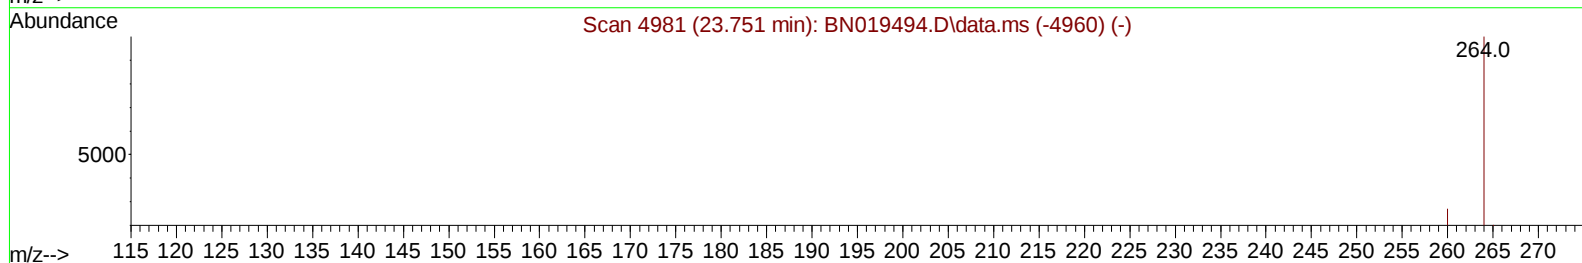
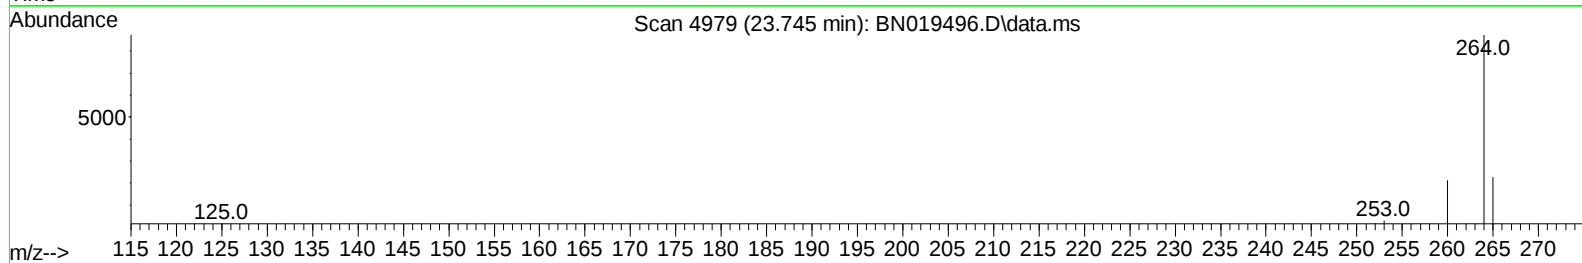


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
 Data File : BN019496.D
 Acq On : 19 Apr 2022 13:33
 Operator : CG/JU
 Sample : N2388-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 20 02:54:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

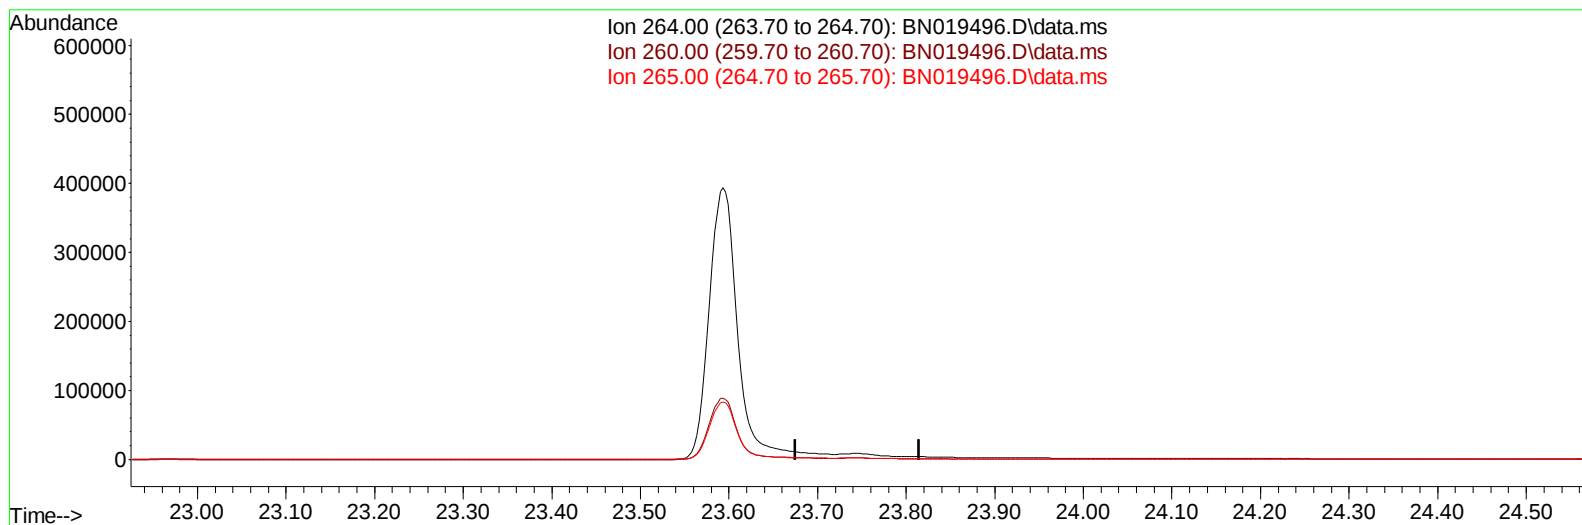

TIC: BN019496.D\data.ms

(23) Perylene-d12 (I)




23.745min (-23.745) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
Data File : BN019496.D
Acq On : 19 Apr 2022 13:33
Operator : CG/JU
Sample : N2388-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 20 02:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

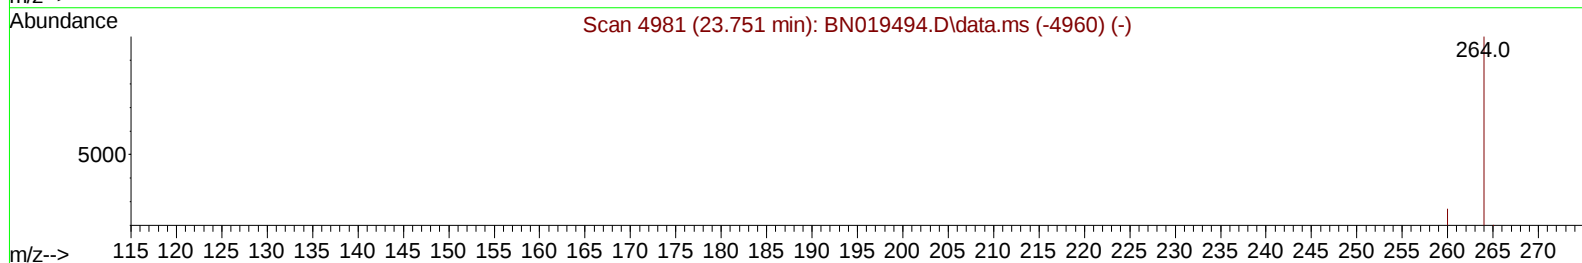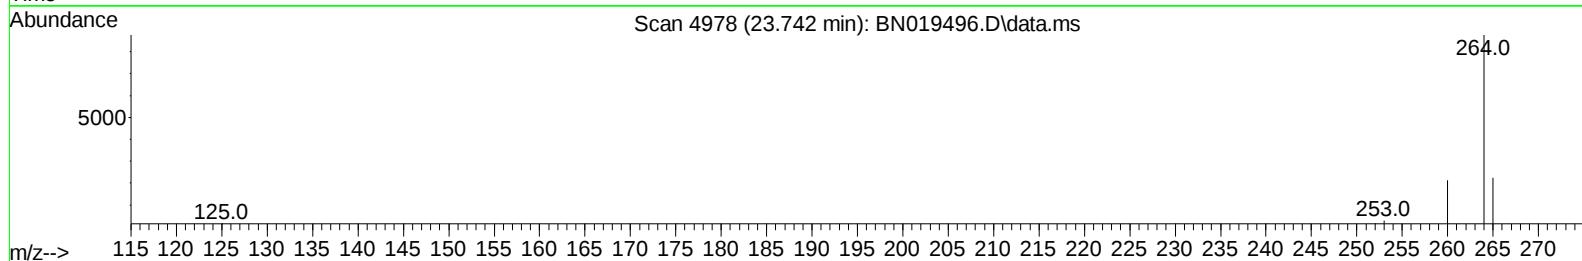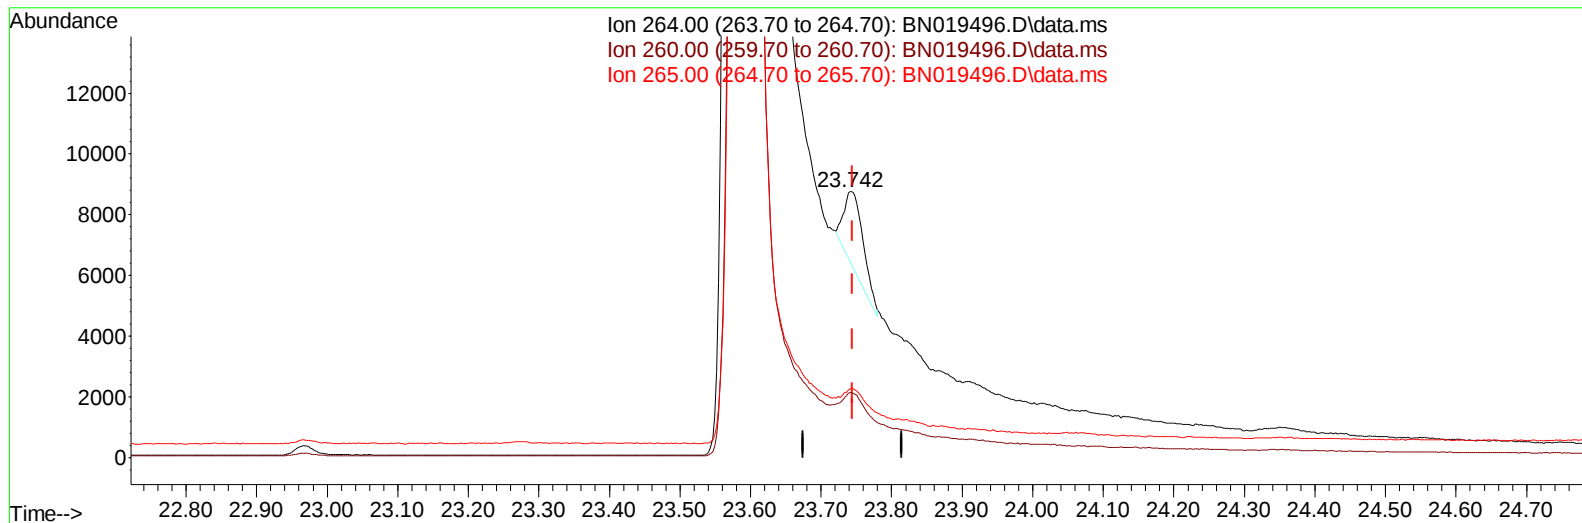

TIC: BN019496.D\data.ms

(23) Perylene-d12 (I)

23.742min (-0.003) 0.40 ng/ul m

response 4459

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.41
265.00	45.70	25.81#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
 Data File : BN019496.D
 Acq On : 19 Apr 2022 13:33
 Operator : CG/JU
 Sample : N2388-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 20 02:54:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	4807	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.613	136	14445	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	9061	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188	17396	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240	8762	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	4459m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	29640	5.087	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	8384	0.433	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	18577	0.520	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.662	128	1298	0.032	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
Data File : BN019496.D
Acq On : 19 Apr 2022 13:33
Operator : CG/JU
Sample : N2388-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 20 02:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

