

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
 Data File : BN019496.D
 Acq On : 19 Apr 2022 13:33
 Operator : CG/JU
 Sample : N2388-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE5

Quant Time: Apr 20 02:54:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	4807	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.613	136	14445	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	9061	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188	17396	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240	8762	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	4459m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	29640	5.087	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	8384	0.433	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	18577	0.520	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.662	128	1298	0.032	ng/ul#	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041922\
Data File : BN019496.D
Acq On : 19 Apr 2022 13:33
Operator : CG/JU
Sample : N2388-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFE5


Quant Time: Apr 20 02:54:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

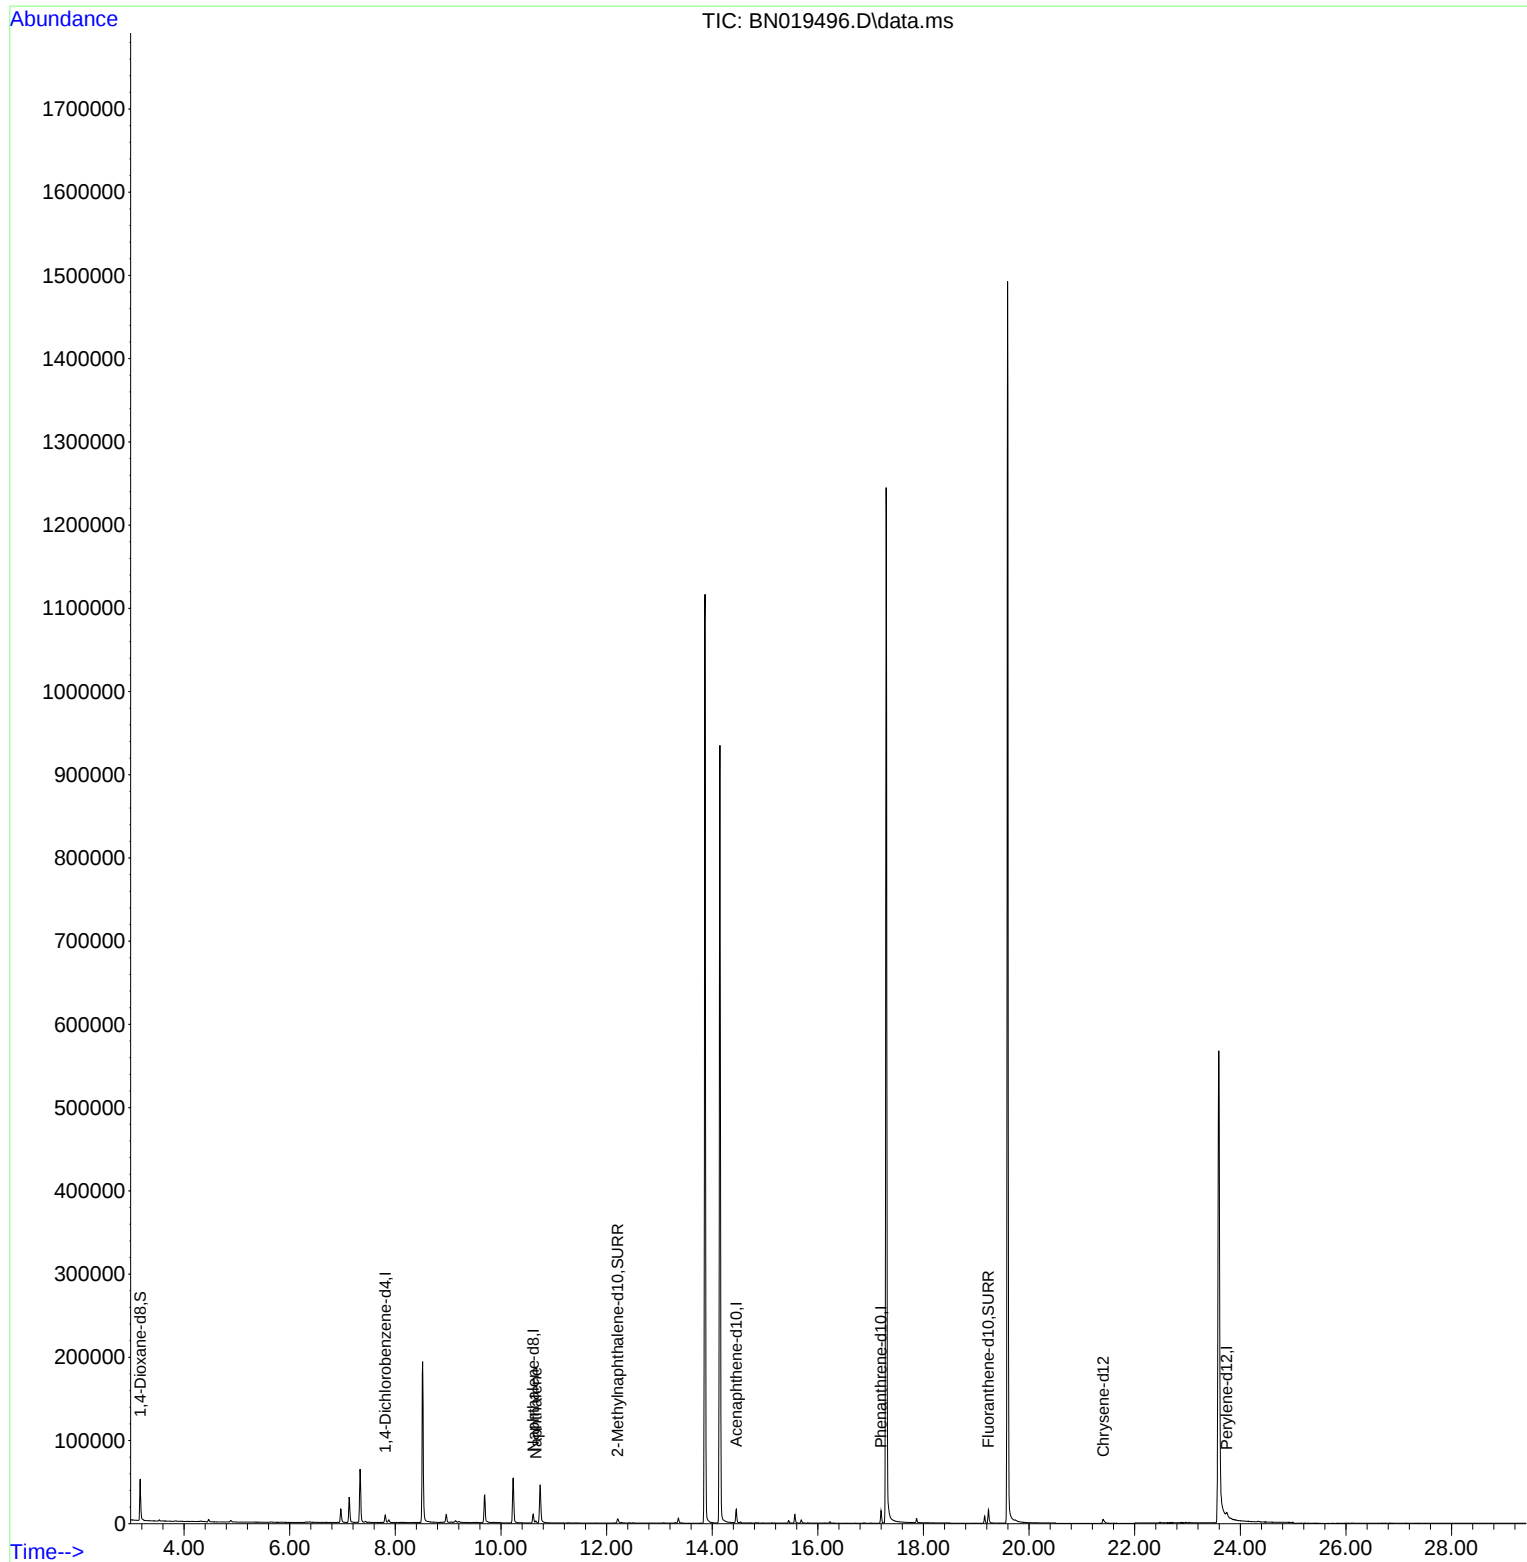

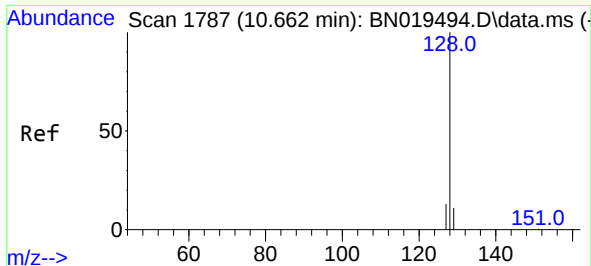

#5
Naphthalene
Concen: 0.032 ng/ul
RT: 10.662 min Scan# 11
Delta R.T. -0.005 min
Lab File: BN019496.D
Acq: 19 Apr 2022 13:33

Instrument :
BNA_N
ClientSampleId :
BFFE5

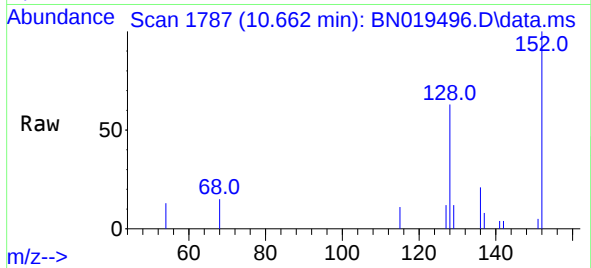

Tgt Ion:	128	Resp:	1298
Ion	Ratio	Lower	Upper
128	100		
129	19.0	9.5	14.3#
127	18.4	11.0	16.4#

