

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN024996.D
 Acq On : 19 Apr 2023 11:30
 Operator : CG/JU
 Sample : PB152182BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK182

Quant Time: Apr 20 04:20:13 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	9333	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	28838	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.576	164	16434	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.322	188	34709	0.400	ng/ul	0.00
17) Chrysene-d12	21.524	240	26396	0.400	ng/ul	0.00
23) Perylene-d12	23.959	264	26596	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	58310	5.721	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	11889	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.355	212	26293	0.401	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.570	166	4112	0.069	ng/ul#	11
20) Pyrene	19.722	202	4071	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.801	252	7773	0.088	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN024996.D
Acq On : 19 Apr 2023 11:30
Operator : CG/JU
Sample : PB152182BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK182

Quant Time: Apr 20 04:20:13 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration




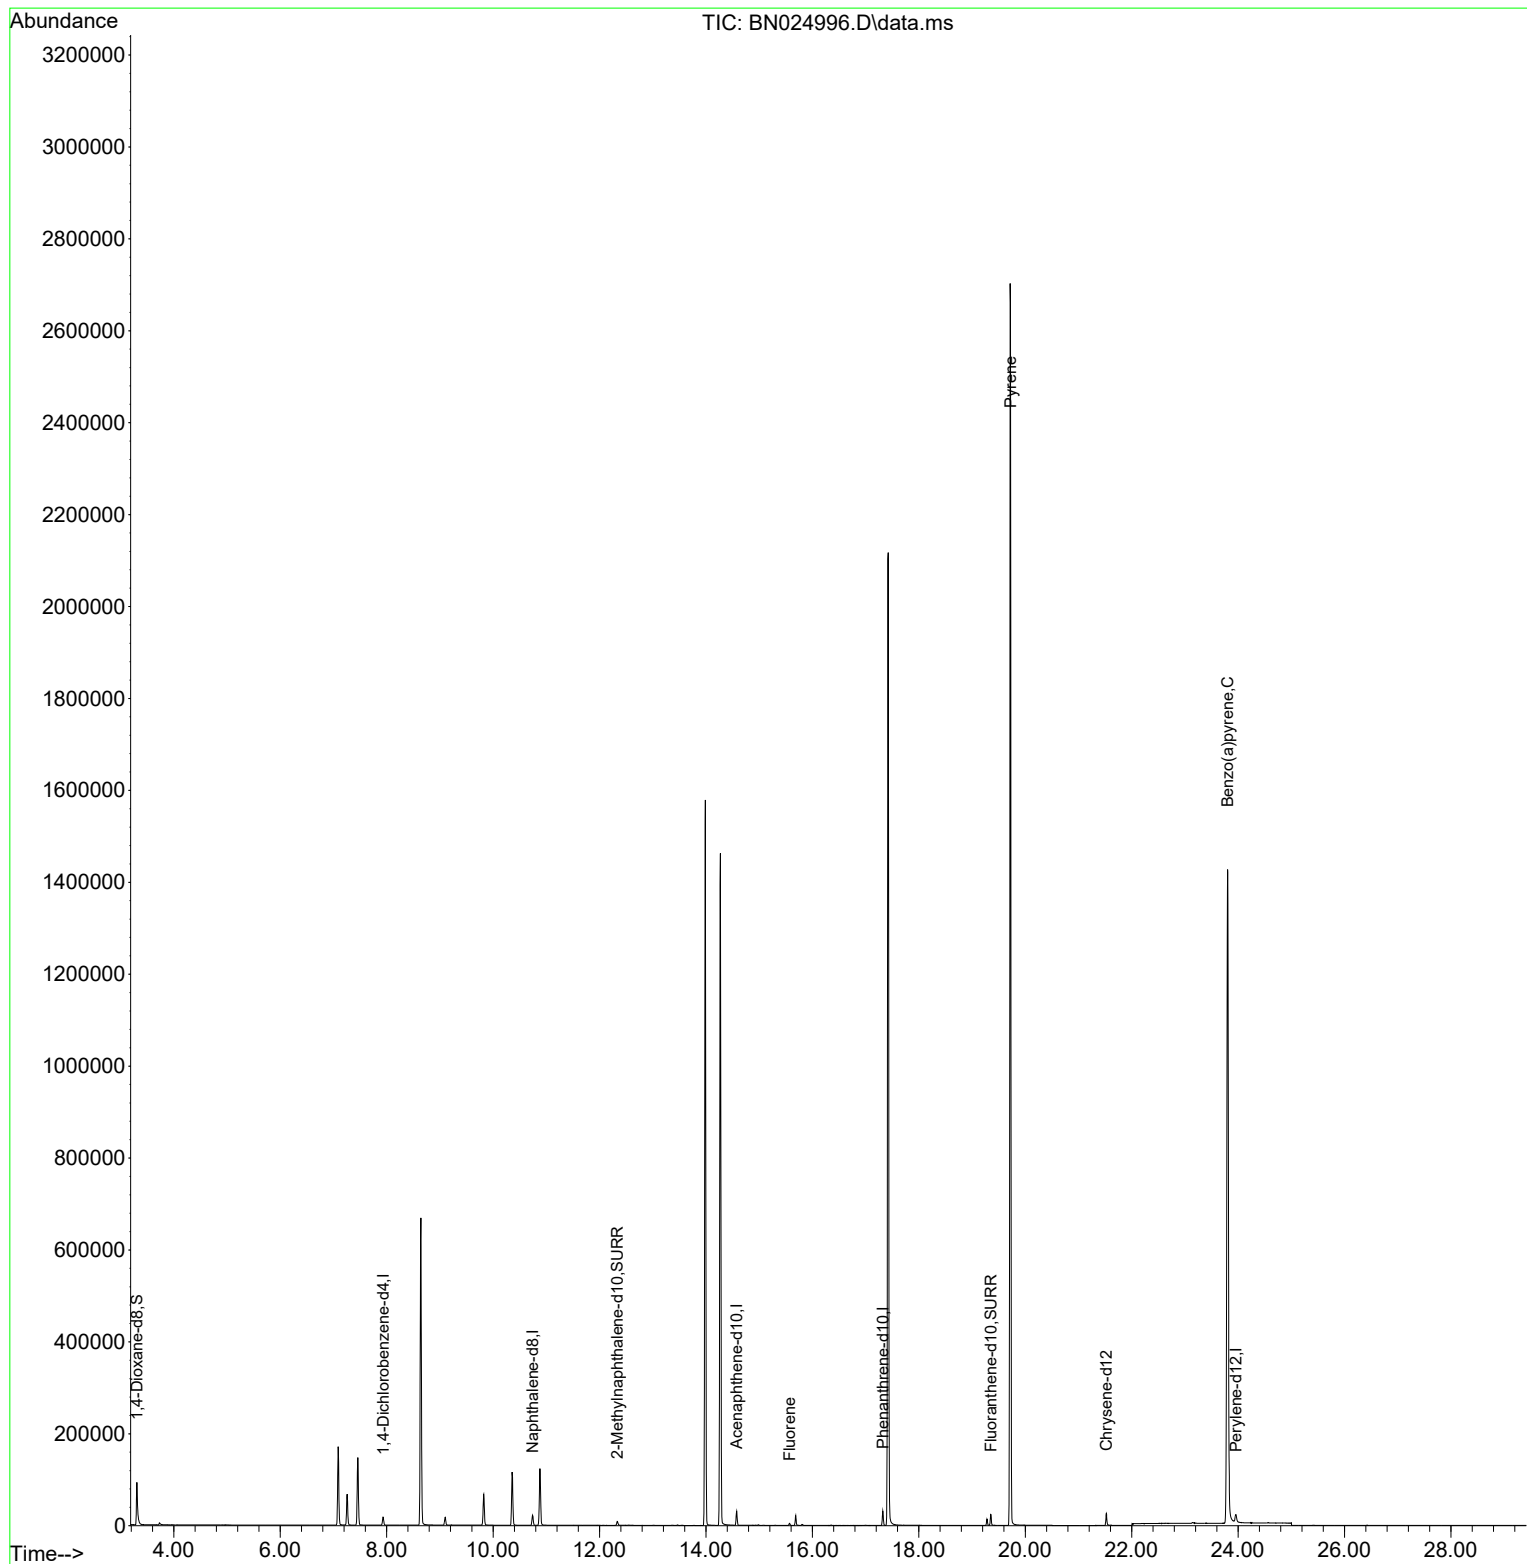


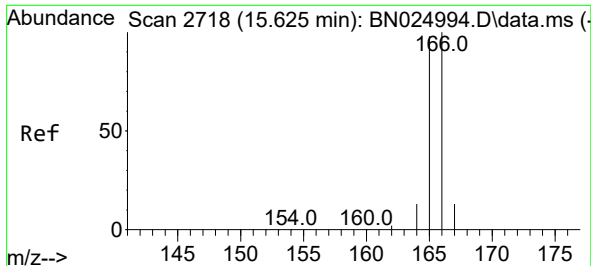

#12
Fluorene
Concen: 0.069 ng/ul
RT: 15.570 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN024996.D
Acq: 19 Apr 2023 11:30




Instrument :
BNA_N
ClientSampleId :
SBLK182


Tgt Ion:166 Resp: 4112
Ion Ratio Lower Upper
166 100
165 6.6 80.1 120.1#
167 34.8 10.7 16.1#

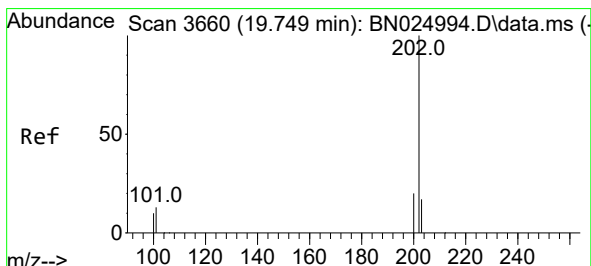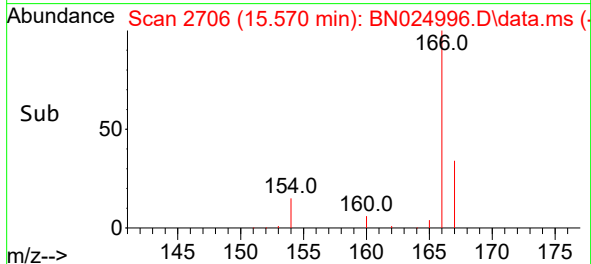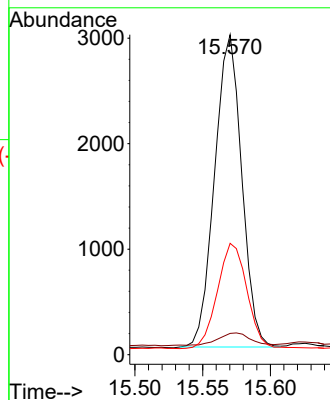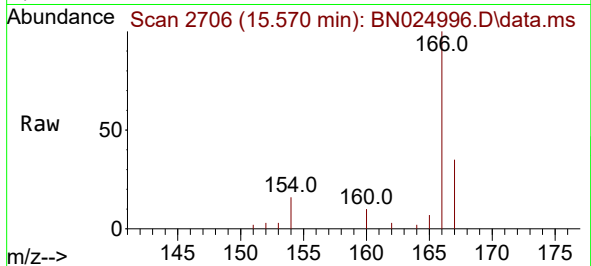

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.722 min Scan# 3654
Delta R.T. -0.027 min
Lab File: BN024996.D
Acq: 19 Apr 2023 11:30


Tgt Ion:202 Resp: 4071
Ion Ratio Lower Upper
202 100
101 166.9 11.8 17.8#
100 1185.4 9.5 14.3#

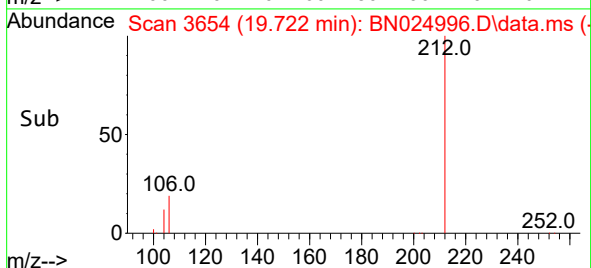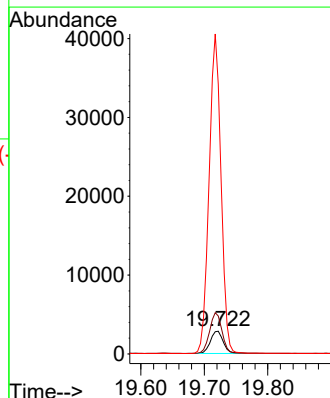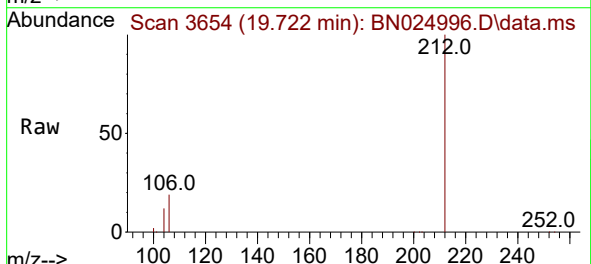

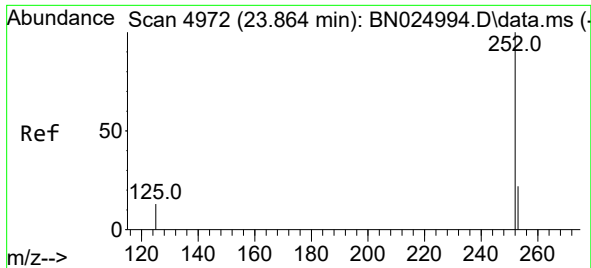

#26
Benzo(a)pyrene
Concen: 0.088 ng/ul
RT: 23.801 min Scan# 4950
Delta R.T. -0.063 min
Lab File: BN024996.D
Acq: 19 Apr 2023 11:30

Instrument :
BNA_N
ClientSampleId :
SBLK182

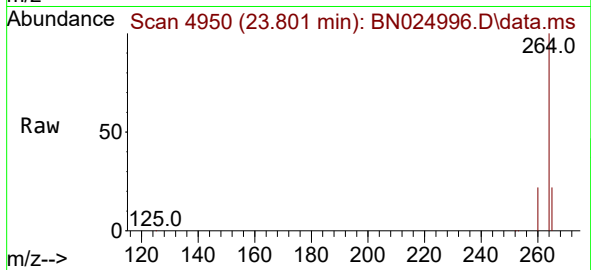

Tgt Ion:252 Resp: 7773
Ion Ratio Lower Upper
252 100
253 44.6 20.7 31.1#
125 39.1 15.9 23.9#

