

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN025012.D
 Acq On : 19 Apr 2023 21:38
 Operator : CG/JU
 Sample : PB152206BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK206

Quant Time: Apr 20 05:10:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 20 05:08:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	6950	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	22125	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.575	164	13176	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	28497	0.400	ng/ul	0.00
17) Chrysene-d12	21.514	240	23707	0.400	ng/ul	0.00
23) Perylene-d12	23.943	264	23146	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	44770	5.899	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	9779	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.354	212	22880	0.389	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.716	202	3698	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.788	252	6885	0.089	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN025012.D
Acq On : 19 Apr 2023 21:38
Operator : CG/JU
Sample : PB152206BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK206

Quant Time: Apr 20 05:10:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 05:08:16 2023
Response via : Initial Calibration




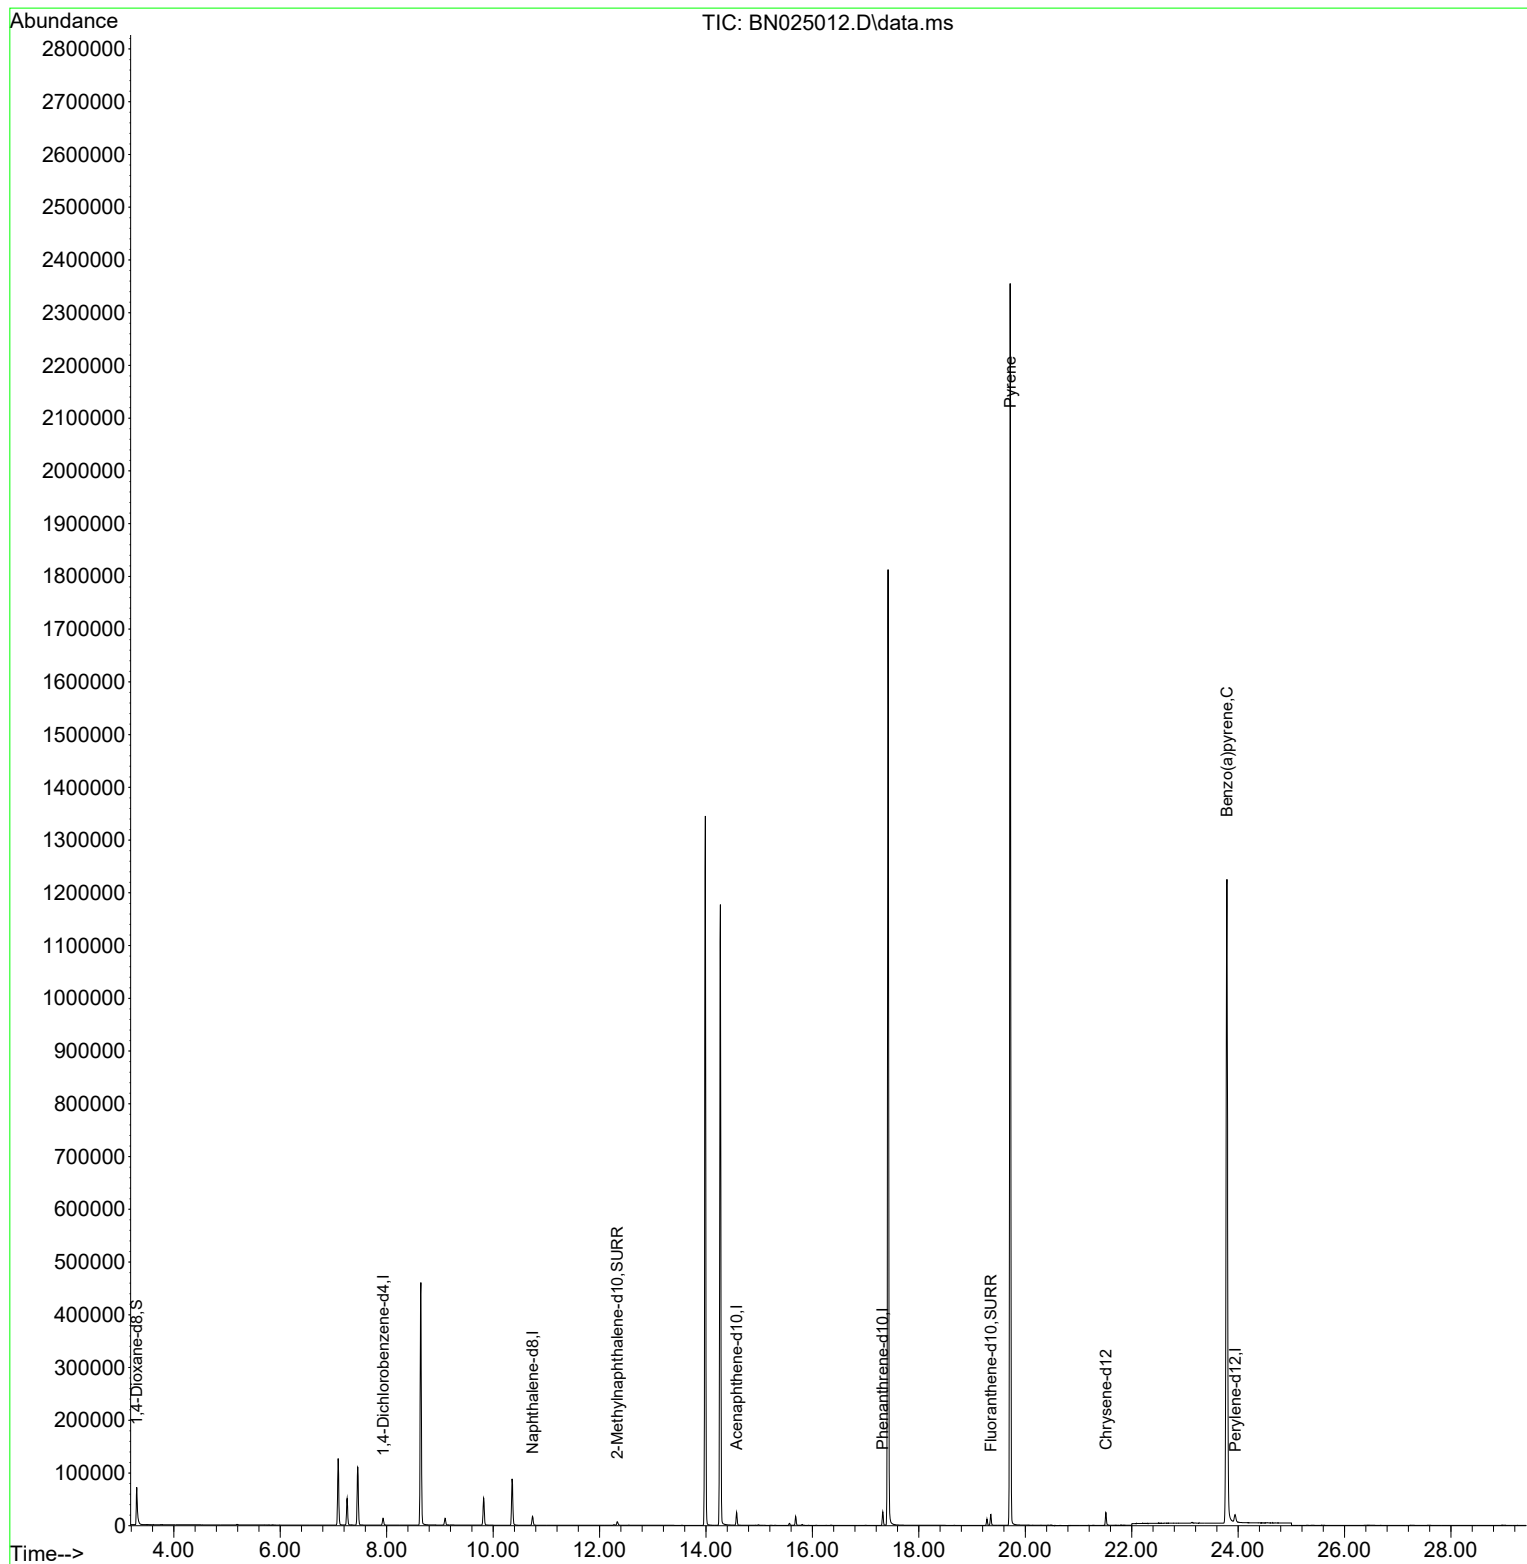


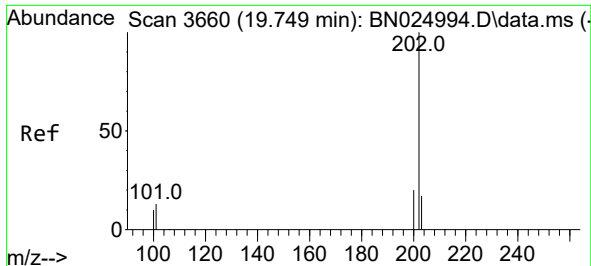

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.716 min Scan# 3653
Delta R.T. -0.028 min
Lab File: BN025012.D
Acq: 19 Apr 2023 21:38

Instrument :
BNA_N
ClientSampleId :
SBLK206

Tgt Ion:202 Resp: 3698
Ion Ratio Lower Upper
202 100
101 179.4 11.8 17.8#
100 1316.5 9.5 14.3#

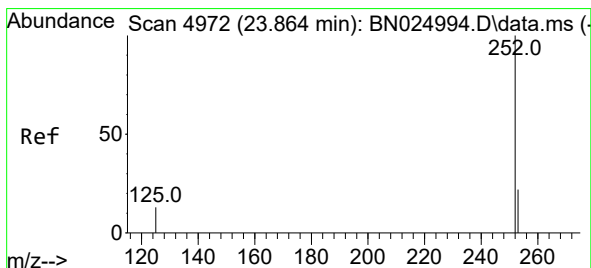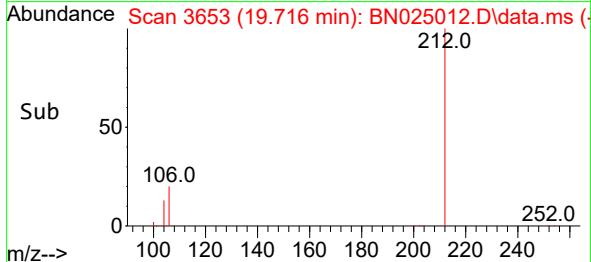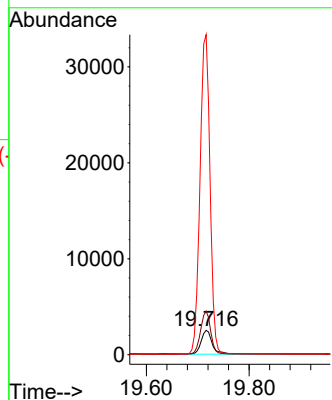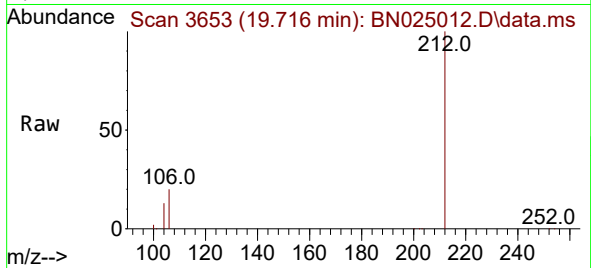

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.788 min Scan# 4946
Delta R.T. -0.064 min
Lab File: BN025012.D
Acq: 19 Apr 2023 21:38

Tgt Ion:252 Resp: 6885
Ion Ratio Lower Upper
252 100
253 50.6 20.7 31.1#
125 40.4 15.9 23.9#

