




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN024999.D
Acq On : 19 Apr 2023 13:17
Operator : CG/JU
Sample : 02340-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE05

Manual IntegrationsAPPROVED

Quant Time: Apr 20 04:20:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/20/2023
Supervised By :Jagrut Upadhyay 04/20/2023

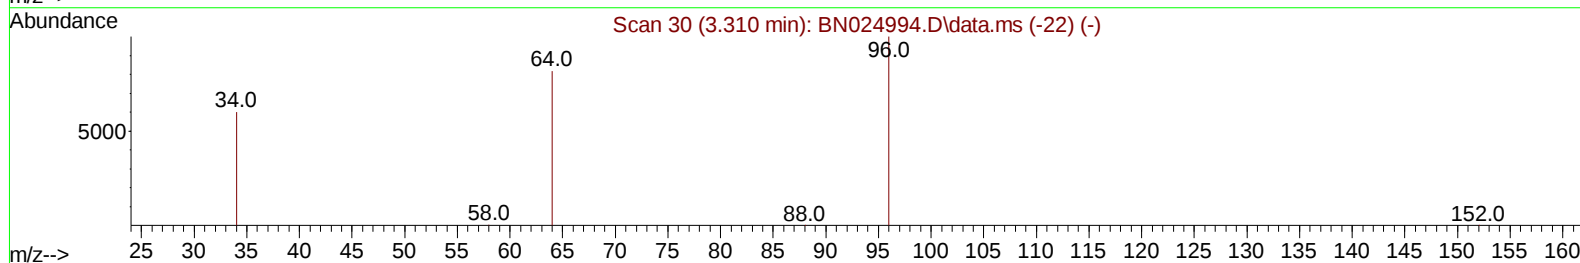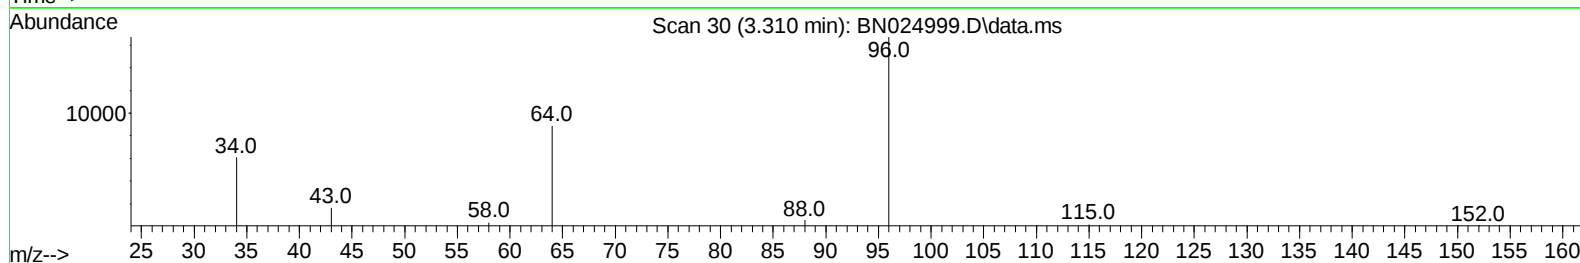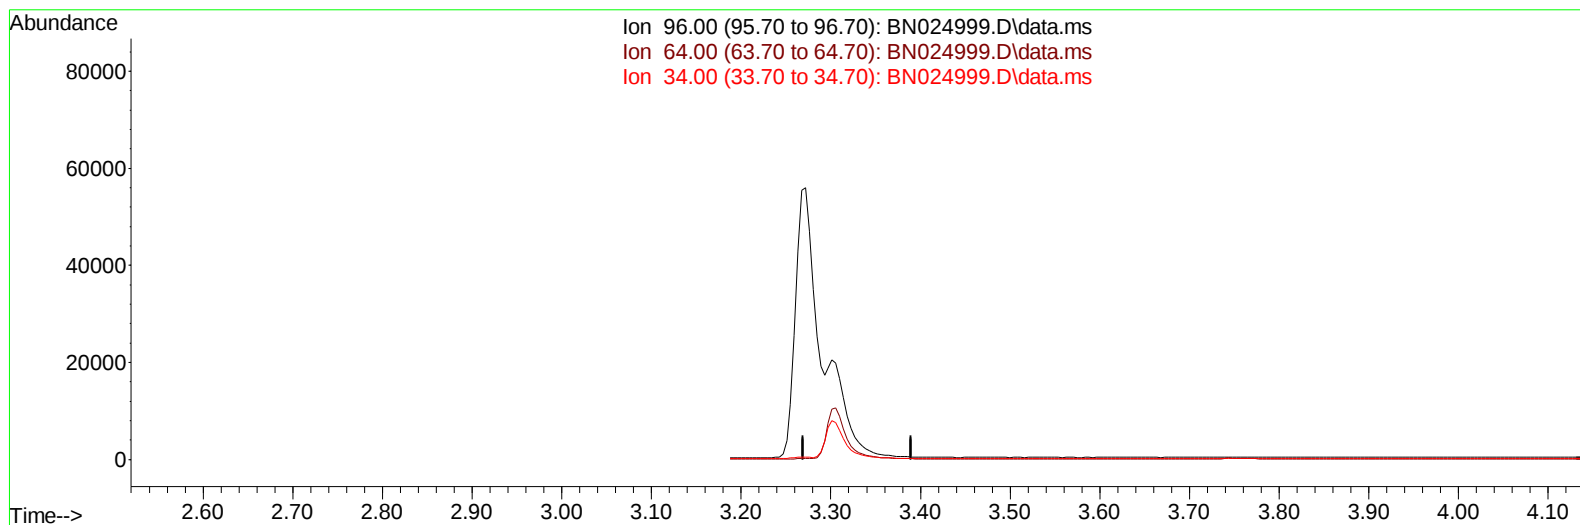

TIC: BN024999.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.310min (-3.310) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	76.40	0.00#
34.00	61.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN024999.D
 Acq On : 19 Apr 2023 13:17
 Operator : CG/JU
 Sample : 02340-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE05

Manual IntegrationsAPPROVED

Quant Time: Apr 20 04:20:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/20/2023
 Supervised By :Jagrut Upadhyay 04/20/2023

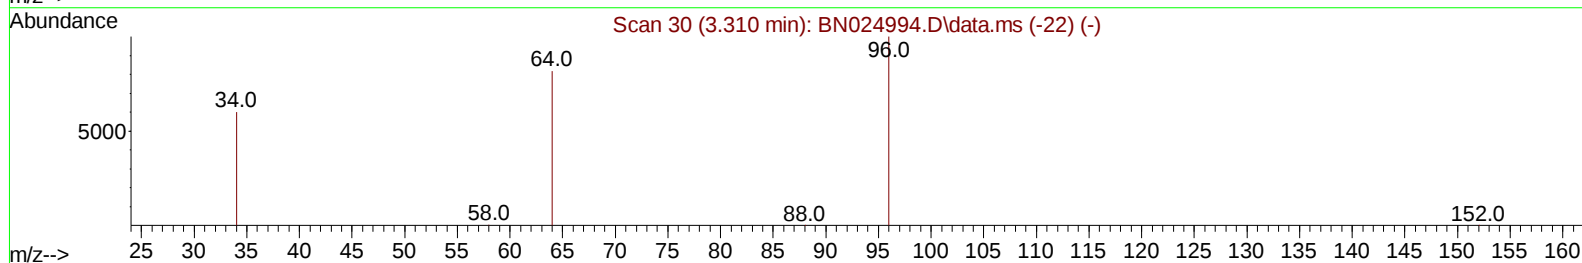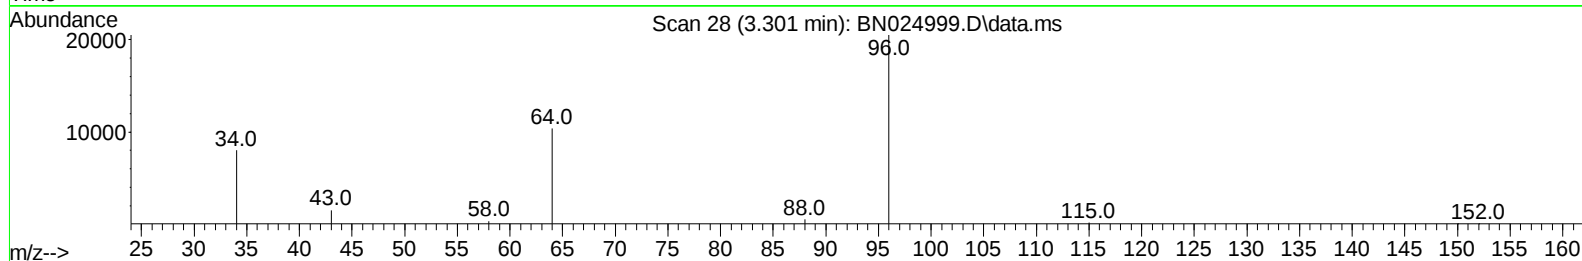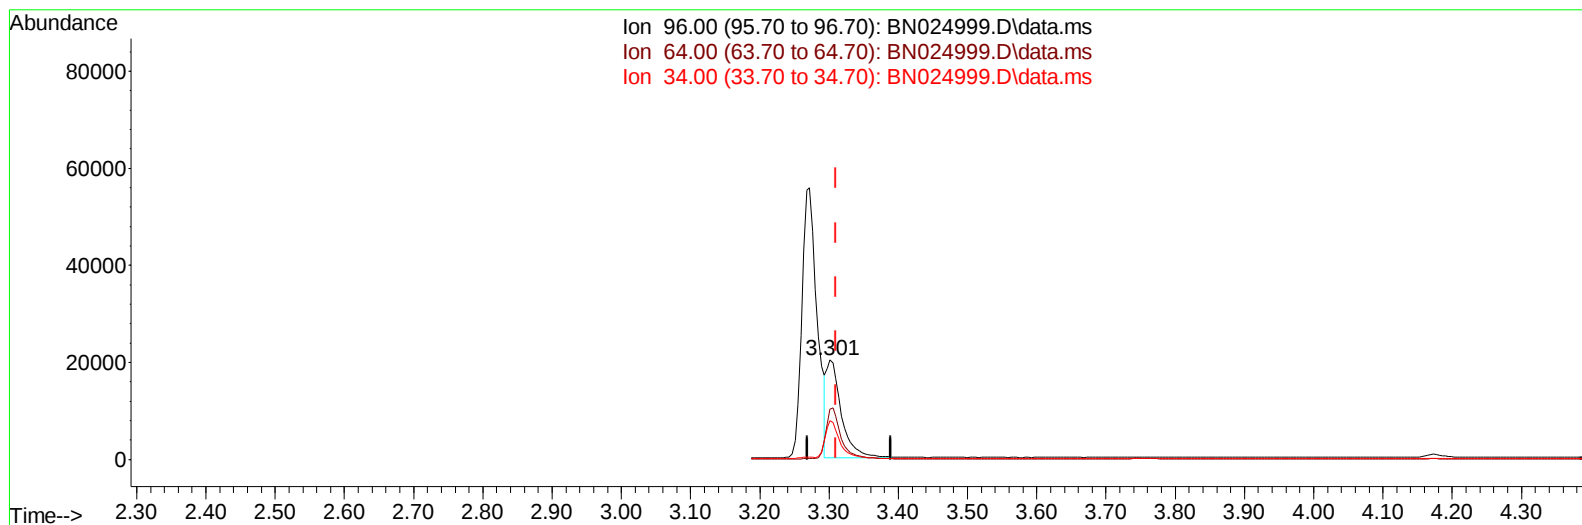

TIC: BN024999.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.301min (-0.008) 3.49 ng/ul m

response 30074

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	50.59#
34.00	61.90	39.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN024999.D
 Acq On : 19 Apr 2023 13:17
 Operator : CG/JU
 Sample : 02340-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE05

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/20/2023
 Supervised By :Jagrut Upadhyay 04/20/2023

Quant Time: Apr 20 04:20:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.934	152		7888	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136		24601	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.575	164		14412	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188		31761	0.400	ng/ul	0.00
17) Chrysene-d12	21.520	240		27075	0.400	ng/ul	0.00
23) Perylene-d12	23.967	264		26585	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.301	96		30074m	3.491	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152		10038	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.354	212		27513	0.409	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.339	88		62087	6.542	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN024999.D
Acq On : 19 Apr 2023 13:17
Operator : CG/JU
Sample : 02340-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE05

Manual IntegrationsAPPROVED

Quant Time: Apr 20 04:20:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/20/2023
Supervised By :Jagrut Upadhyay 04/20/2023

