




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN025002.D
 Acq On : 19 Apr 2023 15:04
 Operator : CG/JU
 Sample : 02340-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE06

Manual IntegrationsAPPROVED

Quant Time: Apr 20 04:20:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/20/2023
 Supervised By :Jagrut Upadhyay 04/20/2023

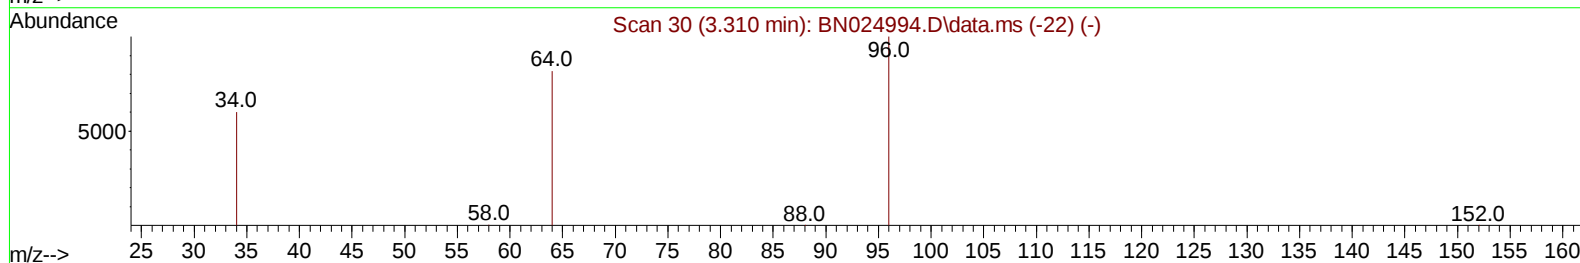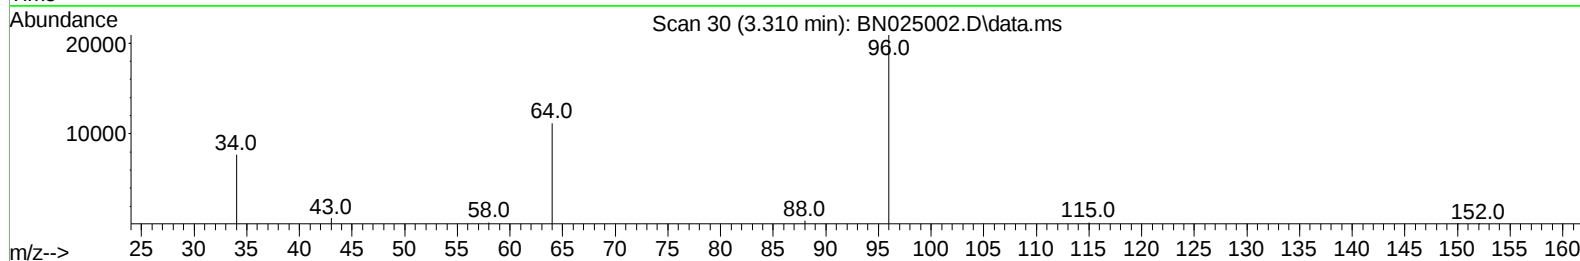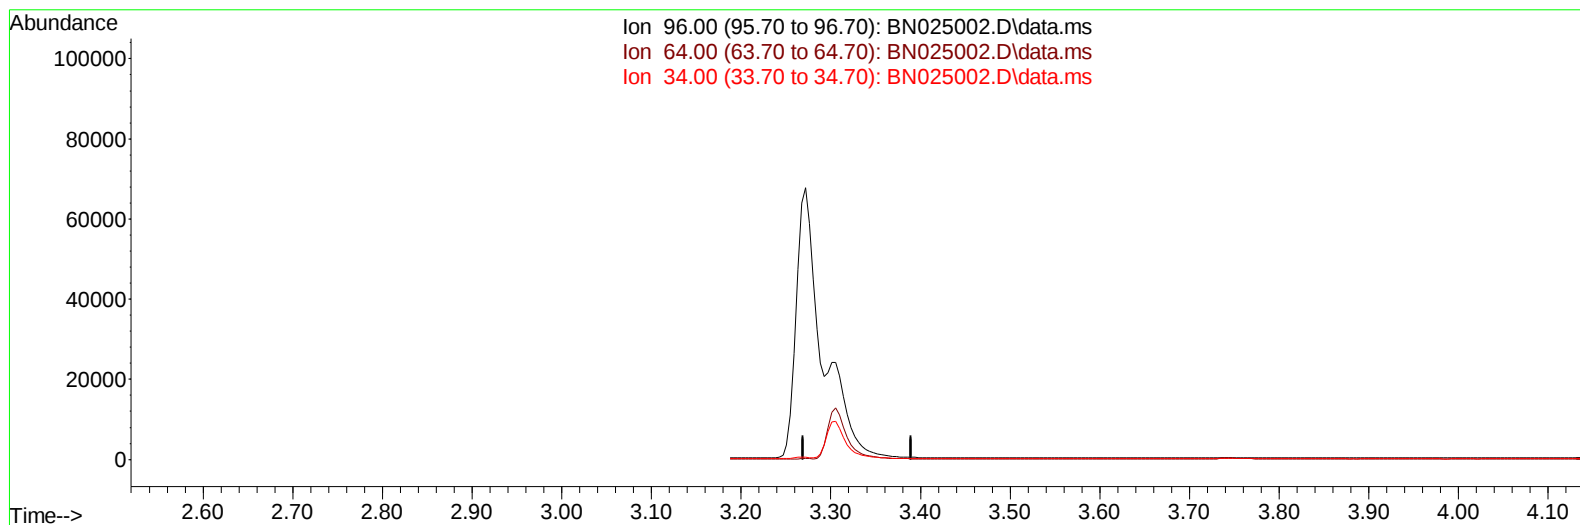

TIC: BN025002.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.310min (-3.310) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	76.40	0.00#
34.00	61.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN025002.D
Acq On : 19 Apr 2023 15:04
Operator : CG/JU
Sample : 02340-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE06

Manual IntegrationsAPPROVED

Quant Time: Apr 20 04:20:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/20/2023
Supervised By :Jagrut Upadhyay 04/20/2023

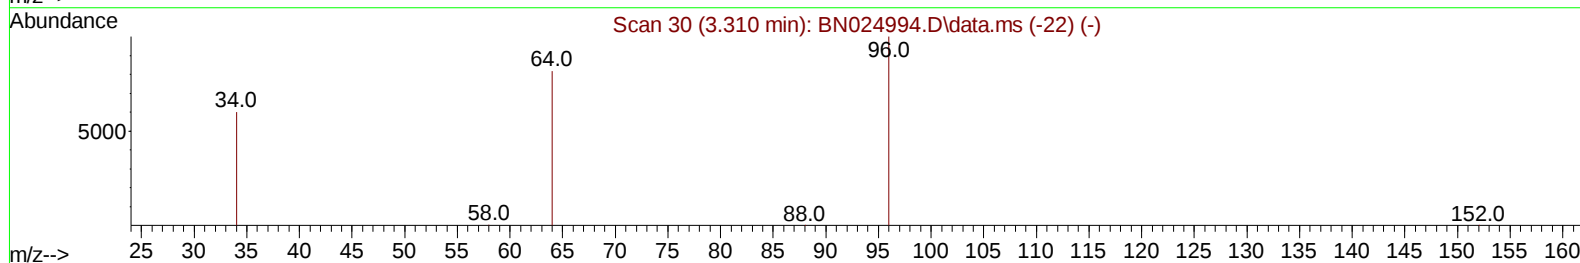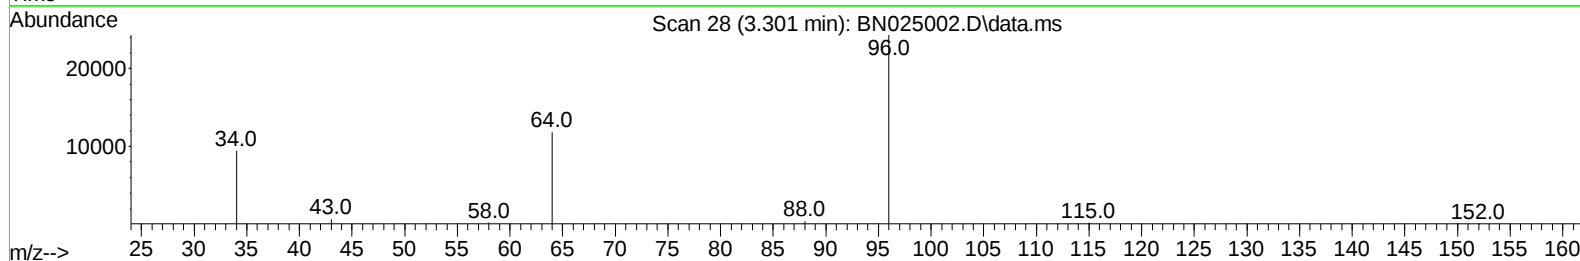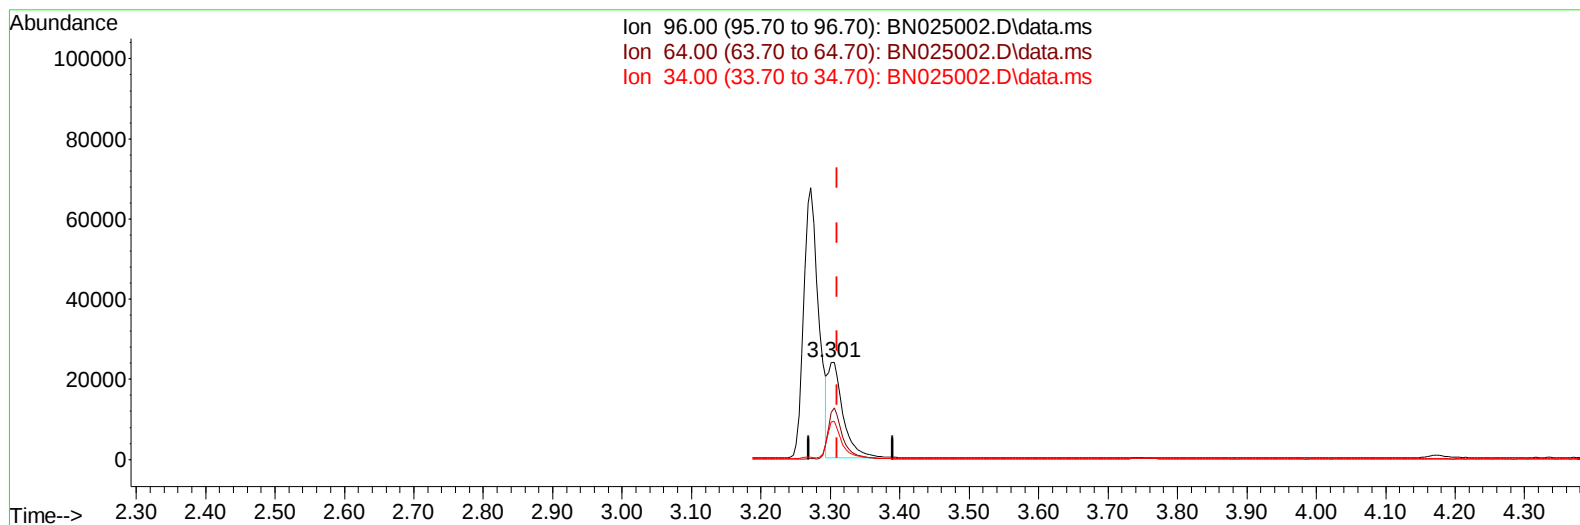

TIC: BN025002.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.301min (-0.008) 4.63 ng/ul m

response 36217

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.40	48.72#
34.00	61.90	38.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN025002.D
 Acq On : 19 Apr 2023 15:04
 Operator : CG/JU
 Sample : 02340-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE06

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/20/2023
 Supervised By :Jagrut Upadhyay 04/20/2023

Quant Time: Apr 20 04:20:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.934	152		7166	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136		22598	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.575	164		13278	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188		29233	0.400	ng/ul	0.00
17) Chrysene-d12	21.520	240		24773	0.400	ng/ul	0.00
23) Perylene-d12	23.964	264		24426	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.301	96		36217m	4.628	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152		11555	0.398	ng/ul	0.00
18) Fluoranthene-d10	19.354	212		30868	0.502	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.339	88		58361	6.769	ng/ul	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN025002.D
Acq On : 19 Apr 2023 15:04
Operator : CG/JU
Sample : 02340-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE06

Manual IntegrationsAPPROVED

Quant Time: Apr 20 04:20:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/20/2023
Supervised By :Jagrut Upadhyay 04/20/2023

