

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN024999.D
 Acq On : 19 Apr 2023 13:17
 Operator : CG/JU
 Sample : 02340-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE05

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/20/2023
 Supervised By : Jagrut Upadhyay 04/20/2023

Quant Time: Apr 20 04:20:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	7888	0.400	ng/u1	0.00
4) Naphthalene-d8	10.743	136	24601	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.575	164	14412	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.326	188	31761	0.400	ng/u1	0.00
17) Chrysene-d12	21.520	240	27075	0.400	ng/u1	0.00
23) Perylene-d12	23.967	264	26585	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	30074m	3.491	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.332	152	10038	0.318	ng/u1	0.00
18) Fluoranthene-d10	19.354	212	27513	0.409	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	62087	6.542	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\  
Data File : BN024999.D  
Acq On    : 19 Apr 2023   13:17  
Operator  : CG/JU  
Sample    : 02340-04  
Misc      :  
ALS Vial  : 7    Sample Multiplier: 1
```


Instrument :
BNA_N
ClientSampleId :
BHE05

Manual Integrations

Reviewed By :Christian Giraldo 04/20/2023
Supervised By :Jagrut Upadhyay 04/20/2023


Quant Time: Apr 20 04:20:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration

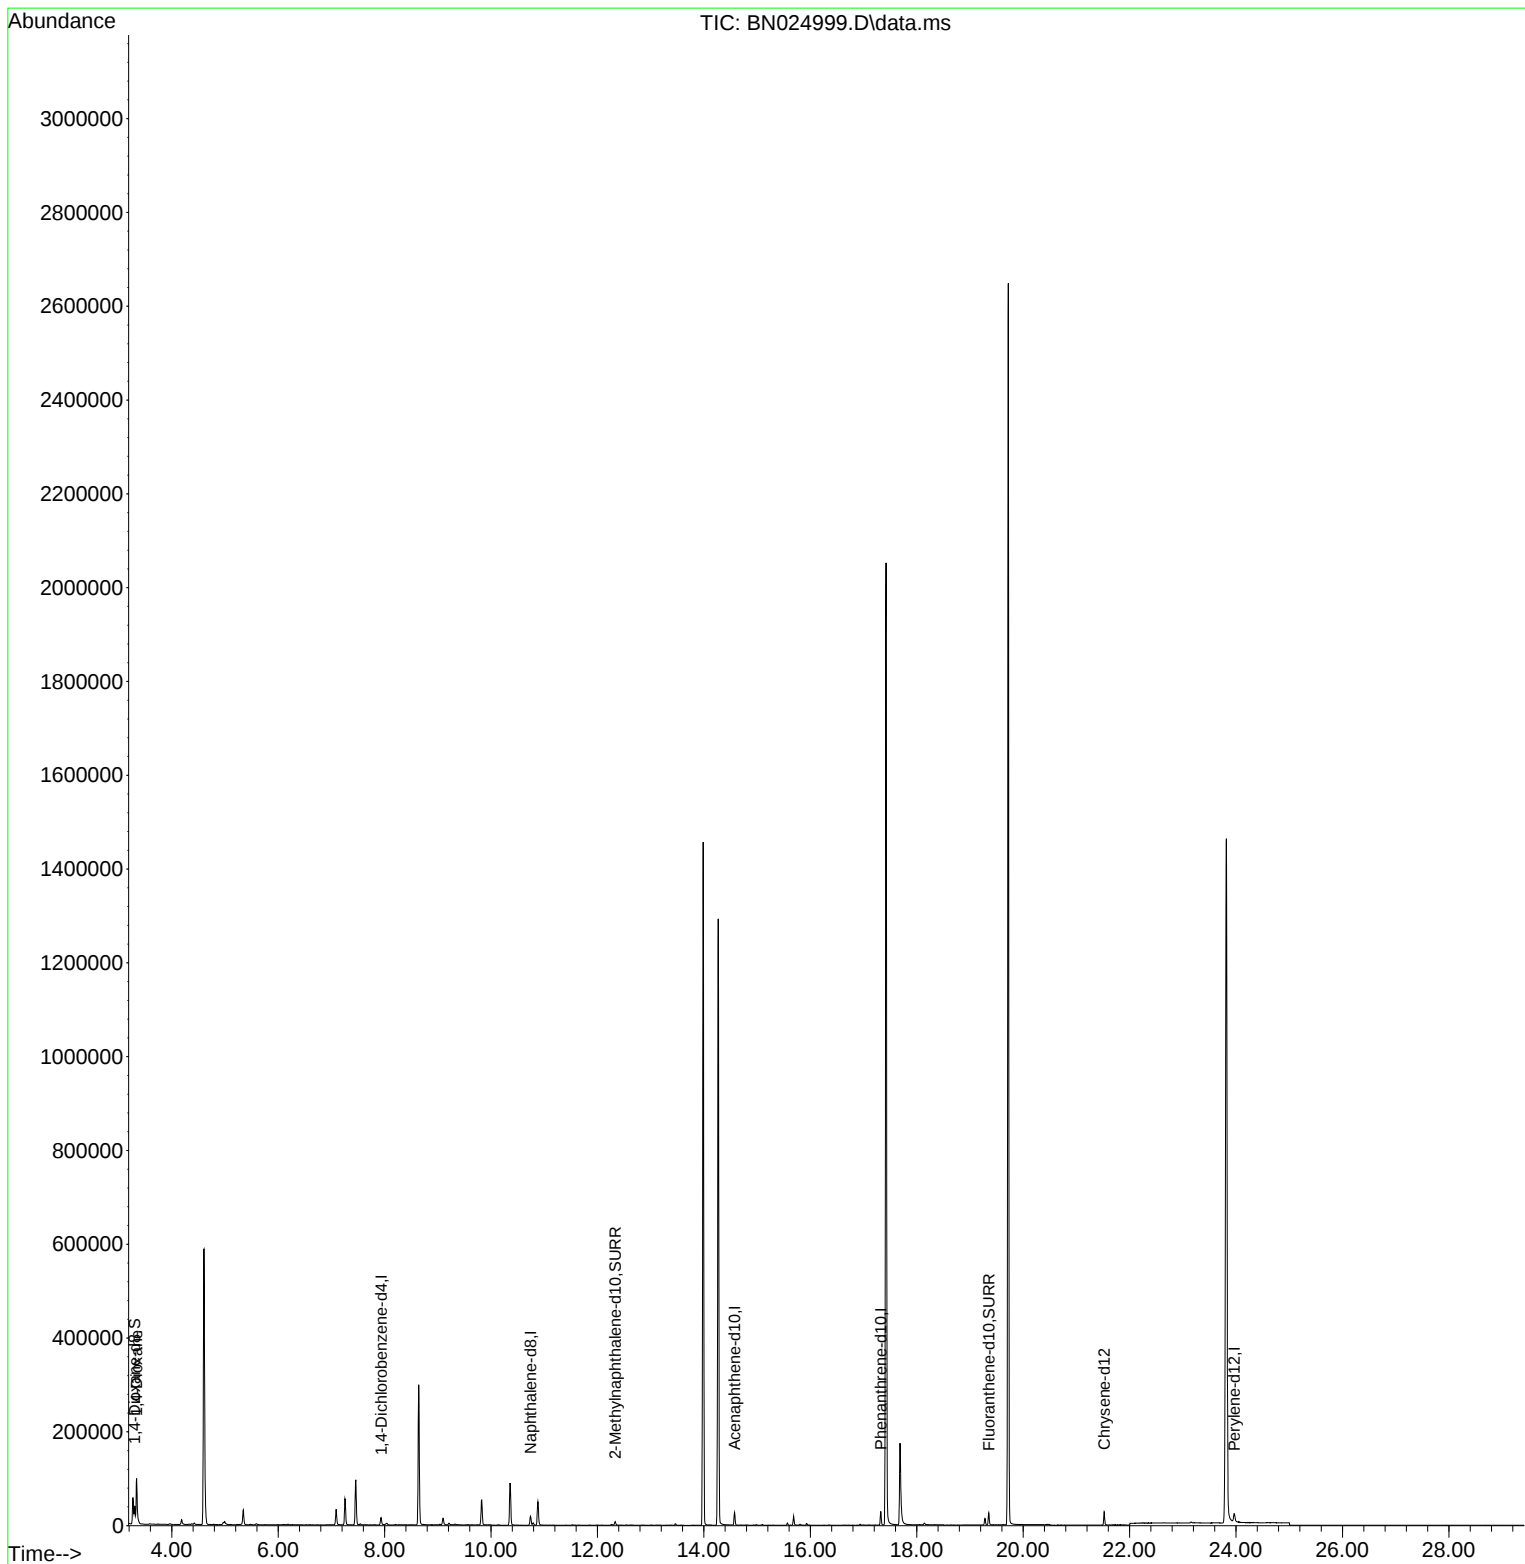

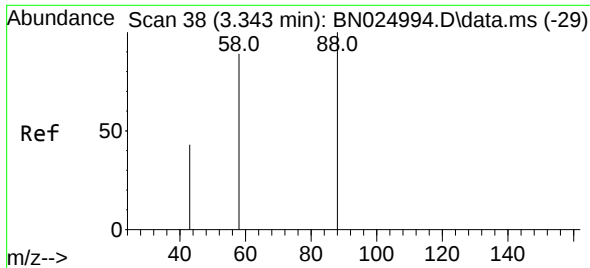

#2
 1,4-Dioxane
 Concen: 6.542 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN024999.D
 Acq: 19 Apr 2023 13:17

Instrument :
 BNA_N
 ClientSampleId :
 BHE05

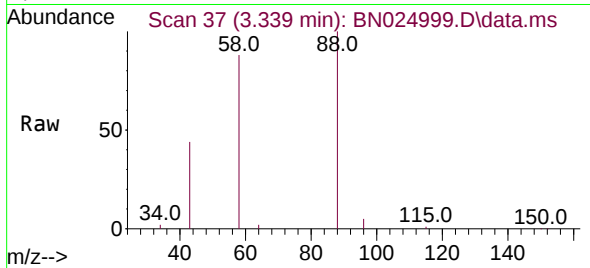

Tgt Ion: 88 Resp: 6208
 Ion Ratio Lower Upper
 88 100
 43 43.9 39.1 58.7
 58 87.6 65.7 98.5

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 04/20/2023
 Supervised By :Jagrut Upadhyay 04/20/2023

