

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
 Data File : BN025001.D
 Acq On : 19 Apr 2023 14:29
 Operator : CG/JU
 Sample : 02340-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE08

Quant Time: Apr 20 04:20:48 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 19 18:38:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	7668	0.400	ng/u1	0.00
4) Naphthalene-d8	10.743	136	23794	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.575	164	13958	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.326	188	30496	0.400	ng/u1	0.00
17) Chrysene-d12	21.523	240	25474	0.400	ng/u1	0.00
23) Perylene-d12	23.969	264	24593	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	20500	2.448	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.332	152	10437	0.342	ng/u1	0.00
18) Fluoranthene-d10	19.354	212	30714	0.485	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.339	88	29328	3.179	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041923\
Data File : BN025001.D
Acq On : 19 Apr 2023 14:29
Operator : CG/JU
Sample : 02340-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE08


Quant Time: Apr 20 04:20:48 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 18:38:47 2023
Response via : Initial Calibration

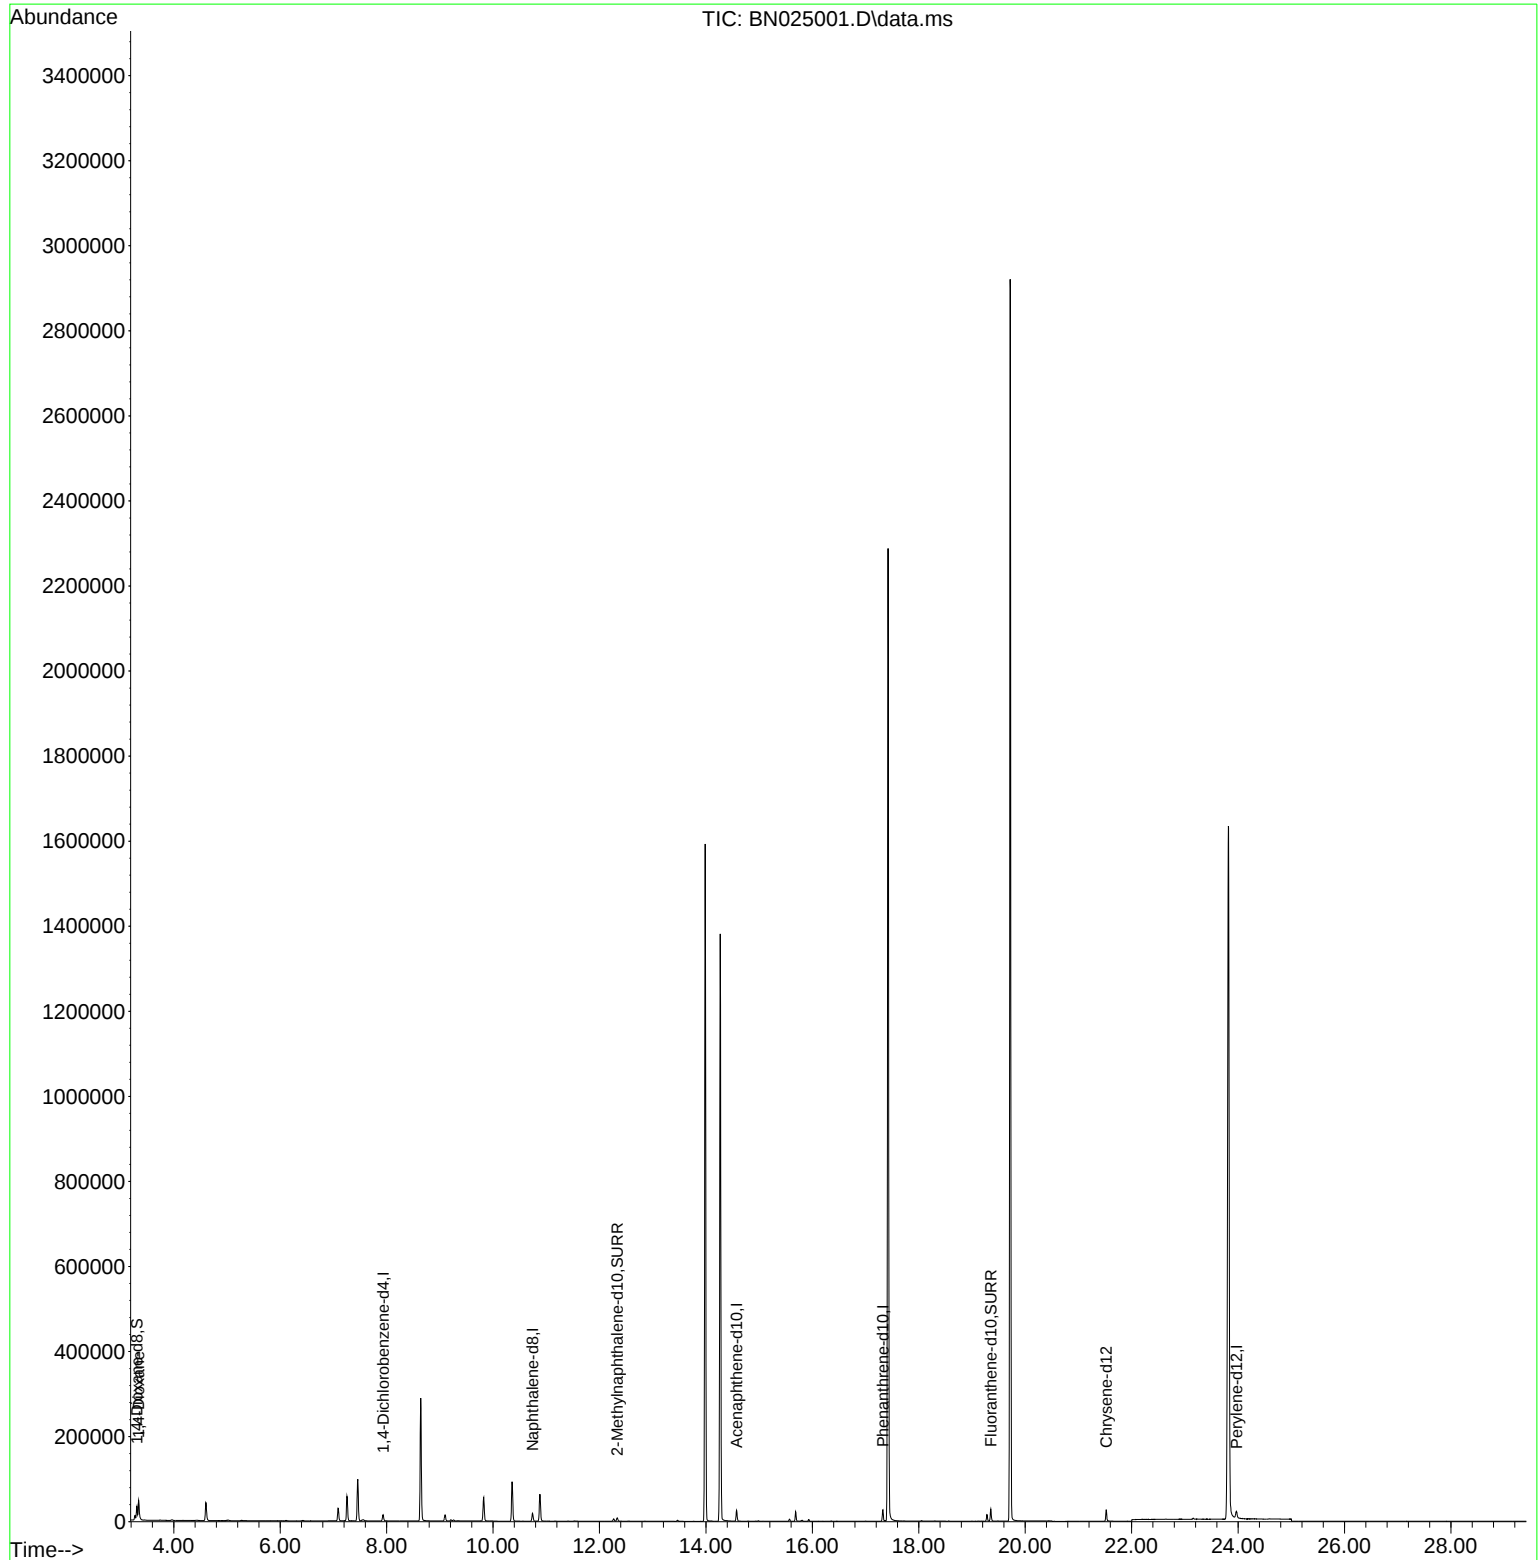

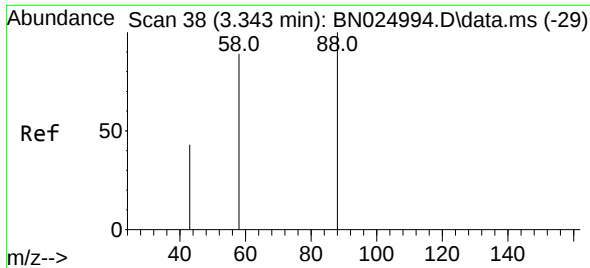

#2
 1,4-Dioxane
 Concen: 3.179 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN025001.D
 Acq: 19 Apr 2023 14:29

Instrument :
 BNA_N
 ClientSampleId :
 BHE08

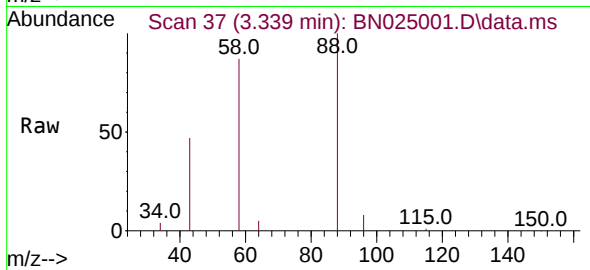

Tgt Ion:	88	Resp:	29328
Ion	Ratio	Lower	Upper
88	100		
43	47.4	39.1	58.7
58	87.4	65.7	98.5

