

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031057.D
 Acq On : 20 Apr 2024 02:59
 Operator : MA/JU
 Sample : P2145-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07Y0

Quant Time: Apr 20 03:32:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	102899	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	474224	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	319773	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.033	188	760737	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	876541	20.000	ng/ul	0.00
88) Perylene-d12	24.168	264	1170554	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	7485	3.398	ng/uL	0.00
4) Pyridine-d5	3.558	84	62039	9.781	ng/ul	0.00
7) Phenol-d5	6.810	99	113404	13.065	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	108314	21.447	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	89142	13.190	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	89202	12.220	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	71326	20.934	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	69114	19.514	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	92550	13.251	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	91992	8.428	ng/ul	0.00
46) Dimethylphthalate-d6	13.698	166	533145	23.959	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	375010	14.872	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	55216	11.889	ng/ul	0.00
60) Fluorene-d10	15.275	176	334499	17.268	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	49430	12.879	ng/ul	0.00
73) Anthracene-d10	17.128	188	529334	16.054	ng/ul	0.00
81) Pyrene-d10	19.433	212	713607	16.567	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	921653	16.604	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.180	149	782772	22.059	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031057.D
Acq On : 20 Apr 2024 02:59
Operator : MA/JU
Sample : P2145-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07Y0

Quant Time: Apr 20 03:32:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

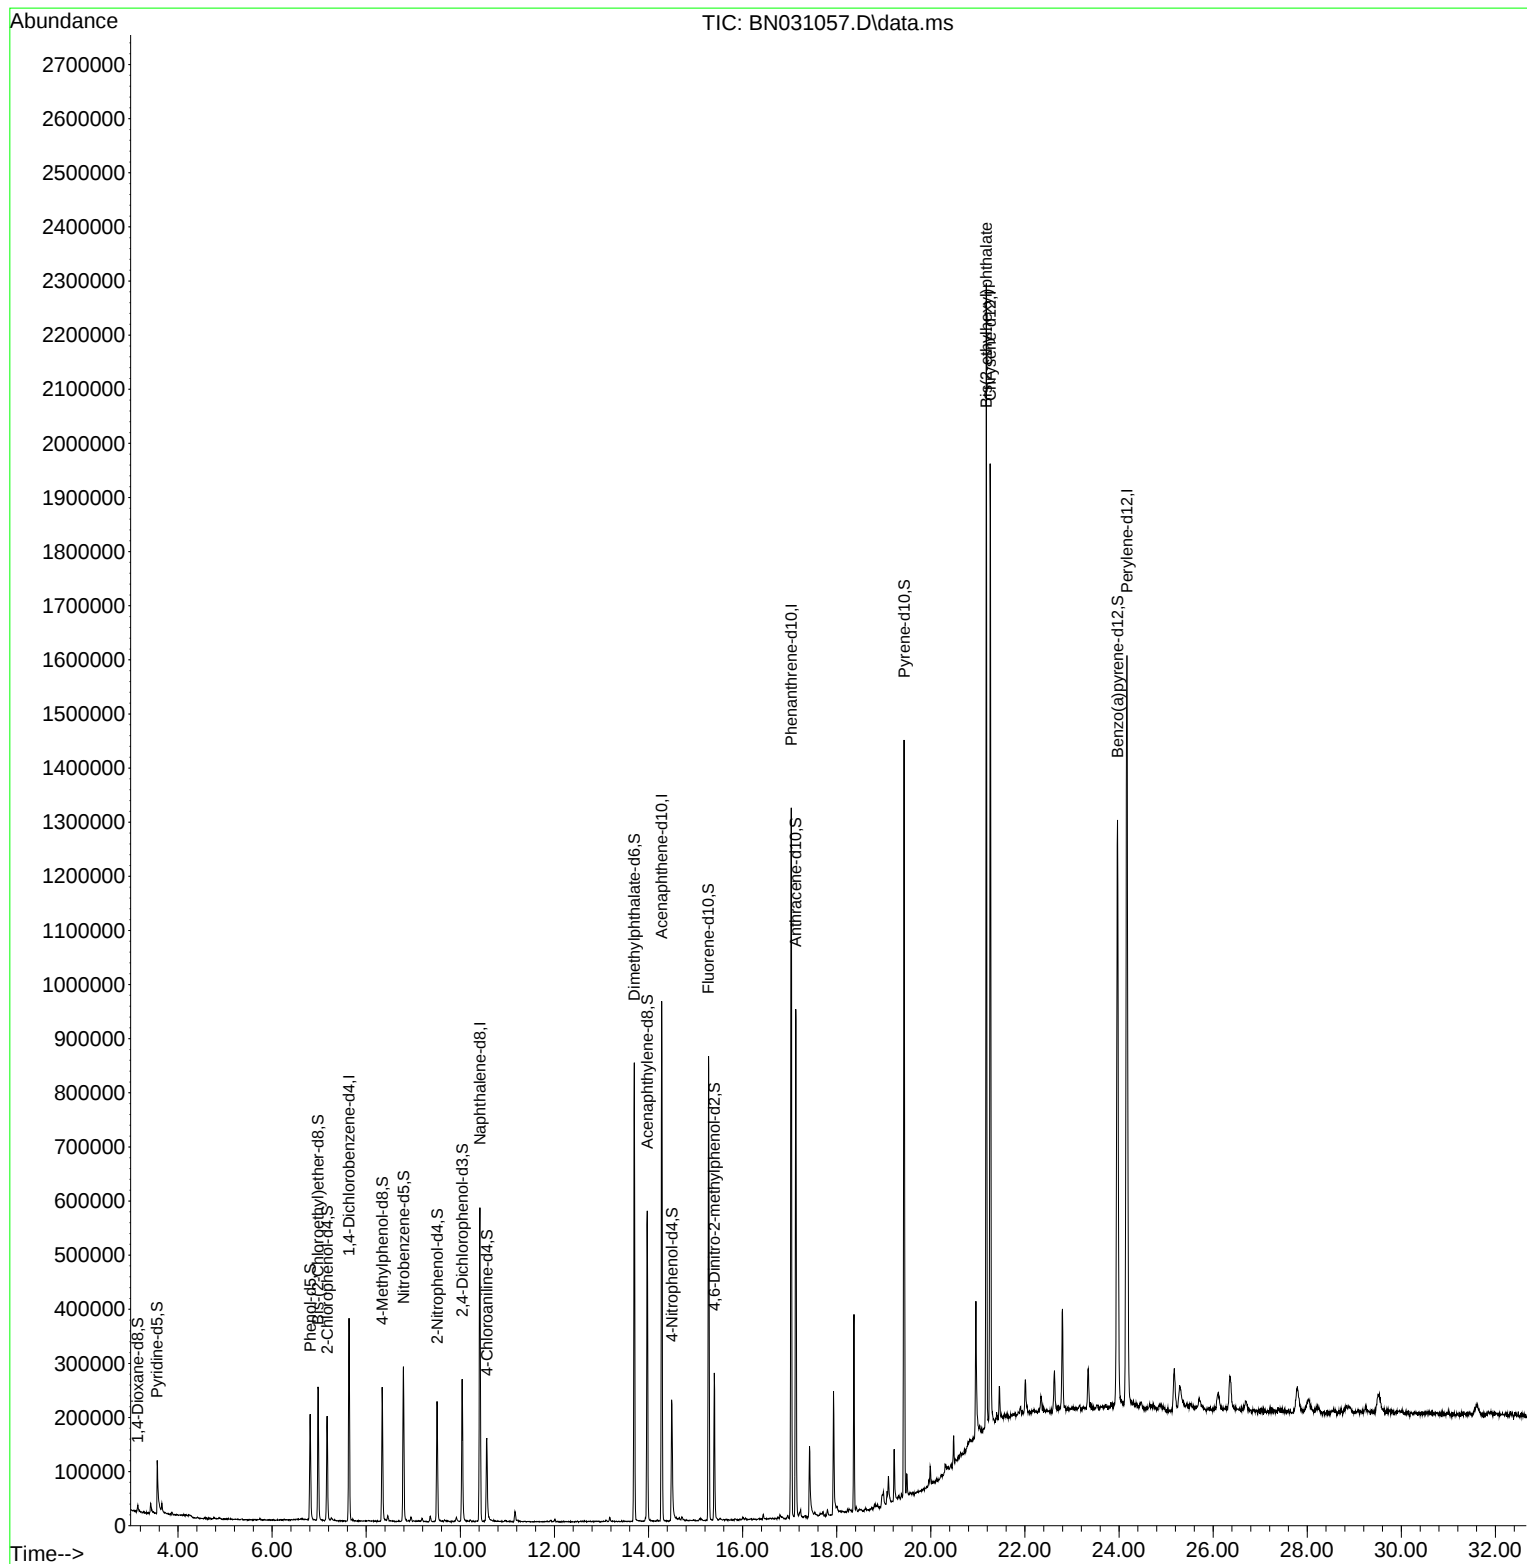

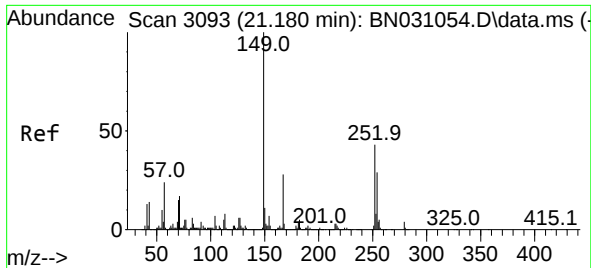

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 22.059 ng/ul
 RT: 21.180 min Scan# 3093
 Delta R.T. -0.000 min
 Lab File: BN031057.D
 Acq: 20 Apr 2024 02:59

Instrument :
 BNA_N
 ClientSampleId :
 E07Y0

Tgt Ion:149 Resp: 782772
 Ion Ratio Lower Upper
 149 100
 167 27.6 22.3 33.5
 279 4.4 3.0 4.6

