

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031062.D
 Acq On : 20 Apr 2024 06:16
 Operator : MA/JU
 Sample : P2159-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MCOR80

Quant Time: Apr 20 06:47:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	111588	20.000	ng/u1	0.00
20) Naphthalene-d8	10.416	136	512742	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.281	164	351295	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.033	188	806442	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	986848	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1332571	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	9756	4.085	ng/uL	0.00
4) Pyridine-d5	3.563	84	47001	6.833	ng/u1	0.01
7) Phenol-d5	6.810	99	52782	5.607	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	185579	33.885	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	180490	24.626	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	113284	14.310	ng/u1	0.00
21) Nitrobenzene-d5	8.793	128	130241	35.353	ng/u1	0.00
24) 2-Nitrophenol-d4	9.504	143	125537	32.782	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	223188	29.554	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	324209	27.472	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	885020	36.203	ng/u1	0.00
49) Acenaphthylene-d8	13.975	160	984977	35.557	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	22057	4.323	ng/u1	0.00
60) Fluorene-d10	15.281	176	785900	36.930	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	90281	22.189	ng/u1	0.00
73) Anthracene-d10	17.127	188	1315745	37.642	ng/u1	0.00
81) Pyrene-d10	19.433	212	1737702	35.834	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.968	264	2391923	37.852	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.710	107	13231	1.513	ng/u1	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031062.D
Acq On : 20 Apr 2024 06:16
Operator : MA/JU
Sample : P2159-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R80


Quant Time: Apr 20 06:47:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

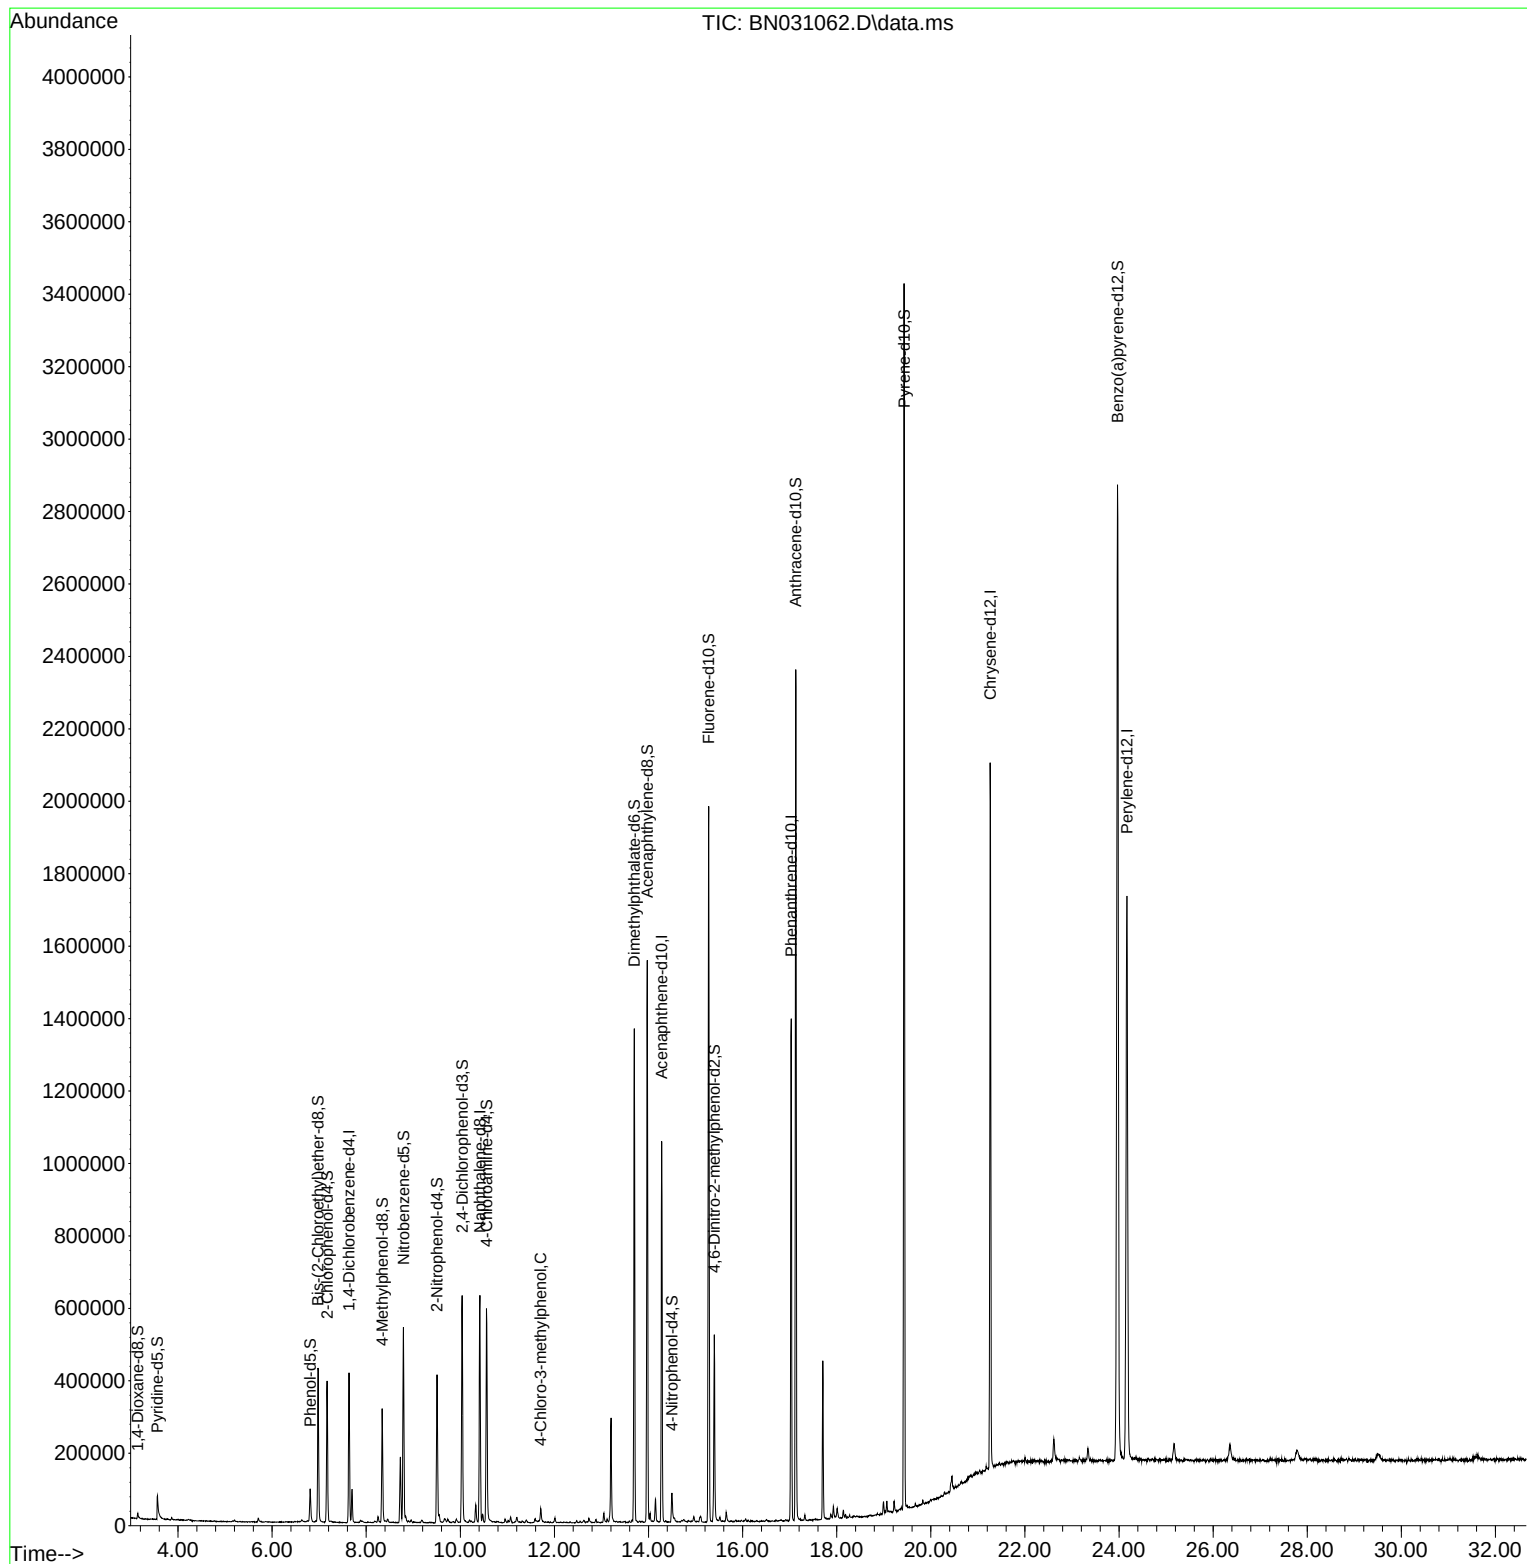

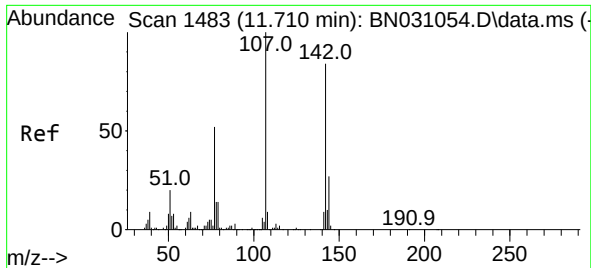

#35
 4-Chloro-3-methylphenol
 Concen: 1.513 ng/ul
 RT: 11.710 min Scan# 14
 Delta R.T. -0.000 min
 Lab File: BN031062.D
 Acq: 20 Apr 2024 06:16

Instrument :
 BNA_N
 ClientSampleId :
 MC0R80

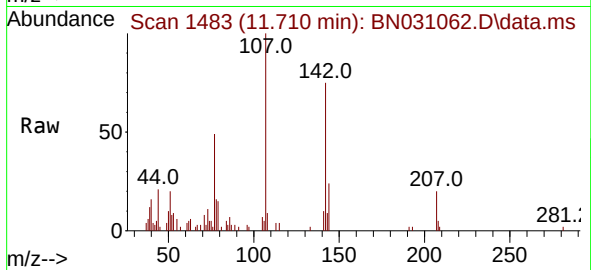

Tgt Ion:	107	Resp:	13231
Ion	Ratio	Lower	Upper
107	100		
144	24.4	20.6	31.0
142	75.3	67.4	101.2

