

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031090.D
 Acq On : 21 Apr 2024 02:02
 Operator : MA/JU
 Sample : P2077-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL3

Quant Time: Apr 21 14:17:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	145022	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	673488	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.281	164	462616	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.033	188	1059636	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1213372	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1530317	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	9091	2.929	ng/uL	0.00
4) Pyridine-d5	3.564	84	34039	3.808	ng/u1	0.01
7) Phenol-d5	6.811	99	52179	4.265	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	177509	24.939	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	171898	18.047	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	113286	11.011	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	123116	25.443	ng/u1	0.00
24) 2-Nitrophenol-d4	9.504	143	114952	22.853	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	218207	21.998	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	300720	19.400	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	939384	29.180	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1008979	27.658	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	22517	3.351	ng/u1	0.00
60) Fluorene-d10	15.275	176	812165	28.981	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	104655	19.576	ng/u1	0.00
73) Anthracene-d10	17.128	188	1450635	31.585	ng/u1	0.00
81) Pyrene-d10	19.433	212	1857123	31.147	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	2451105	33.776	ng/u1	0.00
Target Compounds						
					Qvalue	
35) 4-Chloro-3-methylphenol	11.710	107	12114	1.055	ng/u1	89
59) Diethylphthalate	15.122	149	5228748	153.090	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031090.D
Acq On : 21 Apr 2024 02:02
Operator : MA/JU
Sample : P2077-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAL3

Quant Time: Apr 21 14:17:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration




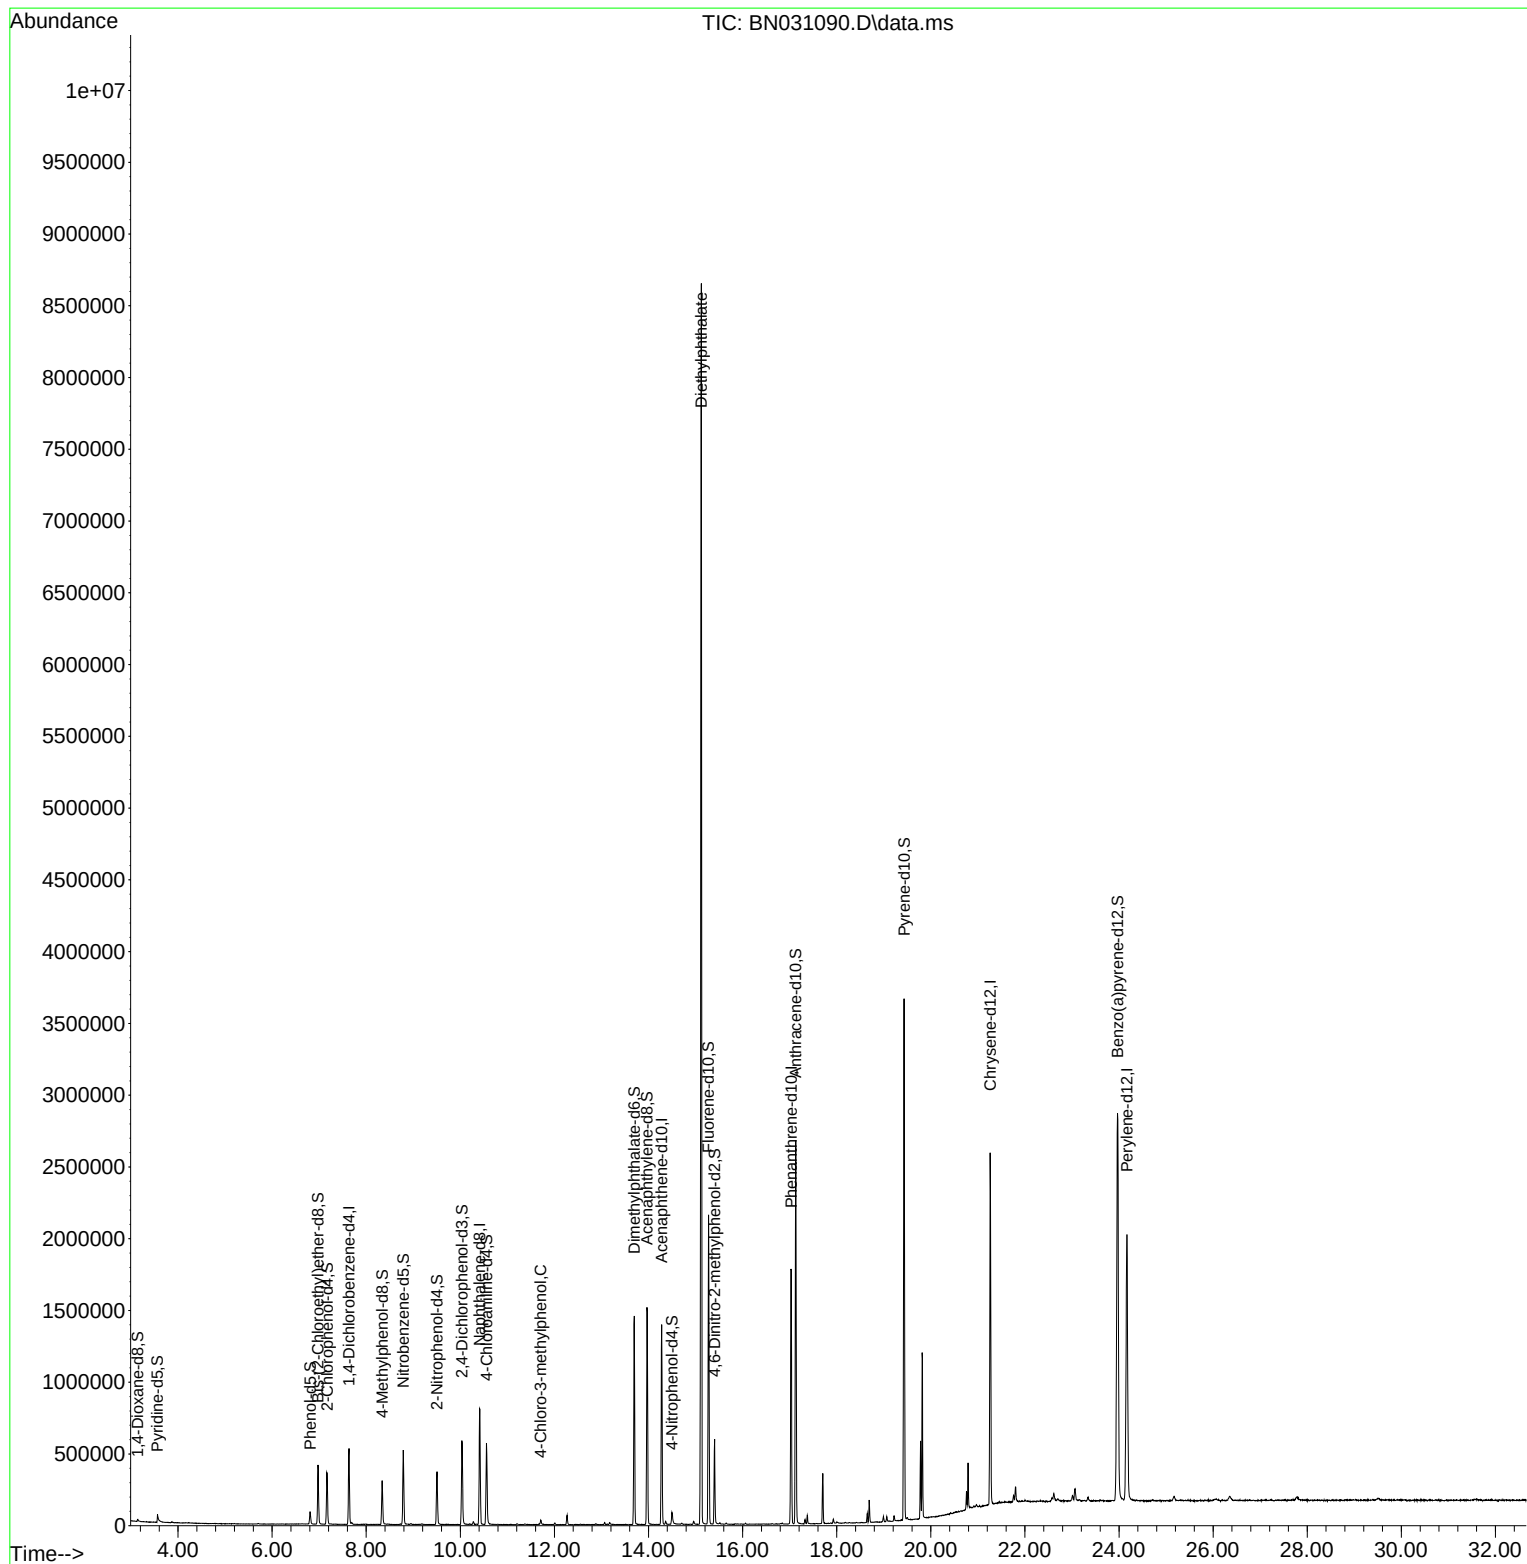


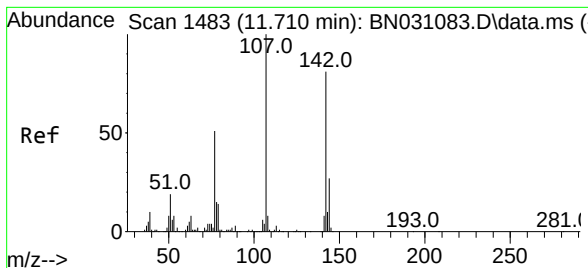

#35
4-Chloro-3-methylphenol
Concen: 1.055 ng/ul
RT: 11.710 min Scan# 1483
Delta R.T. -0.000 min
Lab File: BN031090.D
Acq: 21 Apr 2024 02:02

Instrument :
BNA_N
ClientSampleId :
COAL3

Tgt Ion:107 Resp: 12114
Ion Ratio Lower Upper
107 100
144 22.6 20.6 31.0
142 73.6 67.4 101.2

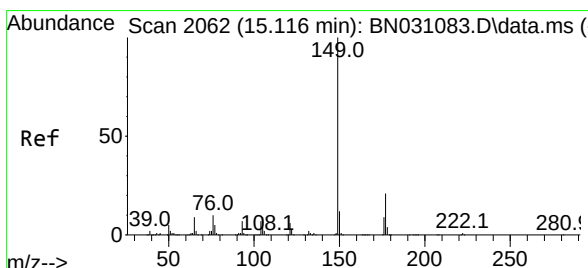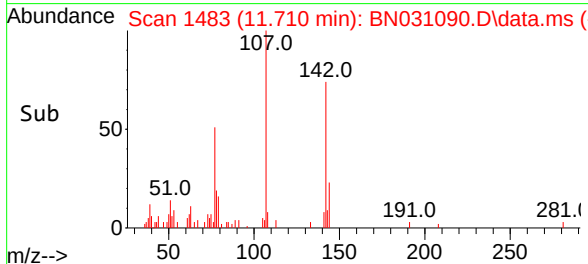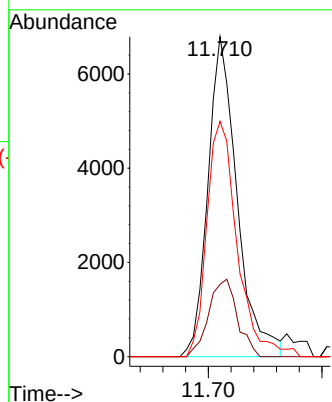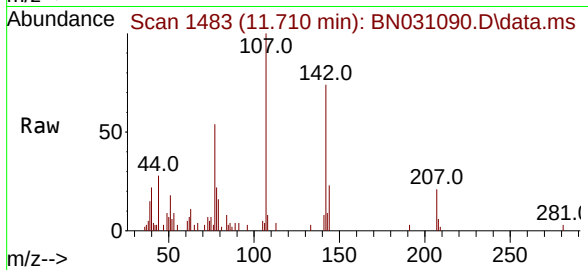

#59
Diethylphthalate
Concen: 153.090 ng/ul
RT: 15.122 min Scan# 2063
Delta R.T. 0.006 min
Lab File: BN031090.D
Acq: 21 Apr 2024 02:02

Tgt Ion:149 Resp: 5228748
Ion Ratio Lower Upper
149 100
177 21.3 16.8 25.2
150 12.7 10.1 15.1

