

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031091.D
 Acq On : 21 Apr 2024 02:41
 Operator : MA/JU
 Sample : P2077-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL4

Quant Time: Apr 21 14:18:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	130078	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	602114	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	426745	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	966847	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	1148300	20.000	ng/ul	0.00
88) Perylene-d12	24.162	264	1466446	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	9311	3.344	ng/uL	0.00
4) Pyridine-d5	3.564	84	40999	5.113	ng/ul	0.01
7) Phenol-d5	6.810	99	51623	4.705	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	168876	26.452	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132	167996	19.663	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	107968	11.700	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	116272	26.877	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	112949	25.117	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	213295	24.052	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	317420	22.905	ng/ul	0.00
46) Dimethylphthalate-d6	13.698	166	851734	28.682	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	942300	28.002	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	21095	3.403	ng/ul	0.00
60) Fluorene-d10	15.281	176	764174	29.560	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	93233	19.113	ng/ul	0.00
73) Anthracene-d10	17.128	188	1335959	31.879	ng/ul	0.00
81) Pyrene-d10	19.433	212	1752529	31.058	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2166868	31.160	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.710	107	10674	1.039	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031091.D
Acq On : 21 Apr 2024 02:41
Operator : MA/JU
Sample : P2077-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL4


Quant Time: Apr 21 14:18:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

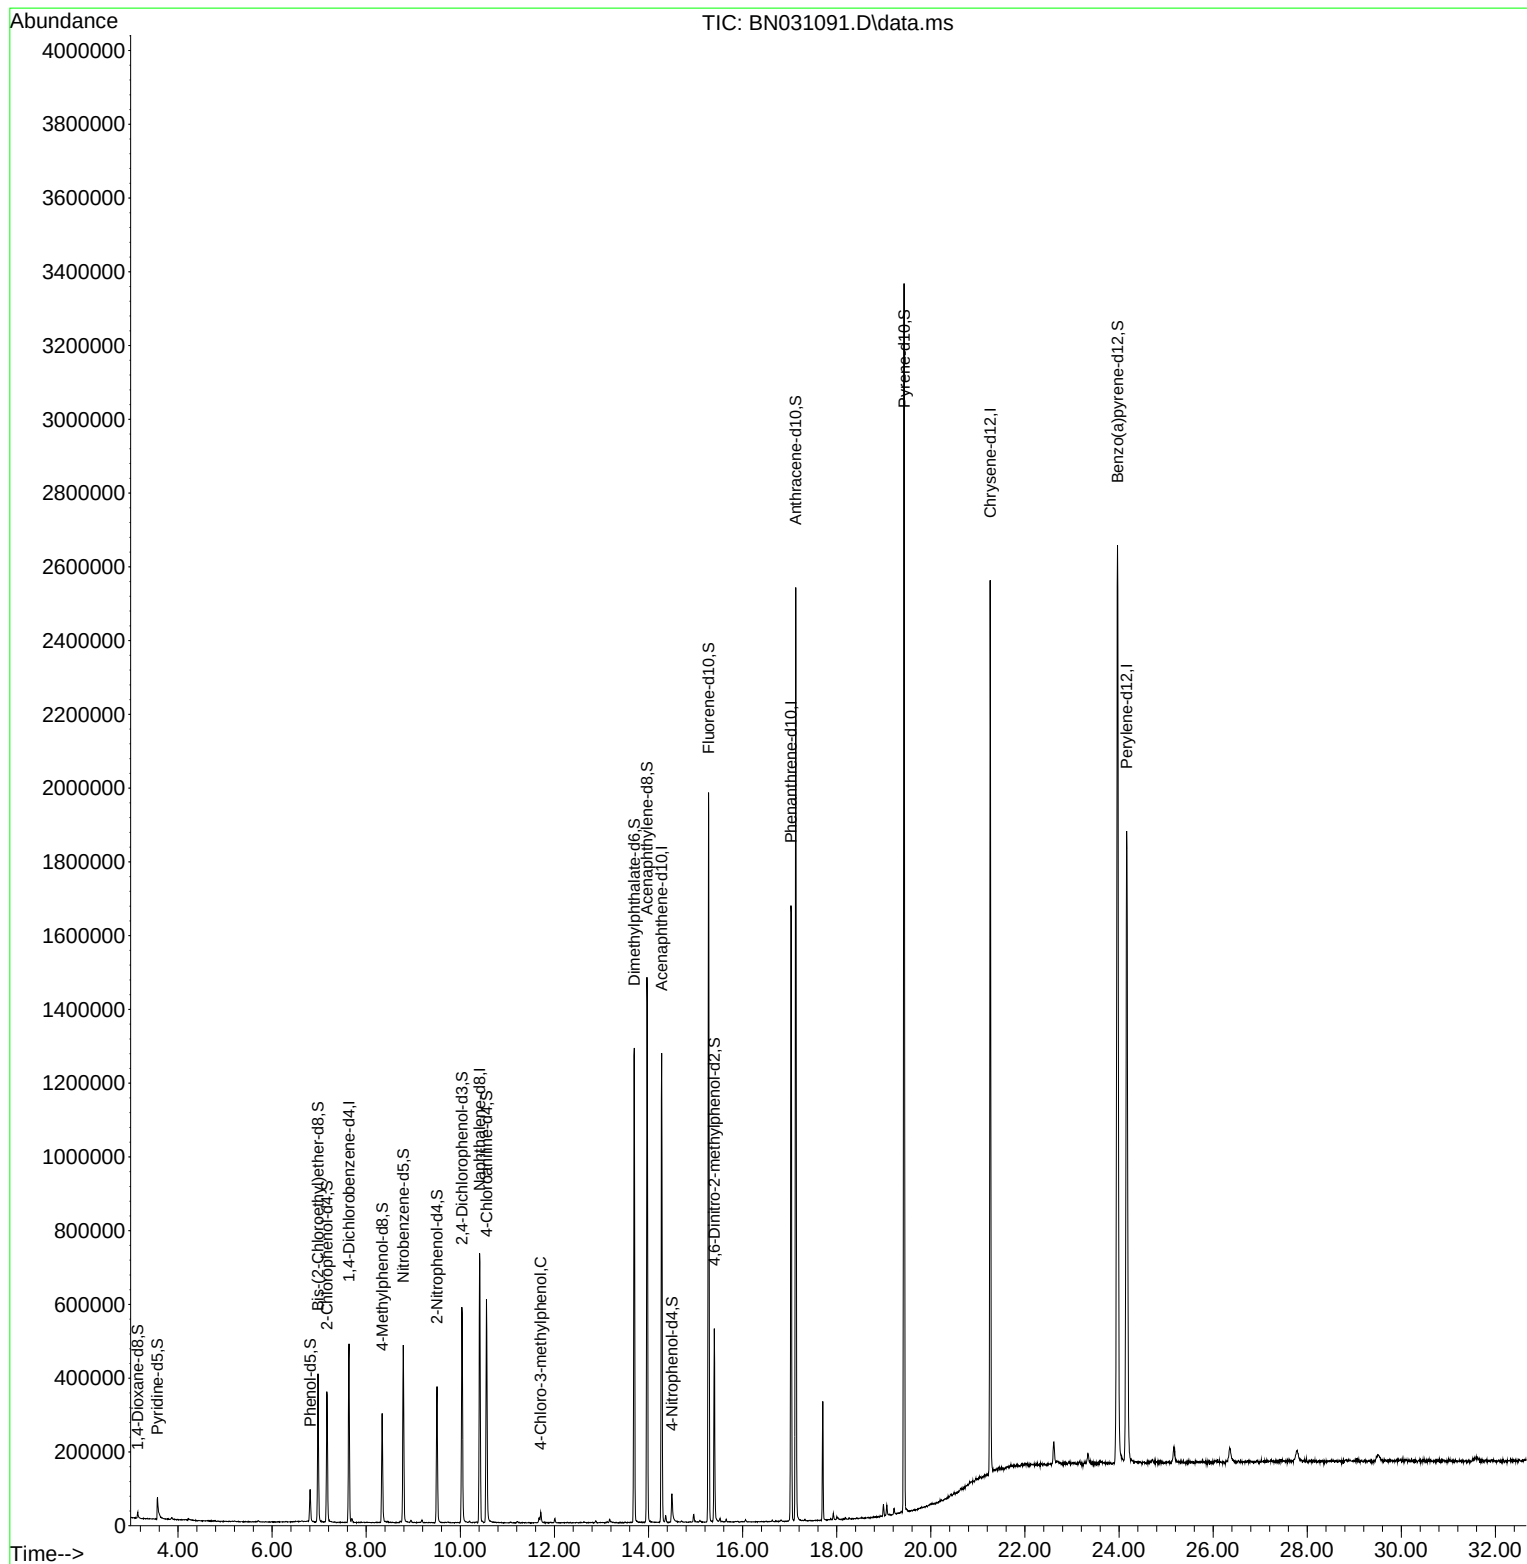

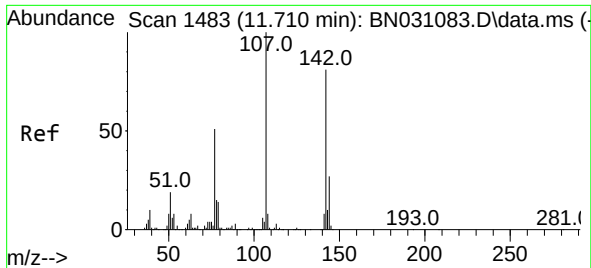

#35
 4-Chloro-3-methylphenol
 Concen: 1.039 ng/ul
 RT: 11.710 min Scan# 14
 Delta R.T. -0.000 min
 Lab File: BN031091.D
 Acq: 21 Apr 2024 02:41

Instrument :
 BNA_N
 ClientSampleId :
 C0AL4

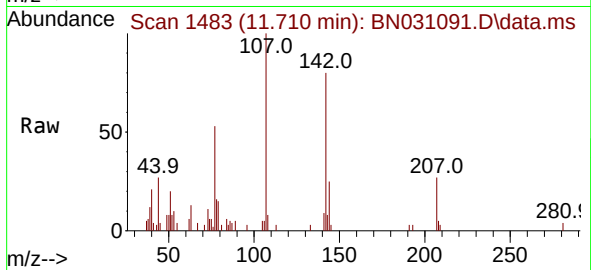

Tgt Ion:	107	Resp:	10674
Ion	Ratio	Lower	Upper
107	100		
144	24.9	20.6	31.0
142	80.2	67.4	101.2

