

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031108.D
 Acq On : 21 Apr 2024 14:28
 Operator : MA/JU
 Sample : P2161-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RJ9

Quant Time: Apr 21 22:20:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	123838	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	553128	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.281	164	371709	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	853213	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1031071	20.000	ng/u1	0.00
88) Perylene-d12	24.163	264	1310765	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	7442	2.808	ng/uL	0.00
4) Pyridine-d5	3.564	84	38679	5.067	ng/u1	0.01
7) Phenol-d5	6.805	99	28418	2.720	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	130461	21.465	ng/u1	0.00
11) 2-Chlorophenol-d4	7.164	132	109680	13.484	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	60532	6.890	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	84898	21.362	ng/u1	0.00
24) 2-Nitrophenol-d4	9.505	143	77835	18.841	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	142697	17.516	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	231609	18.193	ng/u1	0.00
46) Dimethylphthalate-d6	13.693	166	603651	23.337	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	638345	21.778	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	9152	1.695	ng/u1	0.00
60) Fluorene-d10	15.275	176	512343	22.753	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	53632	12.459	ng/u1	0.00
73) Anthracene-d10	17.128	188	870386	23.536	ng/u1	0.00
81) Pyrene-d10	19.428	212	1105534	21.820	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.963	264	1436356	23.108	ng/u1	-0.01
Target Compounds						
75) 1,2,3,4-Tetrachloroben...	13.063	216	28479	2.846	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031108.D
Acq On : 21 Apr 2024 14:28
Operator : MA/JU
Sample : P2161-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RJ9


Quant Time: Apr 21 22:20:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

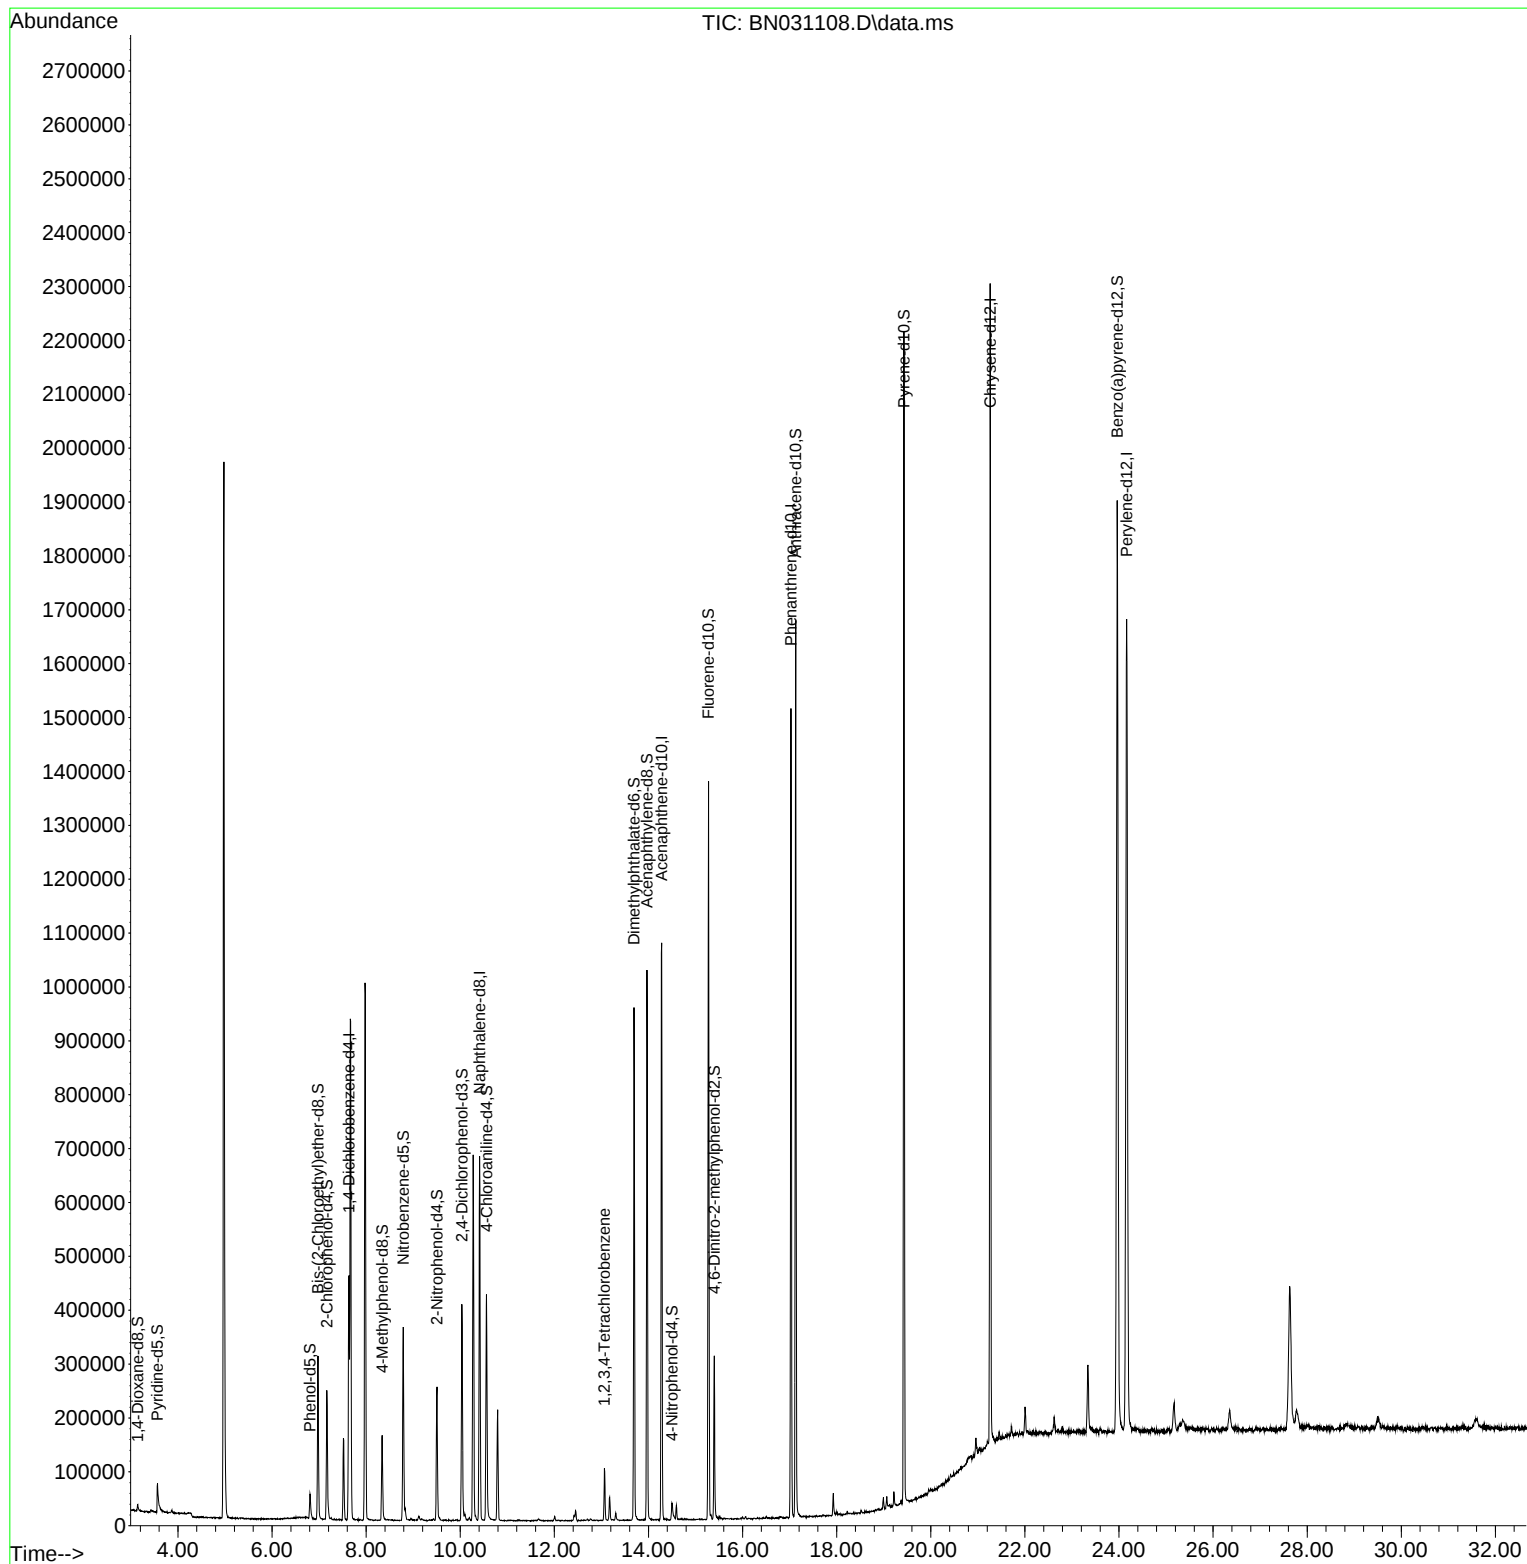

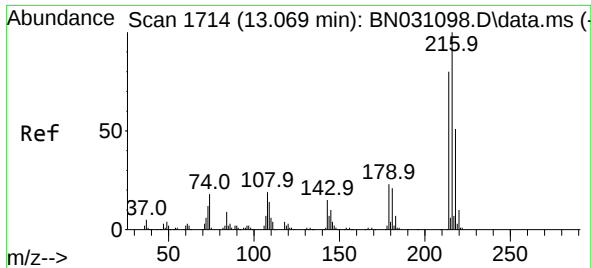

#75
 1,2,3,4-Tetrachlorobenzene
 Concen: 2.846 ng/uL
 RT: 13.063 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BN031108.D
 Acq: 21 Apr 2024 14:28

Instrument :
 BNA_N
 ClientSampleId :
 C0RJ9

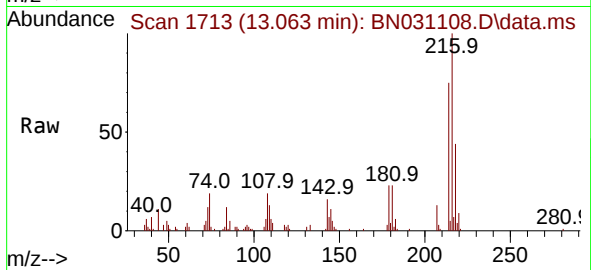

Tgt Ion:216 Resp: 28479
 Ion Ratio Lower Upper
 216 100
 214 75.3 63.0 94.6
 218 43.6 38.3 57.5

