

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031052.D
 Acq On : 19 Apr 2024 23:02
 Operator : MA/JU
 Sample : PB160366BL
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	32	rBV	21018	29626	0.59%	0.081%
2	3.552	94	96	120	rBV	200187	380135	7.61%	1.040%
3	6.810	644	650	663	rVB	424858	669873	13.42%	1.833%
4	6.981	673	679	690	rVB	346613	546000	10.94%	1.494%
5	7.169	704	711	722	rBV	432442	678692	13.59%	1.857%
6	7.634	784	790	800	rBV	400664	647191	12.96%	1.771%
7	8.340	903	910	923	rBV	550561	884755	17.72%	2.421%
8	8.793	980	987	1001	rBV	425379	693876	13.90%	1.899%
9	9.504	1101	1108	1118	rBV	331850	560351	11.22%	1.533%
10	10.040	1191	1199	1215	rBV	554872	911506	18.26%	2.494%
11	10.416	1255	1263	1274	rBV	623504	1030018	20.63%	2.818%
12	10.557	1279	1287	1298	rBV	404611	711694	14.26%	1.947%
13	12.010	1526	1534	1542	rBV2	9306	15604	0.31%	0.043%
14	13.181	1725	1733	1737	rBV3	8685	13808	0.28%	0.038%
15	13.698	1814	1821	1835	rBV	1125343	1541089	30.87%	4.217%
16	13.975	1862	1868	1879	rBV	1273430	1852264	37.10%	5.068%
17	14.281	1912	1920	1930	rBV	1063718	1540117	30.85%	4.214%
18	14.492	1950	1956	1977	rBV	481240	818515	16.40%	2.240%
19	15.281	2082	2090	2099	rBV	1675854	2361526	47.30%	6.462%
20	15.398	2104	2110	2123	rVV	462687	664739	13.32%	1.819%
21	15.516	2127	2130	2134	rVB4	6736	9191	0.18%	0.025%
22	16.069	2220	2224	2229	rVB3	6124	7601	0.15%	0.021%
23	17.033	2382	2388	2398	rBV	1412035	2017492	40.41%	5.520%
24	17.133	2398	2405	2422	rVB	1924620	2753862	55.16%	7.535%
25	18.539	2639	2644	2645	rBV5	9049	11359	0.23%	0.031%
26	18.574	2645	2650	2665	rVB5	14566	65221	1.31%	0.178%
27	18.998	2717	2722	2726	rBV2	29335	45697	0.92%	0.125%
28	19.069	2729	2734	2741	rVV	33753	65224	1.31%	0.178%
29	19.374	2782	2786	2790	rBV6	14439	27068	0.54%	0.074%
30	19.433	2790	2796	2813	rVB	2689640	3587462	71.86%	9.816%
31	21.263	3102	3107	3118	rBV	1923295	2791944	55.92%	7.640%
32	23.974	3558	3568	3583	rVB2	2073185	4992326	100.00%	13.660%
33	24.168	3592	3601	3618	rVB	1487224	3620274	72.52%	9.906%




Sum of corrected areas: 36546100

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031052.D
Acq On : 19 Apr 2024 23:02
Operator : MA/JU
Sample : PB160366BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

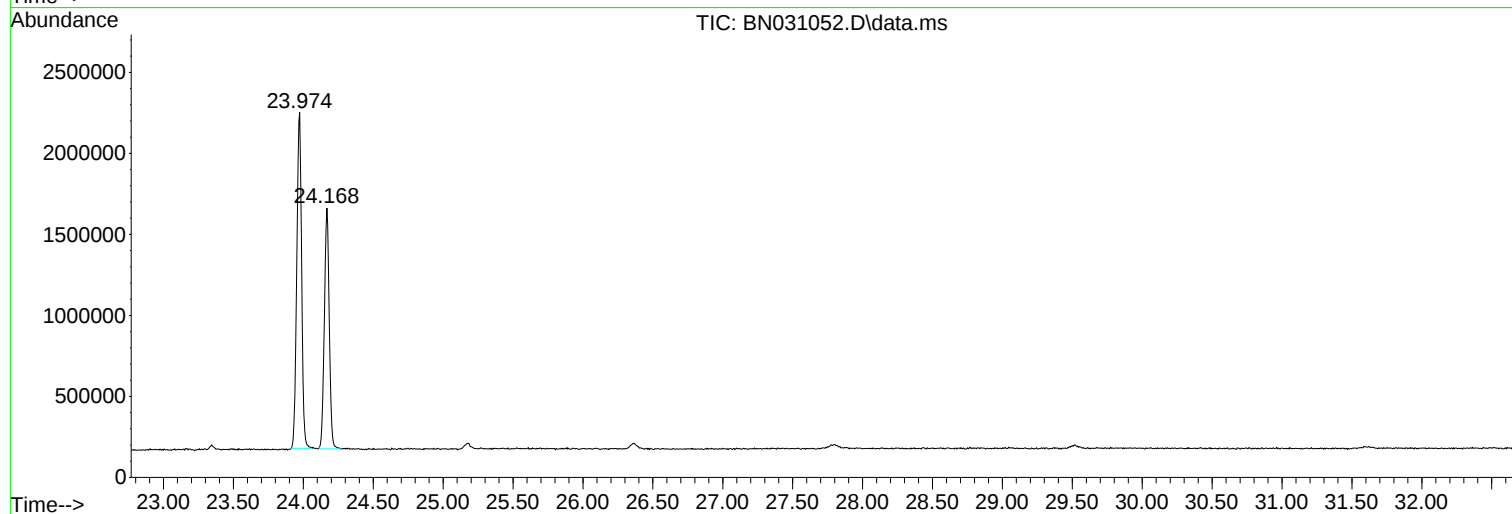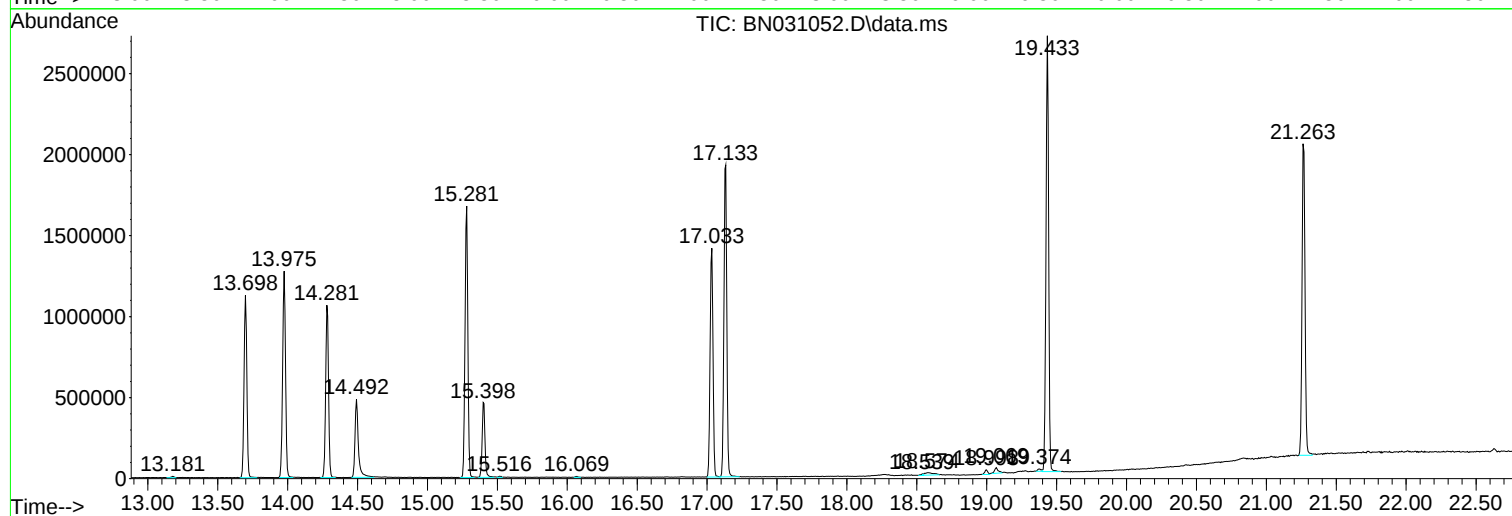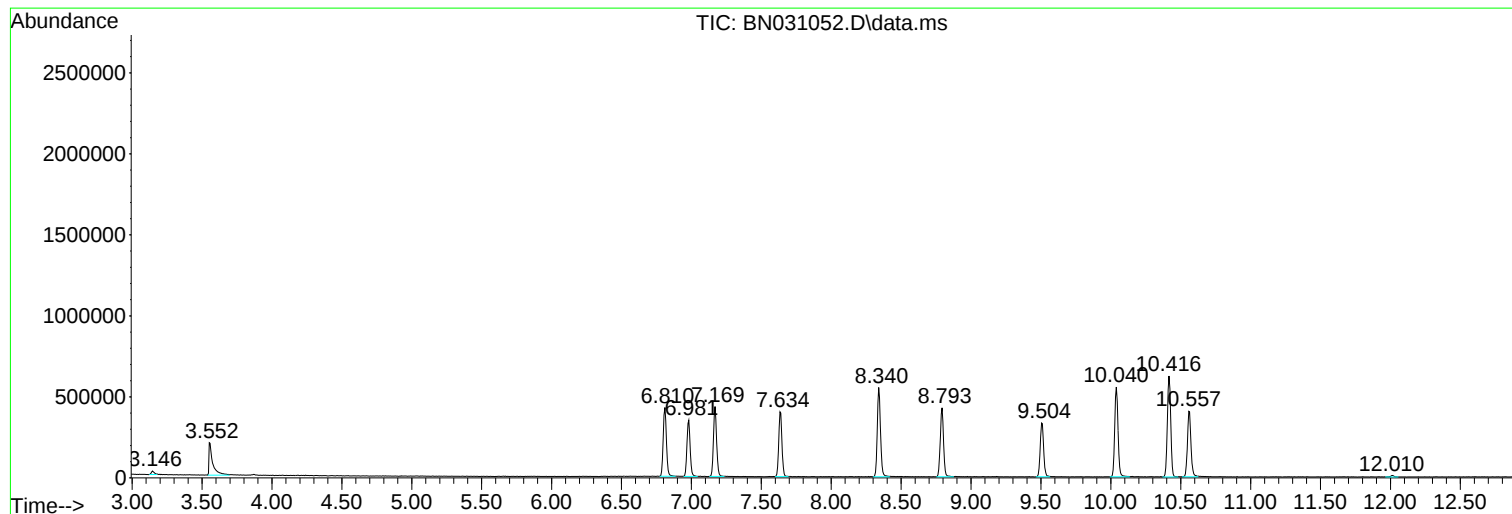

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031052.D
Acq On : 19 Apr 2024 23:02
Operator : MA/JU
Sample : PB160366BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031052.D
Acq On : 19 Apr 2024 23:02
Operator : MA/JU
Sample : PB160366BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------