

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031061.D
 Acq On : 20 Apr 2024 05:36
 Operator : MA/JU
 Sample : P2159-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	36	rVB2	19187	27823	0.45%	0.062%
2	3.558	95	97	114	rBV	116279	221857	3.56%	0.495%
3	3.864	146	149	154	rBV2	9451	15341	0.25%	0.034%
4	4.952	328	334	346	rVB	108932	196825	3.16%	0.440%
5	6.811	644	650	658	rVB	109734	174996	2.81%	0.391%
6	6.975	672	678	695	rBV	484665	779921	12.53%	1.742%
7	7.169	704	711	720	rBV	455389	719415	11.55%	1.607%
8	7.634	783	790	800	rBV	534043	832419	13.37%	1.859%
9	7.981	843	849	856	rBV5	6309	12183	0.20%	0.027%
10	8.340	904	910	923	rBV	329597	523443	8.41%	1.169%
11	8.787	979	986	995	rBV	586633	981001	15.75%	2.191%
12	9.187	1050	1054	1060	rVB2	6682	11095	0.18%	0.025%
13	9.363	1080	1084	1088	rBV6	3386	6261	0.10%	0.014%
14	9.505	1101	1108	1115	rBV	470478	762845	12.25%	1.704%
15	9.558	1115	1117	1127	rVV2	16267	27532	0.44%	0.061%
16	9.669	1130	1136	1143	rBV4	6848	15784	0.25%	0.035%
17	9.916	1168	1178	1183	rBV2	39013	85014	1.37%	0.190%
18	10.040	1191	1199	1214	rBV	707390	1178371	18.92%	2.632%
19	10.299	1235	1243	1250	rBV	34983	66215	1.06%	0.148%
20	10.416	1255	1263	1272	rVV	781127	1296101	20.81%	2.895%
21	10.557	1280	1287	1300	rBV	372676	657459	10.56%	1.468%
22	11.228	1393	1401	1409	rVB4	21224	46262	0.74%	0.103%
23	11.687	1473	1479	1485	rBV6	6971	12910	0.21%	0.029%
24	12.010	1528	1534	1538	rBV2	13650	23624	0.38%	0.053%
25	12.063	1538	1543	1554	rVV2	12450	27805	0.45%	0.062%
26	12.887	1677	1683	1688	rVB7	3332	7158	0.11%	0.016%
27	13.104	1716	1720	1723	rVB5	4914	6297	0.10%	0.014%
28	13.175	1727	1732	1739	rBV	14350	22485	0.36%	0.050%
29	13.698	1814	1821	1830	rBV	1574922	2100641	33.74%	4.692%
30	13.975	1858	1868	1879	rBV	1620404	2385160	38.30%	5.327%
31	14.281	1914	1920	1932	rVB	1286939	1872196	30.07%	4.181%
32	14.498	1951	1957	1971	rBV	98447	195958	3.15%	0.438%
33	14.651	1979	1983	1988	rBV4	12652	19524	0.31%	0.044%
34	14.716	1989	1994	1998	rVB8	8551	14155	0.23%	0.032%
35	14.845	2011	2016	2026	rVB2	24204	54505	0.88%	0.122%
36	15.093	2053	2058	2060	rBV4	5166	9134	0.15%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031061.D
 Acq On : 20 Apr 2024 05:36
 Operator : MA/JU
 Sample : P2159-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RC4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	15.140	2064	2066	2070	rVB4	6338	7245	0.12%	0.016%
38	15.281	2083	2090	2098	rBV	2295734	3284343	52.75%	7.335%
39	15.398	2105	2110	2123	rBV	506414	678752	10.90%	1.516%
40	15.516	2125	2130	2140	rVB8	10787	24089	0.39%	0.054%
41	16.004	2209	2213	2219	rVV3	11820	19740	0.32%	0.044%
42	16.063	2219	2223	2229	rVB5	10205	13471	0.22%	0.030%
43	16.534	2300	2303	2307	rBV	11821	15584	0.25%	0.035%
44	16.798	2344	2348	2354	rBV4	17024	27898	0.45%	0.062%
45	16.845	2354	2356	2361	rVB6	6862	8329	0.13%	0.019%
46	17.034	2381	2388	2397	rBV	1706026	2431502	39.05%	5.430%
47	17.128	2398	2404	2416	rVV2	2519332	3679509	59.09%	8.218%
48	17.322	2435	2437	2442	rVB4	5864	7715	0.12%	0.017%
49	17.428	2450	2455	2458	rBV6	4879	10149	0.16%	0.023%
50	17.534	2470	2473	2477	rVB2	14476	17340	0.28%	0.039%
51	17.928	2536	2540	2545	rBV	100717	139758	2.24%	0.312%
52	18.004	2551	2553	2556	rVB	8354	8123	0.13%	0.018%
53	18.228	2588	2591	2594	rBV4	14653	17854	0.29%	0.040%
54	18.263	2595	2597	2602	rVB6	8414	12070	0.19%	0.027%
55	18.363	2611	2614	2618	rBV6	12047	14765	0.24%	0.033%
56	18.416	2618	2623	2631	rBV4	36997	63015	1.01%	0.141%
57	18.869	2697	2700	2704	rBV5	13084	16257	0.26%	0.036%
58	18.998	2718	2722	2727	rVB	40995	54279	0.87%	0.121%
59	19.063	2730	2733	2738	rBV	39861	56470	0.91%	0.126%
60	19.222	2756	2760	2766	rBV2	63282	78542	1.26%	0.175%
61	19.433	2790	2796	2804	rBV	3785131	4899554	78.69%	10.943%
62	20.957	3051	3055	3063	rBV3	75374	137608	2.21%	0.307%
63	21.263	3102	3107	3114	rBV	2309626	3295083	52.92%	7.359%
64	23.974	3558	3568	3589	rVB	2589773	6226766	100.00%	13.907%
65	24.169	3592	3601	3615	rVB	1728236	4139574	66.48%	9.245%




Sum of corrected areas: 44775099

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031061.D
Acq On : 20 Apr 2024 05:36
Operator : MA/JU
Sample : P2159-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

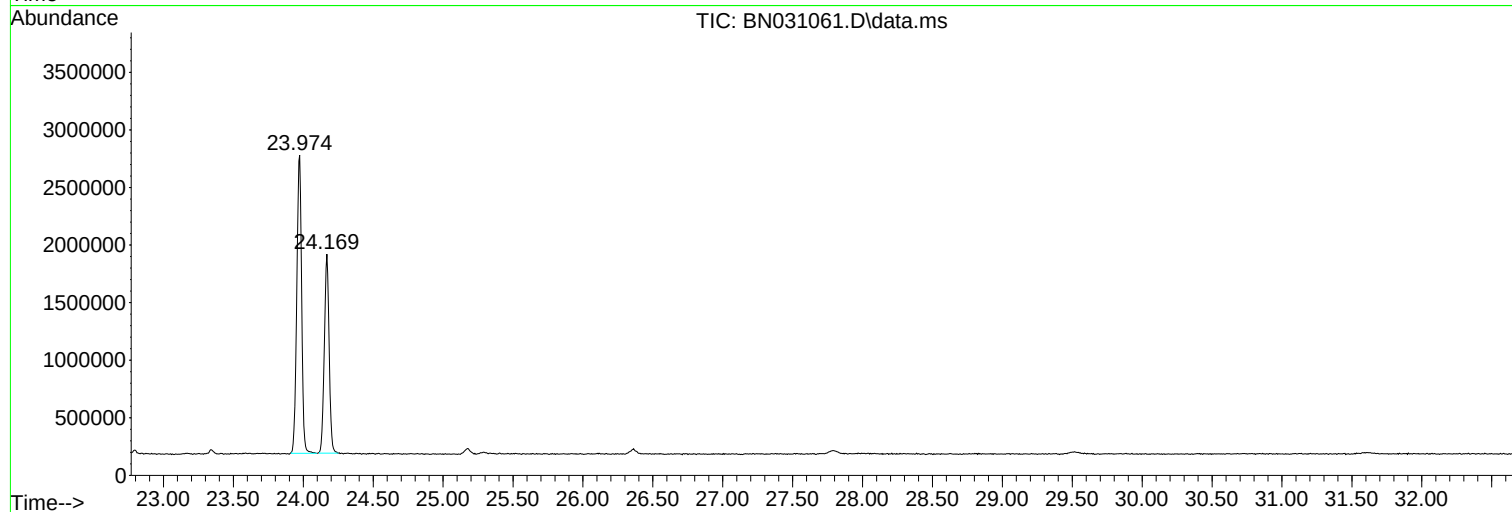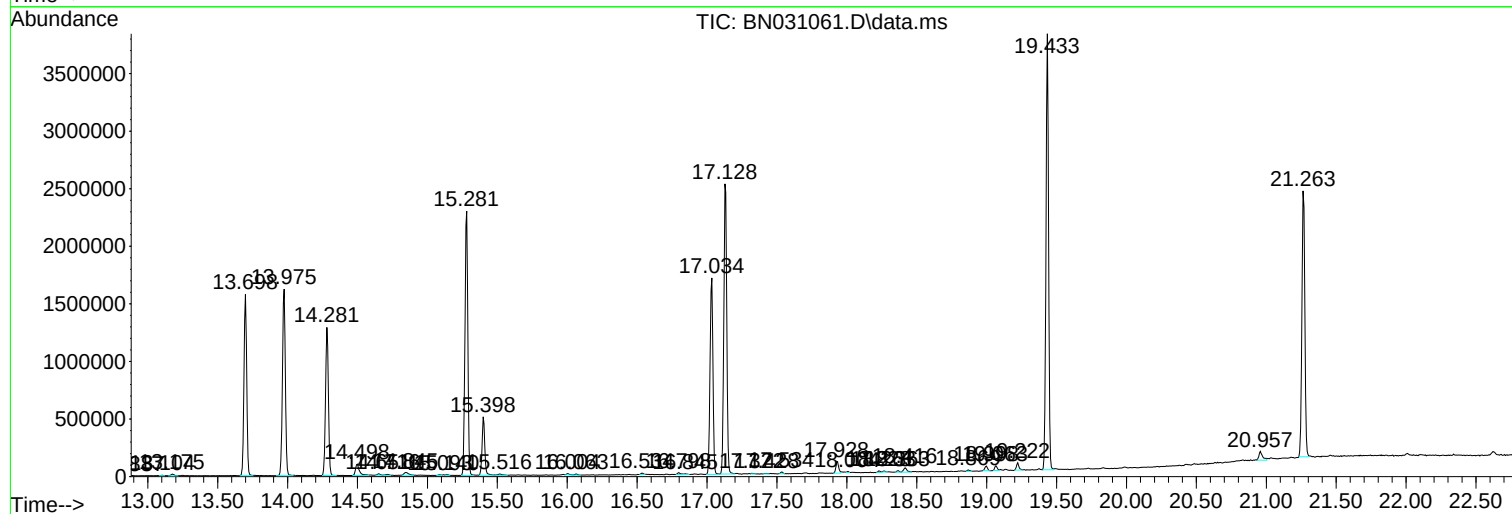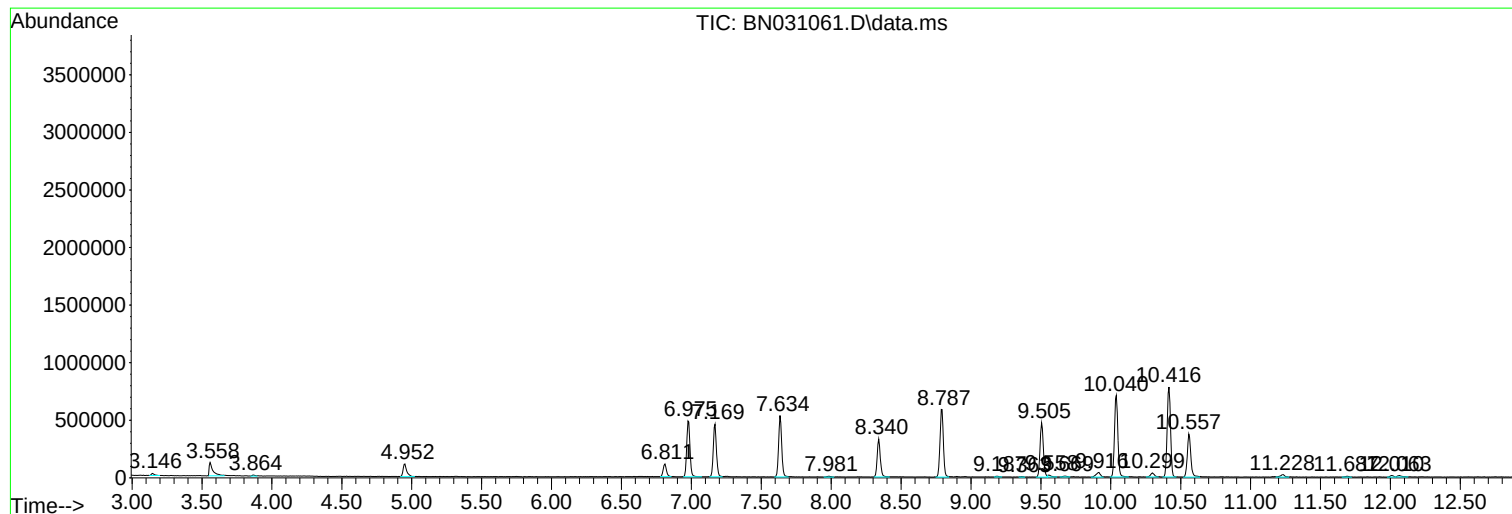

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031061.D
Acq On : 20 Apr 2024 05:36
Operator : MA/JU
Sample : P2159-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RC4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclohexene, 1-chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.952	4.73 ng/ul	196825	1,4-Dichlorobenzene-d4	7.634

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexene, 1-chloro-	116	C6H9Cl	000930-66-5	72
2			.alpha.-Bromo-p-tolunitrile	195	C8H6BrN	017201-43-3	28
3			Pyrimidine,2,4-difluoro-	116	C4H2F2N2	002802-61-1	9
4			Indene	116	C9H8	000095-13-6	9
5			4-Imidazolidinone, 2-thioxo-	116	C3H4N2OS	000503-87-7	9

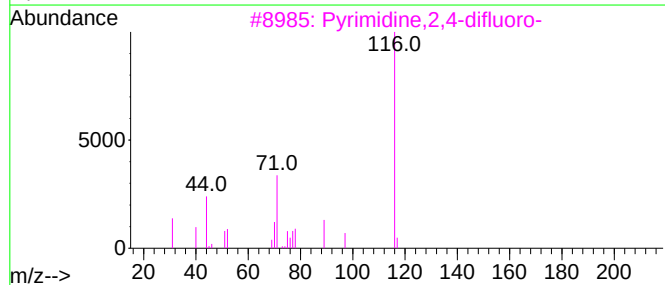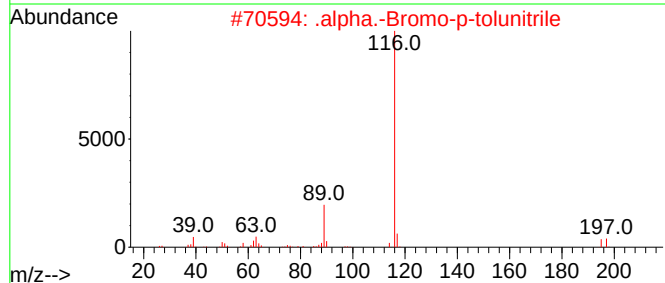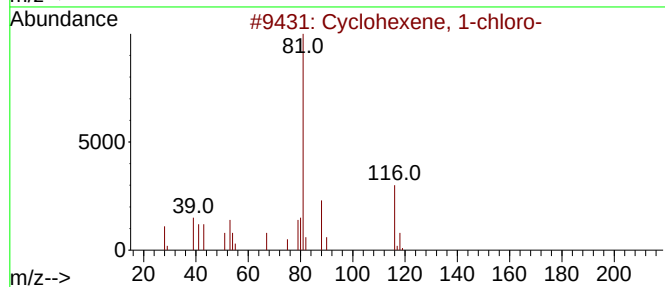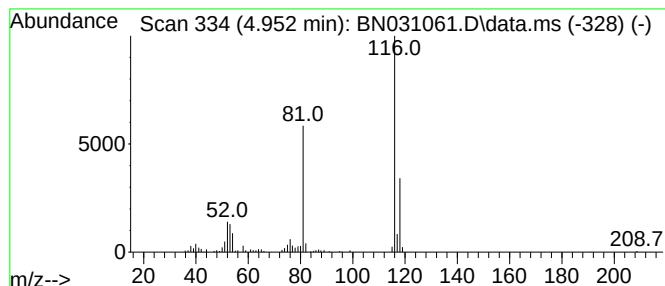

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031061.D
Acq On : 20 Apr 2024 05:36
Operator : MA/JU
Sample : P2159-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclohexene, 1-...	4.952	4.7	ng/u1	196825	1	7.634	832419	20.0