

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031063.D
 Acq On : 20 Apr 2024 06:55
 Operator : MA/JU
 Sample : P2159-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	33	rBV2	15498	23641	0.38%	0.056%
2	3.558	94	97	116	rBV	93656	173778	2.79%	0.414%
3	3.864	146	149	155	rVB3	5760	9155	0.15%	0.022%
4	6.811	645	650	659	rVB	75909	124440	2.00%	0.297%
5	6.975	672	678	690	rVB	399253	637835	10.23%	1.520%
6	7.169	704	711	721	rBV	346636	550008	8.82%	1.311%
7	7.634	783	790	799	rBV	480819	752439	12.07%	1.793%
8	8.340	903	910	919	rBV	269968	419853	6.73%	1.001%
9	8.787	978	986	996	rBV	489990	814943	13.07%	1.942%
10	9.505	1101	1108	1115	rBV	368472	598119	9.59%	1.426%
11	10.040	1192	1199	1212	rBV	553911	941883	15.11%	2.245%
12	10.416	1256	1263	1272	rBV	724244	1207900	19.37%	2.879%
13	10.557	1280	1287	1303	rBV	502511	849997	13.63%	2.026%
14	11.169	1386	1391	1396	rBV4	5070	9806	0.16%	0.023%
15	12.010	1528	1534	1538	rVB3	10853	16799	0.27%	0.040%
16	12.422	1598	1604	1608	rBV2	10147	17238	0.28%	0.041%
17	13.069	1710	1714	1718	rBV4	6418	9333	0.15%	0.022%
18	13.175	1726	1732	1738	rVB4	9744	16974	0.27%	0.040%
19	13.698	1811	1821	1826	rBV	1360804	1906441	30.58%	4.544%
20	13.740	1826	1828	1834	rVB3	34980	49461	0.79%	0.118%
21	13.975	1861	1868	1881	rVB	1505425	2185076	35.05%	5.208%
22	14.157	1896	1899	1904	rBV3	6833	9660	0.15%	0.023%
23	14.281	1914	1920	1932	rBV	1244813	1794824	28.79%	4.278%
24	14.504	1949	1958	1969	rBV2	394523	899115	14.42%	2.143%
25	14.598	1969	1974	1980	rVB	31048	47552	0.76%	0.113%
26	15.275	2083	2089	2099	rBV	1933775	2856427	45.82%	6.808%
27	15.398	2104	2110	2119	rBV	537614	732218	11.74%	1.745%
28	15.522	2127	2131	2136	rVB3	9167	15157	0.24%	0.036%
29	15.663	2152	2155	2159	rBV5	7423	9659	0.15%	0.023%
30	15.992	2203	2211	2219	rVV5	3646	10232	0.16%	0.024%
31	16.063	2219	2223	2228	rVB7	8654	13408	0.22%	0.032%
32	17.034	2382	2388	2397	rBV	1639145	2322816	37.26%	5.536%
33	17.134	2398	2405	2416	rVV	2451366	3510792	56.31%	8.368%
34	17.439	2450	2457	2463	rBV7	12900	25330	0.41%	0.060%
35	17.639	2486	2491	2493	rBV4	4545	7989	0.13%	0.019%
36	17.710	2499	2503	2505	rBV5	6789	8938	0.14%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031063.D
Acq On : 20 Apr 2024 06:55
Operator : MA/JU
Sample : P2159-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	17.734	2505	2507	2513	rVB5	6759	9069	0.15%	0.022%
38	17.928	2536	2540	2549	rBV	38024	56010	0.90%	0.133%
39	18.004	2549	2553	2557	rVB6	4594	7576	0.12%	0.018%
40	18.363	2611	2614	2619	rBV6	7225	9698	0.16%	0.023%
41	18.522	2638	2641	2644	rVB4	11588	13008	0.21%	0.031%
42	18.892	2700	2704	2709	rVB8	13624	16940	0.27%	0.040%
43	18.992	2716	2721	2726	rBV2	36237	54573	0.88%	0.130%
44	19.063	2729	2733	2737	rVV2	30967	40615	0.65%	0.097%
45	19.222	2756	2760	2765	rBV3	22640	31962	0.51%	0.076%
46	19.369	2783	2785	2789	rVB5	10090	10054	0.16%	0.024%
47	19.433	2790	2796	2803	rBV	3466593	4566267	73.24%	10.883%
48	21.263	3101	3107	3115	rBV	2302909	3253573	52.19%	7.755%
49	23.969	3558	3567	3581	rVB2	2670449	6234506	100.00%	14.859%
50	24.169	3591	3601	3612	rBV	1635560	4073951	65.35%	9.710%




Sum of corrected areas: 41957038

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031063.D
Acq On : 20 Apr 2024 06:55
Operator : MA/JU
Sample : P2159-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

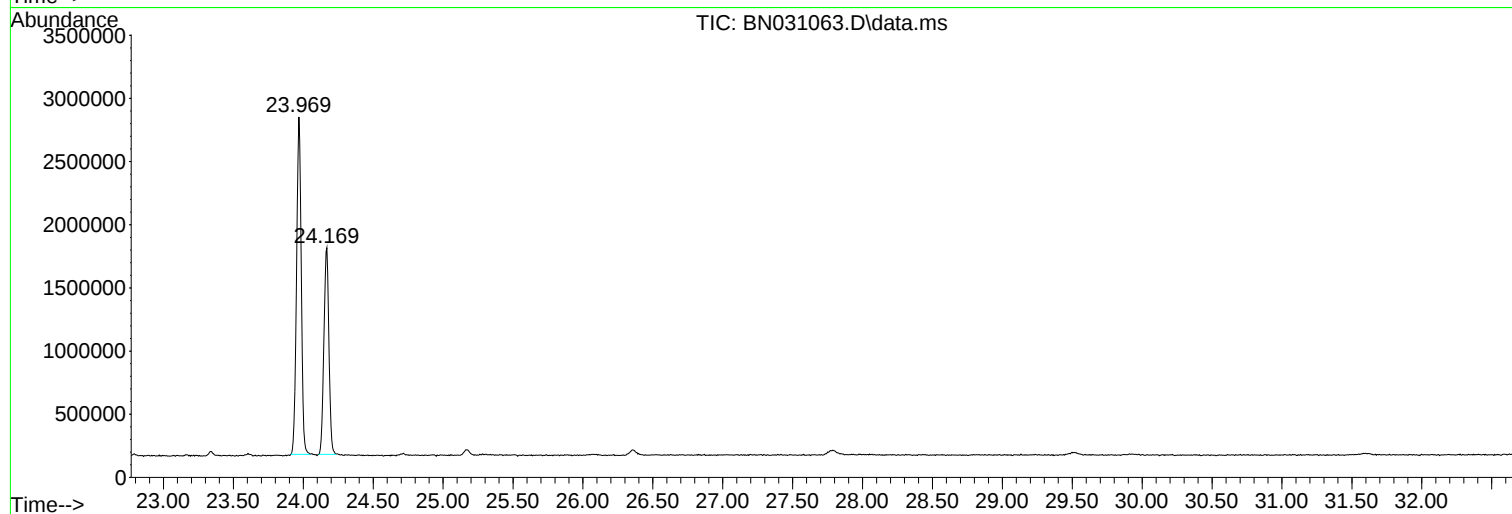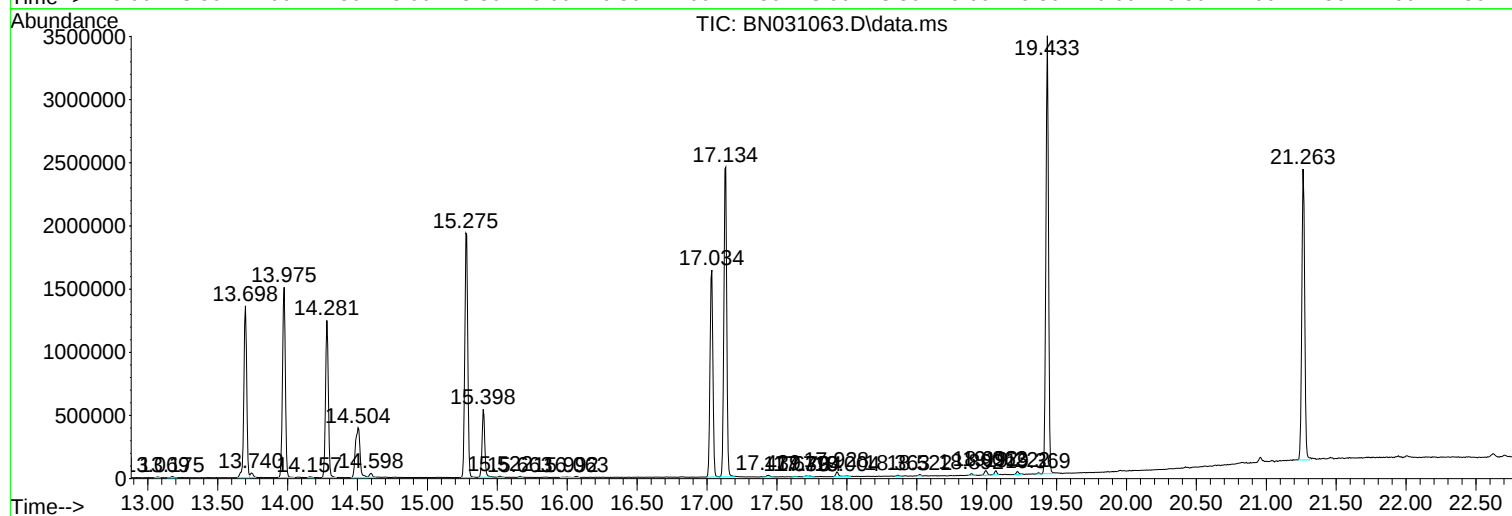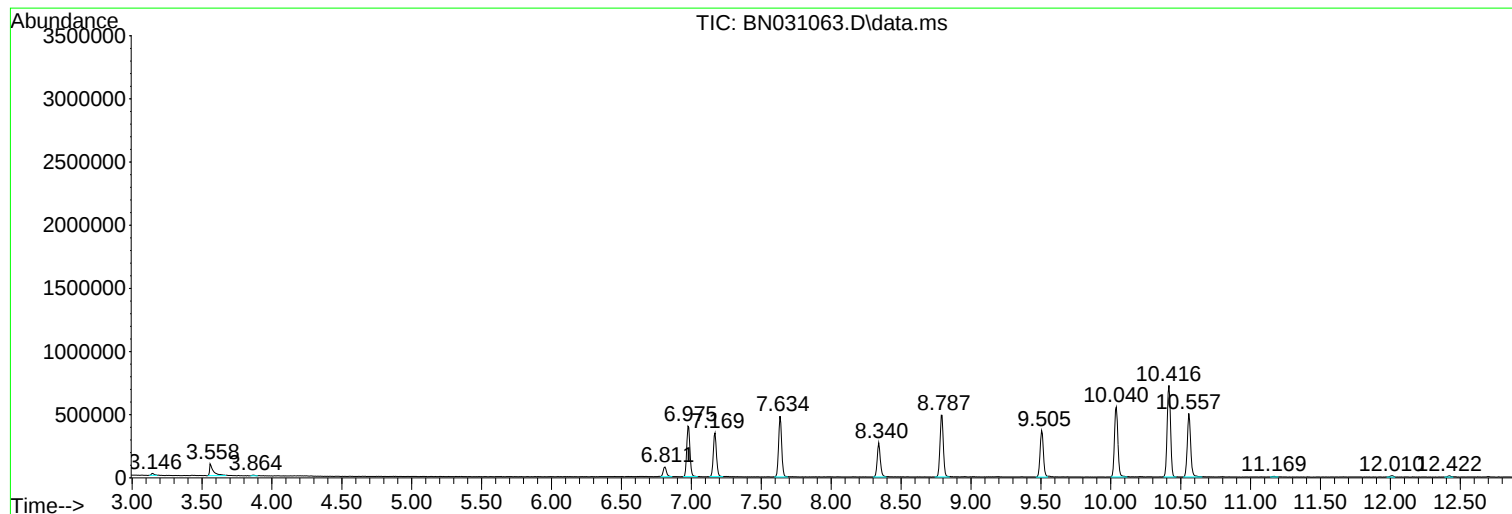

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031063.D
Acq On : 20 Apr 2024 06:55
Operator : MA/JU
Sample : P2159-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031063.D
Acq On : 20 Apr 2024 06:55
Operator : MA/JU
Sample : P2159-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc