

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031065.D
 Acq On : 20 Apr 2024 08:14
 Operator : MA/JU
 Sample : P2159-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	32	rVB	16054	20213	0.27%	0.040%
2	3.558	96	97	109	rBV	99445	166857	2.24%	0.330%
3	3.869	146	150	153	rBV2	7227	9014	0.12%	0.018%
4	6.810	645	650	658	rVB	121877	197183	2.64%	0.390%
5	6.975	672	678	693	rVB	547921	870361	11.66%	1.721%
6	7.169	704	711	721	rBV	508796	812400	10.89%	1.606%
7	7.634	783	790	798	rBV	554167	867774	11.63%	1.716%
8	8.340	903	910	919	rBV	412597	650376	8.72%	1.286%
9	8.793	979	987	1002	rBV	667634	1103178	14.78%	2.181%
10	9.504	1101	1108	1116	rBV	529781	853343	11.44%	1.687%
11	10.040	1190	1199	1213	rBV	782673	1331303	17.84%	2.632%
12	10.416	1255	1263	1273	rBV	846915	1383370	18.54%	2.735%
13	10.557	1280	1287	1303	rBV	495974	853954	11.44%	1.688%
14	12.010	1529	1534	1540	rVB2	15789	25358	0.34%	0.050%
15	12.422	1599	1604	1607	rBV2	14743	22301	0.30%	0.044%
16	12.704	1646	1652	1657	rBV5	5141	8349	0.11%	0.017%
17	13.069	1709	1714	1719	rBV2	8319	11449	0.15%	0.023%
18	13.175	1726	1732	1737	rBV2	16183	25958	0.35%	0.051%
19	13.698	1810	1821	1826	rBV	1807843	2516010	33.72%	4.974%
20	13.740	1826	1828	1835	rVB	51293	72697	0.97%	0.144%
21	13.975	1860	1868	1878	rBV2	1963345	2921159	39.14%	5.775%
22	14.081	1882	1886	1890	rVV6	4967	7587	0.10%	0.015%
23	14.157	1894	1899	1905	rBV3	7695	11177	0.15%	0.022%
24	14.281	1914	1920	1932	rBV	1420841	2035922	27.28%	4.025%
25	14.492	1949	1956	1970	rBV	129070	246868	3.31%	0.488%
26	14.598	1970	1974	1978	rVB	37431	52554	0.70%	0.104%
27	15.281	2080	2090	2104	rBV	2592510	3745243	50.19%	7.404%
28	15.398	2104	2110	2120	rBV	800113	1060396	14.21%	2.096%
29	15.516	2126	2130	2134	rVB	12002	17169	0.23%	0.034%
30	15.663	2151	2155	2162	rVB9	10695	16945	0.23%	0.034%
31	16.063	2219	2223	2230	rVB4	11012	16112	0.22%	0.032%
32	17.033	2381	2388	2398	rBV	1848295	2670273	35.78%	5.279%
33	17.128	2398	2404	2416	rVV2	3009472	4420896	59.24%	8.740%
34	17.439	2452	2457	2462	rVB6	12457	17145	0.23%	0.034%
35	17.622	2484	2488	2495	rBV7	11128	19115	0.26%	0.038%
36	17.733	2504	2507	2512	rVB5	11340	13946	0.19%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031065.D
 Acq On : 20 Apr 2024 08:14
 Operator : MA/JU
 Sample : P2159-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	17.928	2536	2540	2548	rBV2	42534	59961	0.80%	0.119%
38	17.998	2548	2552	2557	rVB5	4449	9009	0.12%	0.018%
39	18.522	2636	2641	2645	rVB7	12405	16977	0.23%	0.034%
40	18.992	2717	2721	2726	rBV2	45924	62615	0.84%	0.124%
41	19.063	2729	2733	2737	rBV	42742	61939	0.83%	0.122%
42	19.222	2756	2760	2764	rBV4	24840	32007	0.43%	0.063%
43	19.433	2790	2796	2802	rBV2	4159138	5654357	75.77%	11.179%
44	19.957	2882	2885	2889	rBV6	10726	17431	0.23%	0.034%
45	20.963	3052	3056	3060	rBV6	32371	57960	0.78%	0.115%
46	21.263	3101	3107	3116	rBV2	2408651	3615561	48.45%	7.148%
47	23.974	3558	3568	3583	rVB2	3050498	7462515	100.00%	14.753%
48	24.168	3592	3601	3616	rVB	1824112	4457468	59.73%	8.812%




Sum of corrected areas: 50581755

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031065.D
Acq On : 20 Apr 2024 08:14
Operator : MA/JU
Sample : P2159-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

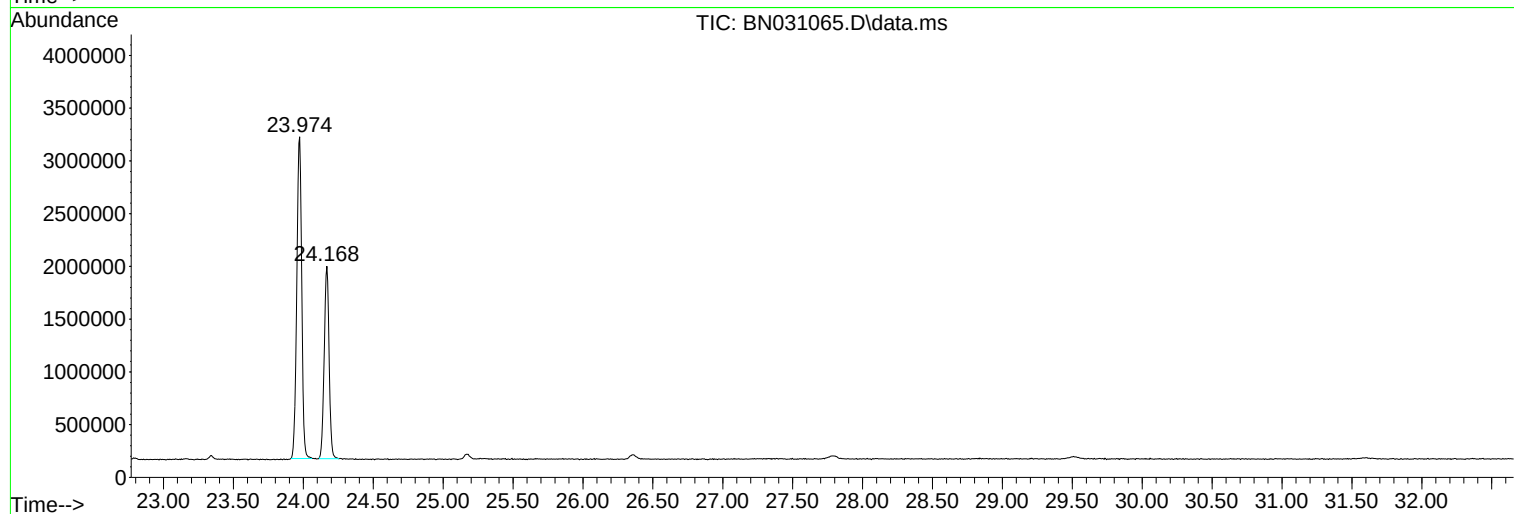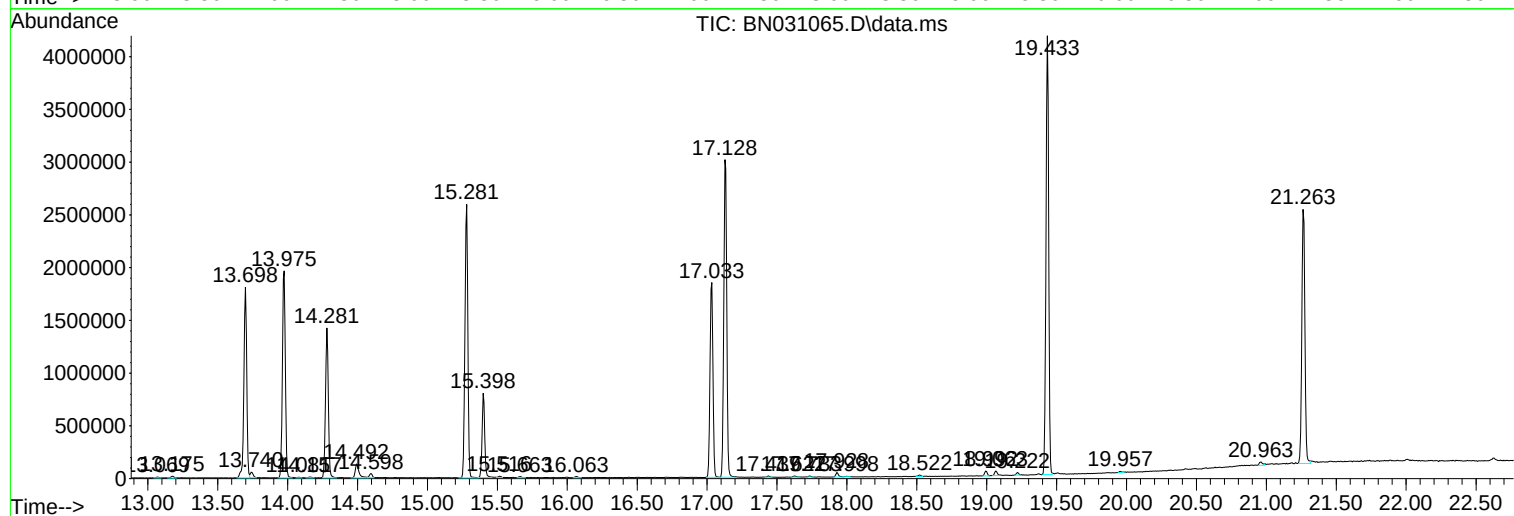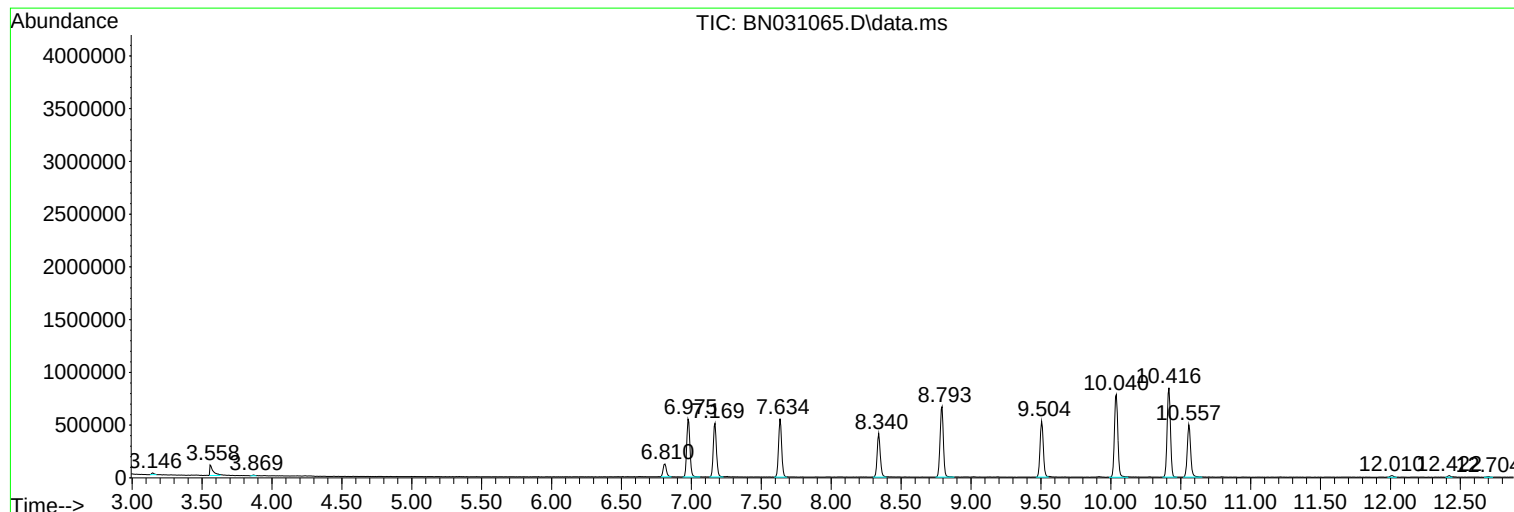

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031065.D
Acq On : 20 Apr 2024 08:14
Operator : MA/JU
Sample : P2159-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031065.D
Acq On : 20 Apr 2024 08:14
Operator : MA/JU
Sample : P2159-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc