

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031067.D
 Acq On : 20 Apr 2024 09:33
 Operator : MA/JU
 Sample : P2159-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	35	rVB2	15103	22787	0.37%	0.058%
2	3.423	72	74	78	rBV3	5551	8748	0.14%	0.022%
3	3.564	96	98	107	rBV	44723	75747	1.23%	0.192%
4	6.811	643	650	662	rVB	77813	132229	2.14%	0.334%
5	6.975	671	678	694	rBV	397580	632154	10.24%	1.599%
6	7.169	704	711	720	rBV	351025	558044	9.04%	1.411%
7	7.634	783	790	799	rBV	448264	703917	11.41%	1.780%
8	8.340	903	910	923	rBV	270874	436886	7.08%	1.105%
9	8.787	979	986	1000	rBV	471231	788733	12.78%	1.994%
10	9.181	1050	1053	1060	rVB5	5371	8697	0.14%	0.022%
11	9.363	1078	1084	1090	rVB7	6486	13815	0.22%	0.035%
12	9.505	1102	1108	1116	rBV	364437	588010	9.53%	1.487%
13	10.040	1190	1199	1211	rBV	547681	925717	15.00%	2.341%
14	10.416	1255	1263	1271	rVB	664777	1106352	17.93%	2.798%
15	10.558	1279	1287	1304	rBV	485258	842626	13.65%	2.131%
16	11.163	1384	1390	1396	rBV	16147	29644	0.48%	0.075%
17	12.010	1528	1534	1542	rBV	11290	18851	0.31%	0.048%
18	12.104	1545	1550	1557	rVB6	4474	8116	0.13%	0.021%
19	13.093	1710	1718	1726	rBV4	19509	33499	0.54%	0.085%
20	13.175	1726	1732	1736	rBV3	9328	14188	0.23%	0.036%
21	13.293	1747	1752	1761	rVB	12740	20769	0.34%	0.053%
22	13.699	1814	1821	1829	rBV	1229892	1708753	27.69%	4.321%
23	13.975	1857	1868	1877	rBV	1419339	2120117	34.36%	5.361%
24	14.281	1913	1920	1929	rBV	1184303	1621020	26.27%	4.099%
25	14.498	1951	1957	1969	rBV2	65940	136337	2.21%	0.345%
26	14.840	2011	2015	2024	rVB2	8258	19121	0.31%	0.048%
27	15.275	2083	2089	2104	rBV	1879170	2705196	43.84%	6.841%
28	15.398	2104	2110	2123	rVV	501254	671691	10.88%	1.698%
29	15.516	2128	2130	2135	rVB4	8474	9407	0.15%	0.024%
30	16.063	2220	2223	2227	rVB5	6122	8143	0.13%	0.021%
31	17.028	2379	2387	2397	rBV	1489058	2136781	34.63%	5.403%
32	17.128	2397	2404	2415	rBV2	2335788	3281309	53.17%	8.297%
33	17.710	2499	2503	2507	rVB3	14255	17450	0.28%	0.044%
34	17.928	2535	2540	2549	rBV	98295	147073	2.38%	0.372%
35	18.992	2717	2721	2728	rVB2	32093	43578	0.71%	0.110%
36	19.063	2729	2733	2737	rBV	33462	44574	0.72%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031067.D
Acq On : 20 Apr 2024 09:33
Operator : MA/JU
Sample : P2159-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	19.222	2756	2760	2769	rBV2	52221	78271	1.27%	0.198%
38	19.434	2790	2796	2804	rBV	3242006	4285221	69.44%	10.836%
39	20.957	3051	3055	3066	rBV2	104889	198288	3.21%	0.501%
40	21.263	3101	3107	3121	rBV2	2130818	3143430	50.94%	7.949%
41	23.969	3558	3567	3586	rVB2	2652686	6170878	100.00%	15.604%
42	24.169	3592	3601	3618	rVB	1659482	4030389	65.31%	10.192%




Sum of corrected areas: 39546556

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031067.D
Acq On : 20 Apr 2024 09:33
Operator : MA/JU
Sample : P2159-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

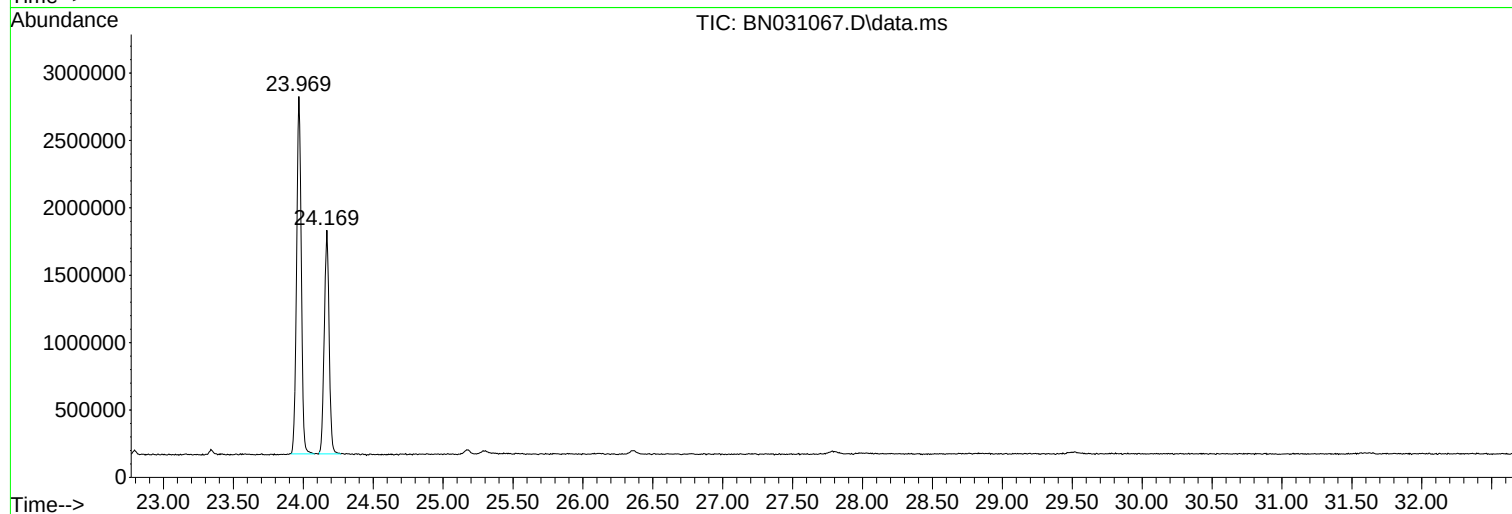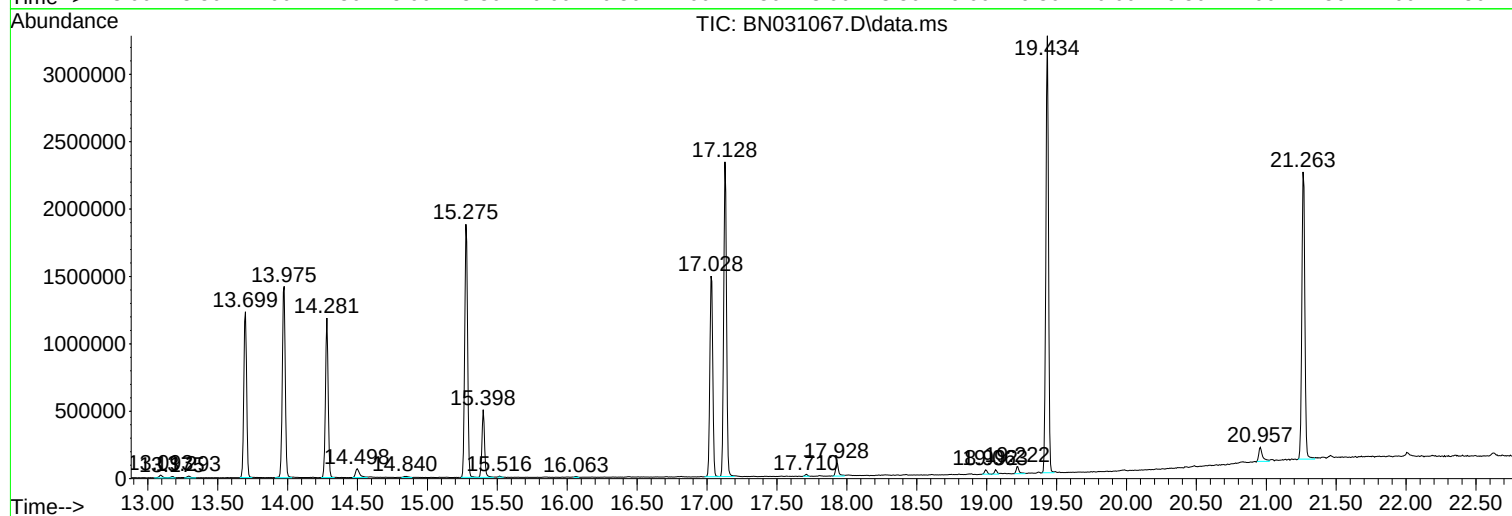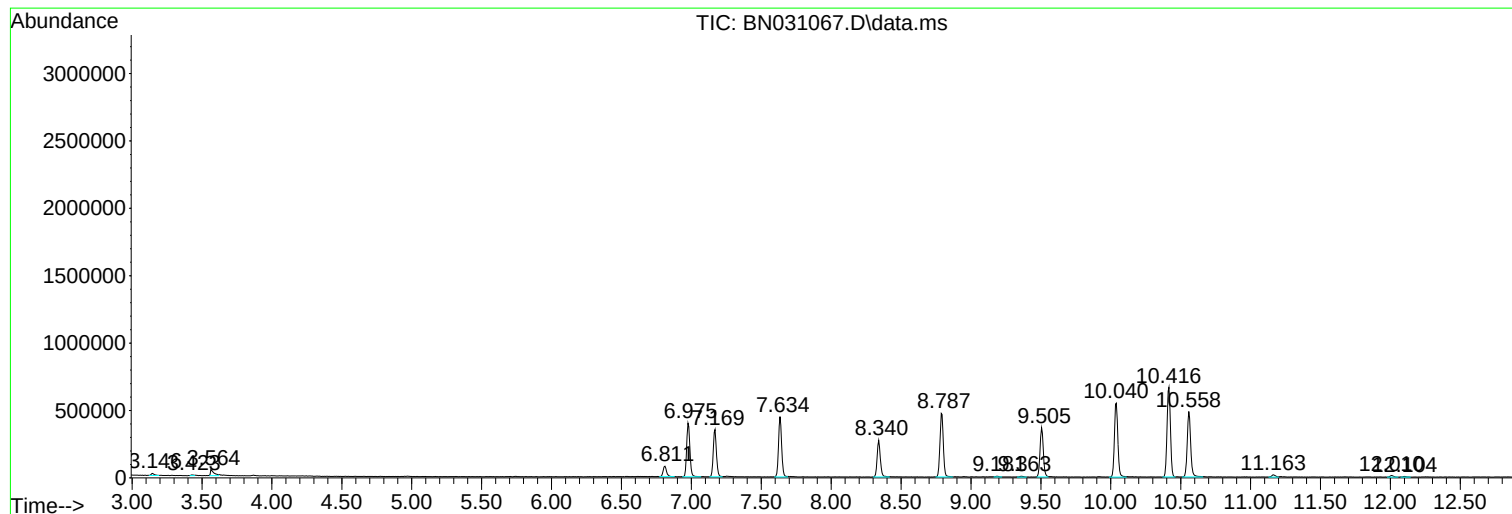

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031067.D
Acq On : 20 Apr 2024 09:33
Operator : MA/JU
Sample : P2159-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031067.D
Acq On : 20 Apr 2024 09:33
Operator : MA/JU
Sample : P2159-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc