

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031085.D
 Acq On : 20 Apr 2024 22:43
 Operator : MA/JU
 Sample : PB160290BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK290

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	32	rBV	22494	29505	0.58%	0.077%
2	3.552	93	96	116	rBV	319952	570676	11.26%	1.483%
3	3.869	146	150	153	rBV4	4618	5946	0.12%	0.015%
4	6.811	643	650	665	rVB	451138	729170	14.39%	1.895%
5	6.975	671	678	688	rBV	368425	594763	11.73%	1.546%
6	7.169	703	711	723	rBV	456891	729571	14.39%	1.896%
7	7.634	783	790	806	rBV	408228	643113	12.69%	1.671%
8	8.340	903	910	924	rBV	607726	959040	18.92%	2.492%
9	8.787	980	986	997	rBV	448363	743562	14.67%	1.932%
10	9.504	1100	1108	1119	rBV	357982	589892	11.64%	1.533%
11	10.040	1191	1199	1212	rBV	607079	1020077	20.12%	2.651%
12	10.416	1255	1263	1273	rBV	632892	1043774	20.59%	2.712%
13	10.557	1279	1287	1300	rBV	657889	1109556	21.89%	2.883%
14	12.010	1526	1534	1542	rVB2	9111	17544	0.35%	0.046%
15	13.175	1727	1732	1737	rVB6	7156	12028	0.24%	0.031%
16	13.698	1814	1821	1828	rBV	1220967	1667483	32.90%	4.333%
17	13.975	1861	1868	1879	rBV	1344935	1997477	39.41%	5.191%
18	14.281	1912	1920	1930	rBV	1103637	1572602	31.02%	4.086%
19	14.492	1949	1956	1980	rBV	534480	908735	17.93%	2.361%
20	15.275	2083	2089	2097	rBV	1754363	2561254	50.53%	6.656%
21	15.398	2104	2110	2120	rBV	478765	650177	12.83%	1.690%
22	15.516	2127	2130	2135	rVB3	8074	10165	0.20%	0.026%
23	16.063	2219	2223	2229	rVB4	5715	8506	0.17%	0.022%
24	16.816	2345	2351	2353	rBV5	2879	5313	0.10%	0.014%
25	17.034	2381	2388	2394	rBV	1458759	2054408	40.53%	5.338%
26	17.128	2398	2404	2420	rVV	2123029	3012844	59.44%	7.829%
27	18.275	2594	2599	2602	rBV7	4161	8258	0.16%	0.021%
28	18.992	2717	2721	2726	rVB3	26065	35085	0.69%	0.091%
29	19.063	2729	2733	2738	rVB	23173	30605	0.60%	0.080%
30	19.222	2757	2760	2764	rBV6	4762	8312	0.16%	0.022%
31	19.433	2790	2796	2804	rBV	2828103	3908495	77.11%	10.156%
32	21.263	3101	3107	3117	rBV	1874768	2783943	54.92%	7.234%
33	23.968	3558	3567	3580	rVB2	2196633	5068922	100.00%	13.172%
34	24.163	3592	3600	3615	rVB	1378052	3392075	66.92%	8.815%

Sum of corrected areas: 38482876

Instrument :

BNA_N

ClientSampleId :




SBLK290

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031085.D
Acq On : 20 Apr 2024 22:43
Operator : MA/JU
Sample : PB160290BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK290

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

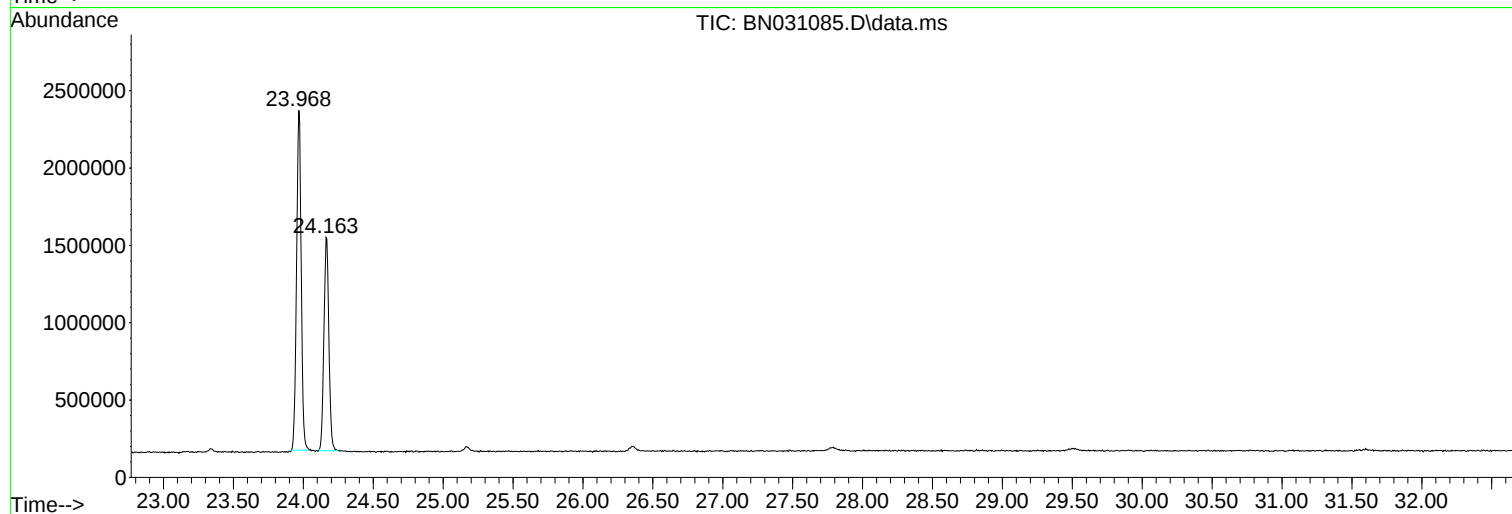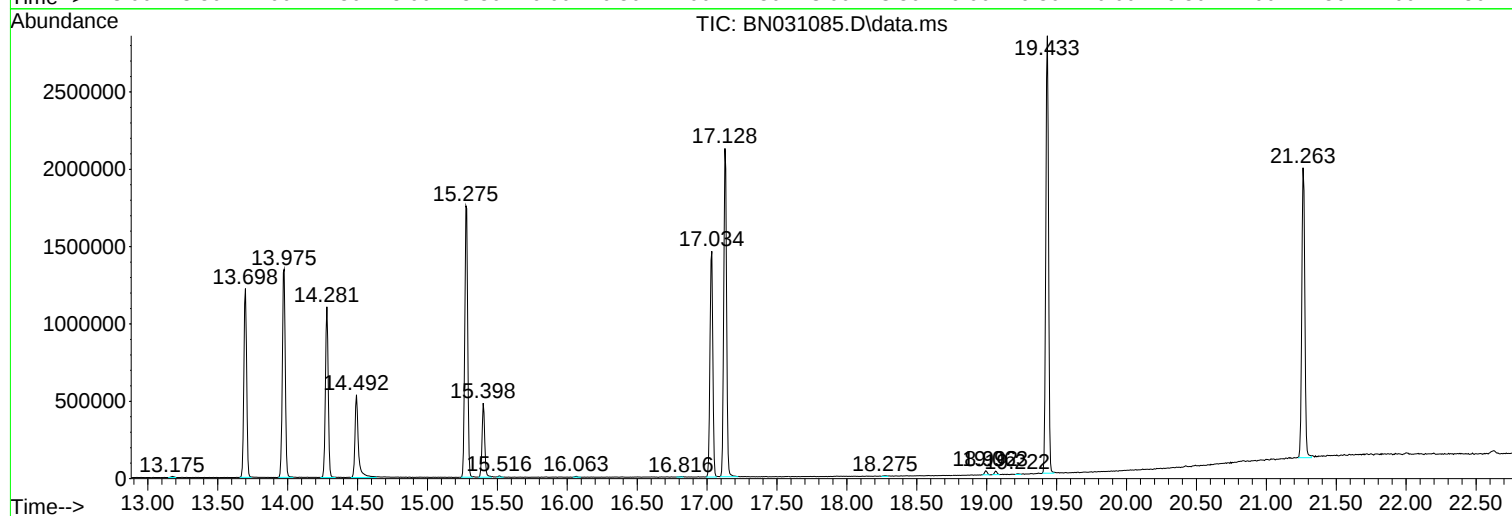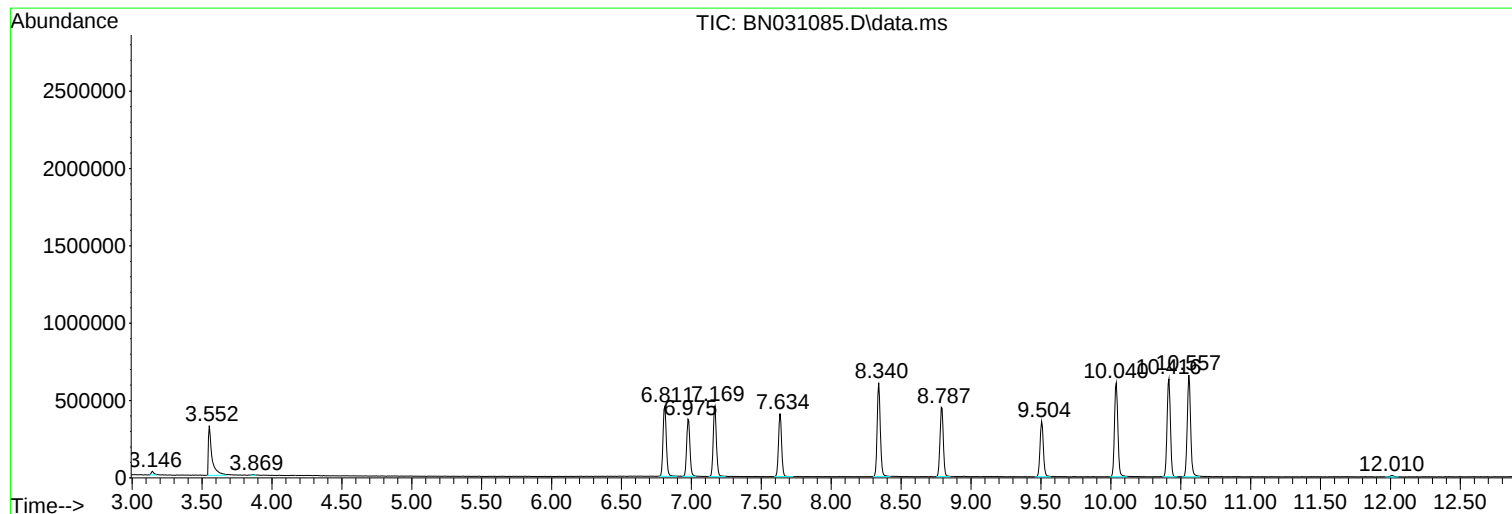

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031085.D
Acq On : 20 Apr 2024 22:43
Operator : MA/JU
Sample : PB160290BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK290

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031085.D
Acq On : 20 Apr 2024 22:43
Operator : MA/JU
Sample : PB160290BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK290

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc