

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031087.D
 Acq On : 21 Apr 2024 00:03
 Operator : MA/JU
 Sample : P2077-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	35	rVB	19778	28591	0.42%	0.057%
2	3.564	96	98	117	rBV	63339	129849	1.93%	0.257%
3	3.864	146	149	159	rVB5	8823	18467	0.27%	0.037%
4	6.763	636	642	645	rBV	21224	31506	0.47%	0.062%
5	6.810	645	650	659	rVB	134173	219722	3.26%	0.436%
6	6.975	672	678	692	rBV	501139	787220	11.69%	1.561%
7	7.169	704	711	721	rBV	473715	759258	11.28%	1.506%
8	7.634	782	790	798	rBV	675950	1067567	15.86%	2.117%
9	7.716	799	804	811	rVB3	9012	18075	0.27%	0.036%
10	8.340	904	910	924	rBV	420232	661008	9.82%	1.311%
11	8.787	979	986	995	rBV	601231	987657	14.67%	1.959%
12	9.187	1048	1054	1060	rVB	144402	210452	3.13%	0.417%
13	9.504	1100	1108	1119	rBV	478514	757447	11.25%	1.502%
14	9.634	1126	1130	1135	rBV2	7231	12960	0.19%	0.026%
15	9.693	1137	1140	1144	rVB2	6134	7949	0.12%	0.016%
16	9.904	1170	1176	1180	rBV7	3500	7370	0.11%	0.015%
17	10.034	1191	1198	1213	rBV	739737	1259890	18.72%	2.498%
18	10.416	1255	1263	1272	rVB	991486	1692611	25.14%	3.356%
19	10.557	1280	1287	1305	rVB	168301	307302	4.57%	0.609%
20	10.951	1351	1354	1359	rBV3	5128	8380	0.12%	0.017%
21	11.393	1426	1429	1435	rVB6	3958	7817	0.12%	0.016%
22	11.675	1470	1477	1483	rBV2	47862	74365	1.10%	0.147%
23	12.004	1529	1533	1541	rVB2	13520	22197	0.33%	0.044%
24	13.175	1727	1732	1737	rBV3	11594	18285	0.27%	0.036%
25	13.451	1772	1779	1784	rBV3	9202	15055	0.22%	0.030%
26	13.504	1784	1788	1793	rVV2	11611	16598	0.25%	0.033%
27	13.557	1793	1797	1801	rVB3	4960	7294	0.11%	0.014%
28	13.698	1812	1821	1832	rBV	1688592	2270077	33.72%	4.502%
29	13.969	1860	1867	1878	rBV	1765534	2645003	39.29%	5.245%
30	14.281	1913	1920	1928	rBV	1735162	2464555	36.61%	4.887%
31	14.492	1950	1956	1969	rBV	133491	255574	3.80%	0.507%
32	14.651	1979	1983	1988	rVV7	3934	6762	0.10%	0.013%
33	14.698	1988	1991	1999	rVB8	5356	9886	0.15%	0.020%
34	15.275	2083	2089	2102	rVB	2397641	3495763	51.93%	6.932%
35	15.398	2104	2110	2125	rBV	713732	972816	14.45%	1.929%
36	15.516	2125	2130	2138	rVB2	11100	18755	0.28%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031087.D
 Acq On : 21 Apr 2024 00:03
 Operator : MA/JU
 Sample : P2077-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	16.063	2218	2223	2227	rBV3	13030	19021	0.28%	0.038%
38	16.110	2227	2231	2237	rVV7	4018	8948	0.13%	0.018%
39	16.169	2237	2241	2246	rVB5	6778	9686	0.14%	0.019%
40	16.957	2371	2375	2379	rBV5	7616	9173	0.14%	0.018%
41	17.033	2381	2388	2398	rBV	2210540	3167398	47.05%	6.281%
42	17.128	2398	2404	2417	rVV	2851422	4078672	60.59%	8.088%
43	17.927	2536	2540	2546	rBV2	120199	167464	2.49%	0.332%
44	18.263	2593	2597	2607	rBV3	17565	31652	0.47%	0.063%
45	18.416	2620	2623	2630	rVB5	13698	20070	0.30%	0.040%
46	18.804	2685	2689	2690	rBV3	7122	7772	0.12%	0.015%
47	18.992	2717	2721	2726	rVB3	41600	56163	0.83%	0.111%
48	19.063	2729	2733	2738	rBV2	46792	66784	0.99%	0.132%
49	19.222	2755	2760	2766	rBV3	51221	76586	1.14%	0.152%
50	19.374	2782	2786	2789	rBV4	10318	10814	0.16%	0.021%
51	19.433	2790	2796	2805	rBV	3992597	5426025	80.60%	10.760%
52	20.957	3051	3055	3064	rBV3	97891	179945	2.67%	0.357%
53	21.263	3101	3107	3118	rBV	2824355	4177007	62.05%	8.283%
54	23.968	3558	3567	3583	rBV2	2793906	6731687	100.00%	13.349%
55	24.168	3592	3601	3614	rVB	1978330	4909277	72.93%	9.735%




Sum of corrected areas: 50428227

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031087.D
Acq On : 21 Apr 2024 00:03
Operator : MA/JU
Sample : P2077-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

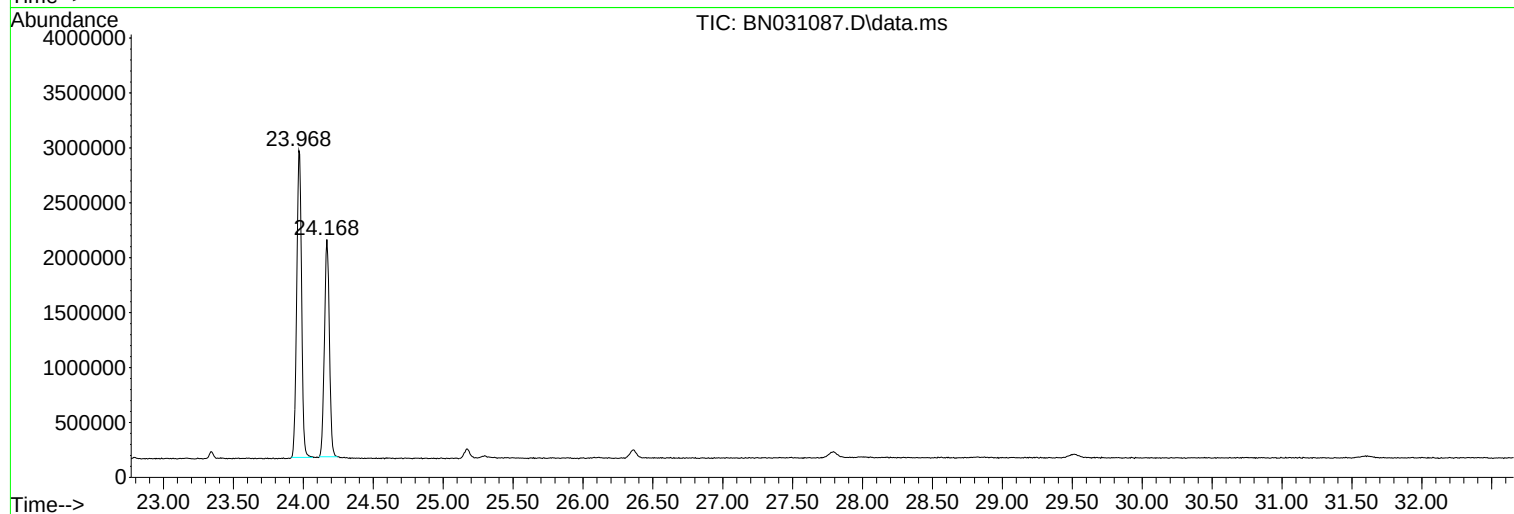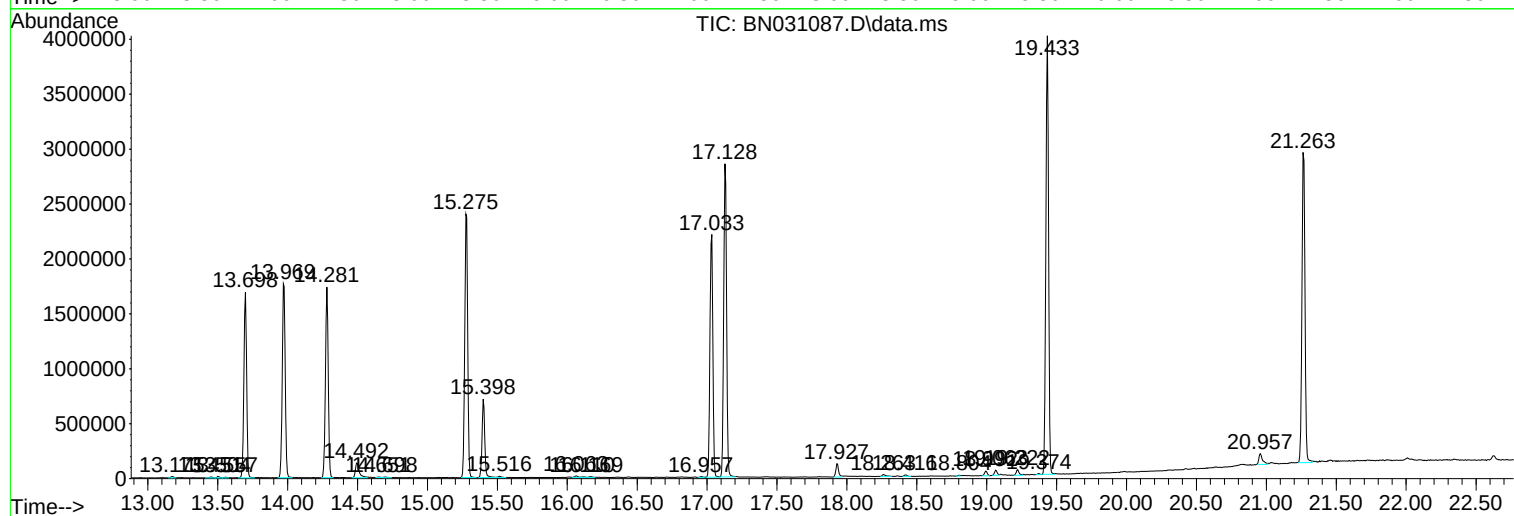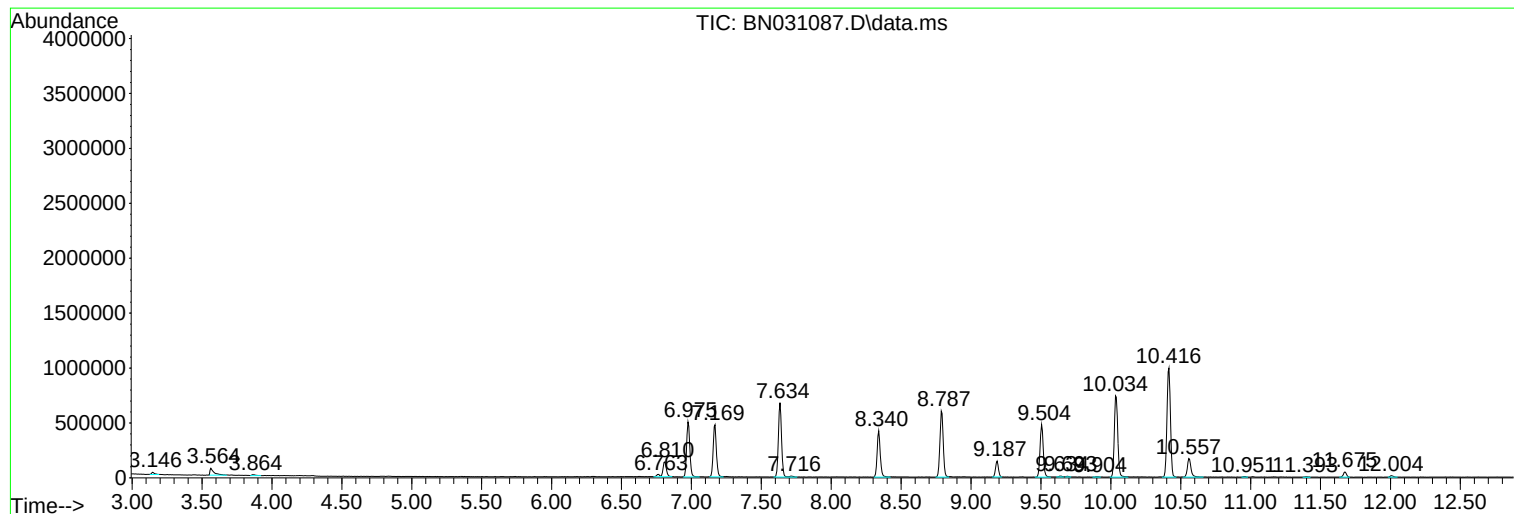

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031087.D
Acq On : 21 Apr 2024 00:03
Operator : MA/JU
Sample : P2077-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.187	2.49 ng/ul	210452	Naphthalene-d8	10.416

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
2			4-(2-Acetylamino-1-(trimethylsil...	339	C16H29N03Si2	1000373-43-5	43
3			Ethiofencarb sulfoxide, TMS deri...	313	C14H23N03SSi	1010485-32-4	43
4			Isoproterenol, 3TMS derivative	427	C20H41N03Si3	029522-12-1	43
5			Plumbane, diethyldimethyl-	296	C6H16Pb	001762-27-2	38

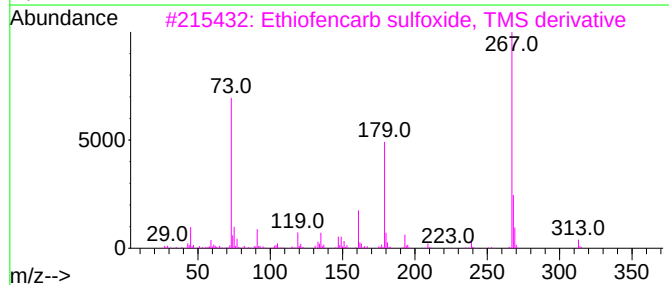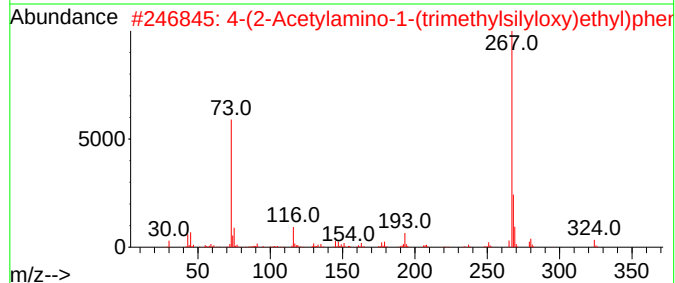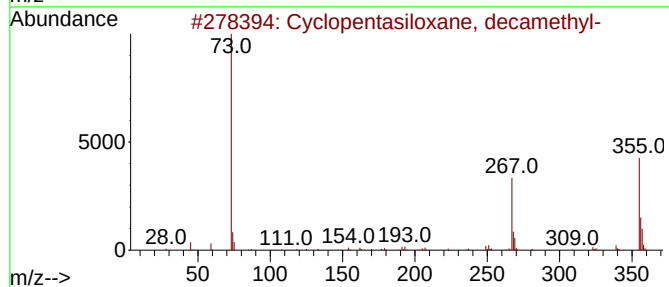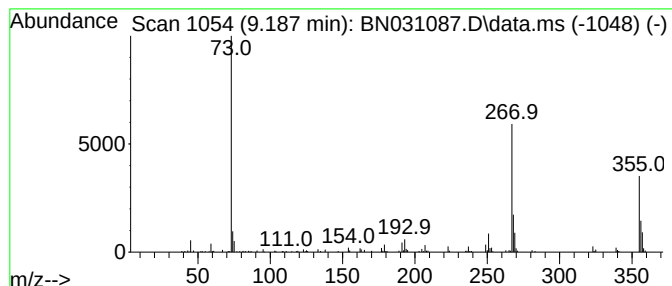

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031087.D
Acq On : 21 Apr 2024 00:03
Operator : MA/JU
Sample : P2077-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasilox...	9.187	2.5	ng/u1	210452	2	10.416	1692610	20.0