

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031088.D
 Acq On : 21 Apr 2024 00:43
 Operator : MA/JU
 Sample : P2077-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	32	rVB3	14454	18371	0.30%	0.042%
2	3.564	96	98	114	rBV	66890	142274	2.33%	0.322%
3	3.864	146	149	156	rVB6	6777	11570	0.19%	0.026%
4	6.810	644	650	661	rVB	98952	166386	2.73%	0.377%
5	6.975	671	678	690	rBV	401965	642950	10.55%	1.456%
6	7.169	704	711	720	rBV	364724	600463	9.85%	1.360%
7	7.634	783	790	800	rBV	568876	905461	14.86%	2.050%
8	7.716	800	804	808	rVB5	8062	14538	0.24%	0.033%
9	8.340	904	910	923	rBV	316587	510082	8.37%	1.155%
10	8.787	979	986	996	rBV	476982	792530	13.00%	1.795%
11	8.952	1009	1014	1022	rVB8	5769	10615	0.17%	0.024%
12	9.181	1049	1053	1059	rVB5	10304	15820	0.26%	0.036%
13	9.357	1078	1083	1089	rVB4	7736	12344	0.20%	0.028%
14	9.504	1101	1108	1117	rBV	381744	602041	9.88%	1.363%
15	9.646	1126	1132	1137	rBV3	6839	13500	0.22%	0.031%
16	9.693	1137	1140	1144	rVB3	4738	6545	0.11%	0.015%
17	10.040	1191	1199	1214	rBV	597008	1017885	16.70%	2.305%
18	10.204	1224	1227	1233	rVB6	3974	6525	0.11%	0.015%
19	10.410	1255	1262	1271	rBV	845870	1422030	23.33%	3.220%
20	10.557	1277	1287	1297	rBV	510229	888963	14.58%	2.013%
21	10.951	1350	1354	1360	rVB6	4907	9499	0.16%	0.022%
22	11.163	1382	1390	1395	rBV	16302	30275	0.50%	0.069%
23	11.669	1472	1476	1483	rVB5	3670	6931	0.11%	0.016%
24	12.010	1529	1534	1540	rBB2	10677	16955	0.28%	0.038%
25	13.175	1726	1732	1736	rBV2	11361	16992	0.28%	0.038%
26	13.451	1773	1779	1783	rBV4	8796	13439	0.22%	0.030%
27	13.504	1783	1788	1793	rVV	10658	16224	0.27%	0.037%
28	13.551	1793	1796	1803	rVV5	3904	6885	0.11%	0.016%
29	13.698	1813	1821	1829	rBV	1410870	1935722	31.76%	4.383%
30	13.975	1857	1868	1880	rBV	1490474	2230727	36.60%	5.051%
31	14.281	1914	1920	1928	rBV	1437613	2075300	34.05%	4.699%
32	14.498	1951	1957	1976	rBV	91470	192702	3.16%	0.436%
33	15.275	2082	2089	2100	rBV	2120177	3039667	49.87%	6.883%
34	15.398	2104	2110	2121	rBV	535124	709383	11.64%	1.606%
35	15.516	2126	2130	2133	rVB3	7781	9577	0.16%	0.022%
36	15.839	2181	2185	2192	rBV8	3457	7849	0.13%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031088.D
 Acq On : 21 Apr 2024 00:43
 Operator : MA/JU
 Sample : P2077-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

37	16.010	2209	2214	2216	rBV5	6133	8128	0.13%	0.018%
38	16.063	2219	2223	2227	rVV5	12890	19970	0.33%	0.045%
39	16.110	2228	2231	2236	rVV3	4361	7628	0.13%	0.017%
40	16.169	2237	2241	2247	rVB7	6627	10820	0.18%	0.025%
41	16.357	2266	2273	2278	rBV5	3412	7846	0.13%	0.018%
42	16.433	2282	2286	2291	rVB6	5196	7365	0.12%	0.017%
43	16.916	2363	2368	2371	rVB5	5037	7200	0.12%	0.016%
44	16.957	2371	2375	2379	rBV2	16307	20288	0.33%	0.046%
45	17.028	2381	2387	2394	rBV	1848835	2694366	44.20%	6.101%
46	17.128	2398	2404	2415	rVV	2468581	3536801	58.03%	8.009%
47	17.428	2449	2455	2460	rVB10	7142	12602	0.21%	0.029%
48	17.710	2499	2503	2507	rVB4	10515	13489	0.22%	0.031%
49	17.928	2535	2540	2548	rBV	144632	216290	3.55%	0.490%
50	18.263	2593	2597	2607	rVV4	15220	35385	0.58%	0.080%
51	18.363	2611	2614	2617	rVB4	9696	10763	0.18%	0.024%
52	18.422	2622	2624	2630	rVB5	7159	7744	0.13%	0.018%
53	18.804	2684	2689	2694	rBV6	13978	28763	0.47%	0.065%
54	18.992	2717	2721	2726	rVB3	36113	51180	0.84%	0.116%
55	19.063	2729	2733	2737	rBV2	38655	57341	0.94%	0.130%
56	19.222	2756	2760	2766	rBV2	67730	94466	1.55%	0.214%
57	19.369	2783	2785	2789	rVB4	10028	9711	0.16%	0.022%
58	19.433	2790	2796	2803	rVV	3563856	4750319	77.93%	10.757%
59	20.957	3051	3055	3062	rBV3	147507	241227	3.96%	0.546%
60	21.263	3101	3107	3122	rBV2	2511640	3653592	59.94%	8.273%
61	23.968	3558	3567	3579	rBV2	2525856	6095287	100.00%	13.802%
62	24.168	3592	3601	3614	rVB	1868111	4444351	72.91%	10.064%


Sum of corrected areas: 44161942

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031088.D
Acq On : 21 Apr 2024 00:43
Operator : MA/JU
Sample : P2077-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

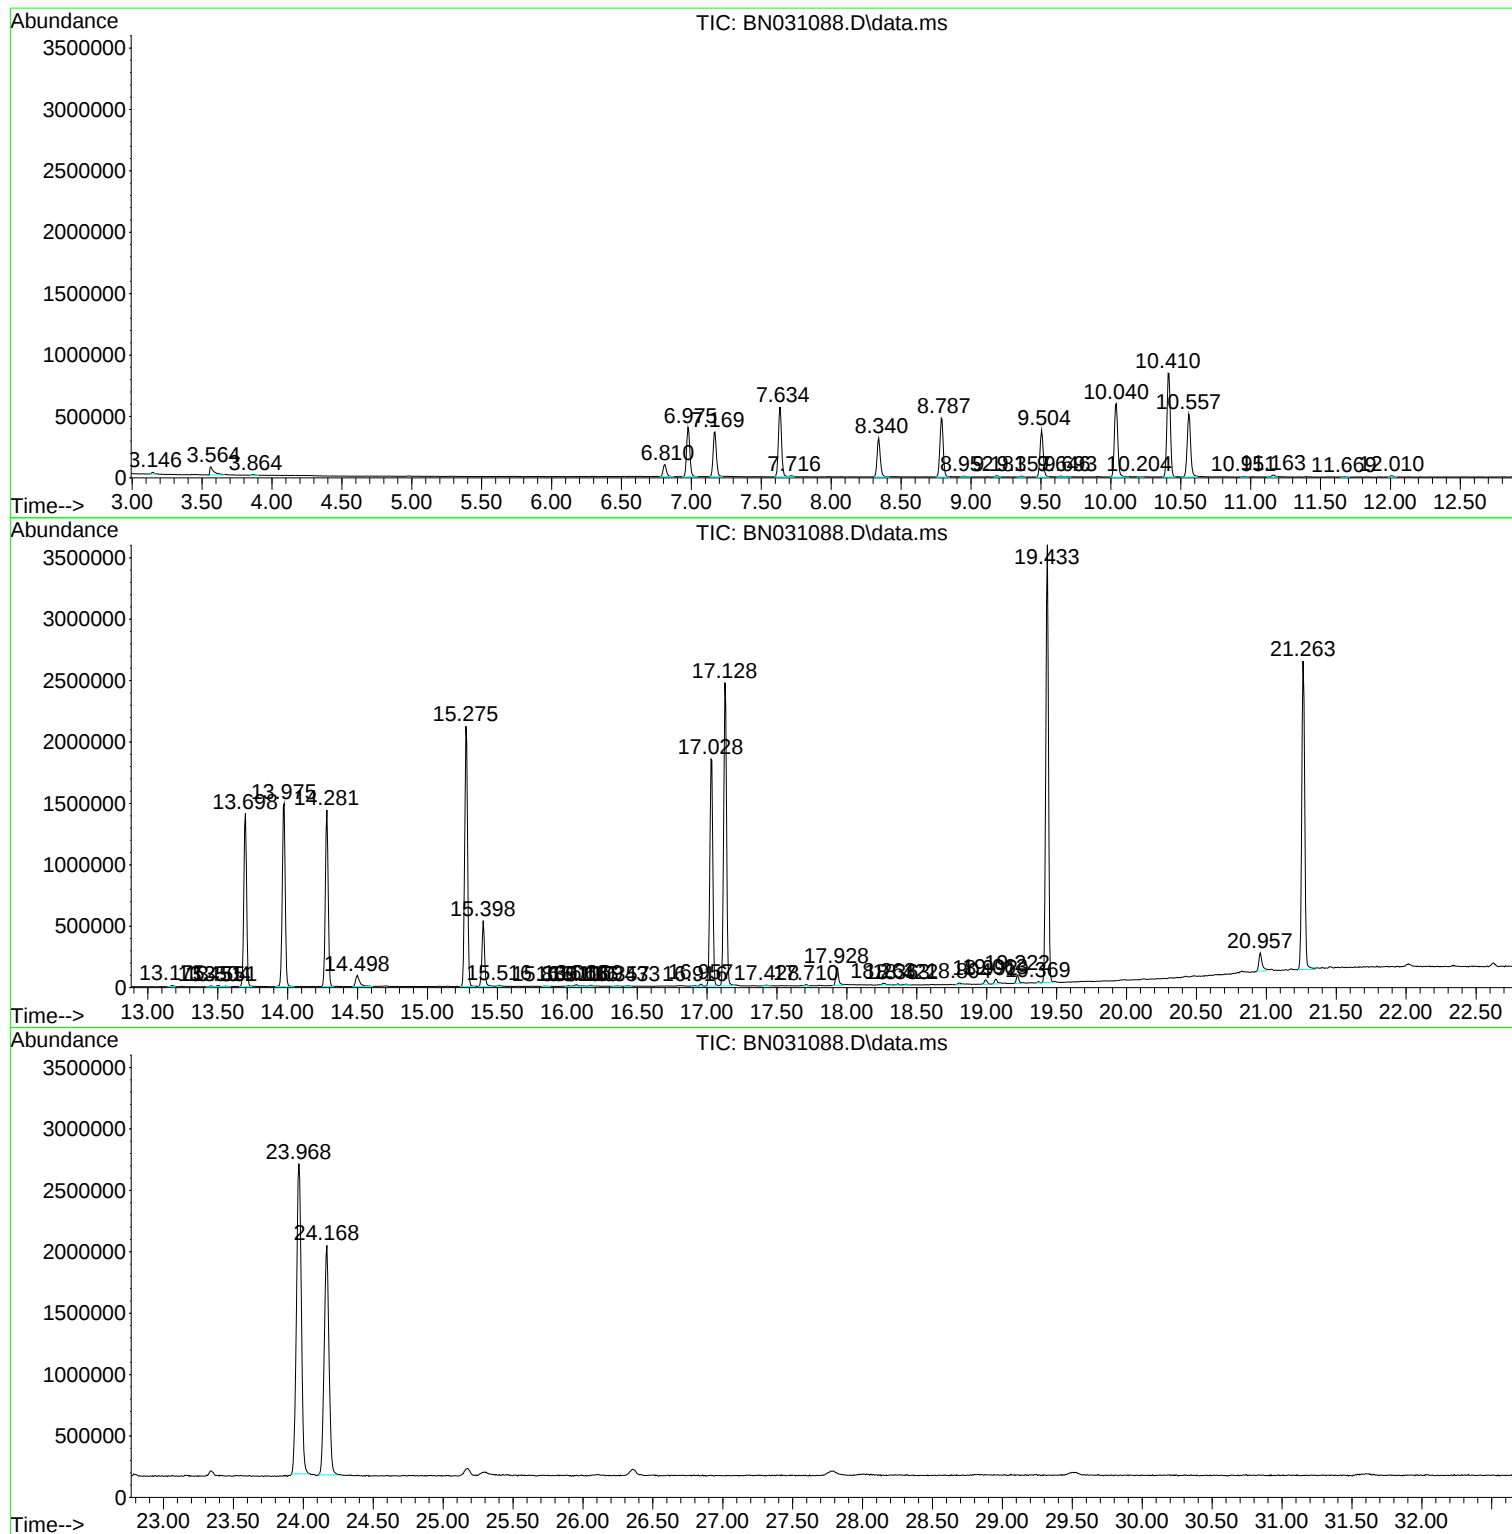

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031088.D
Acq On : 21 Apr 2024 00:43
Operator : MA/JU
Sample : P2077-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031088.D
Acq On : 21 Apr 2024 00:43
Operator : MA/JU
Sample : P2077-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc