

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031092.D
 Acq On : 21 Apr 2024 03:21
 Operator : MA/JU
 Sample : P2159-13
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	37	rVB	20439	31773	0.52%	0.077%
2	3.558	95	97	113	rBV	83094	153756	2.52%	0.374%
3	4.975	333	338	346	rVB	16204	26470	0.43%	0.064%
4	6.811	643	650	659	rBV	127094	209358	3.43%	0.509%
5	6.975	671	678	691	rBV	428439	665751	10.92%	1.619%
6	7.163	704	710	723	rBV	420616	667578	10.95%	1.623%
7	7.634	782	790	805	rBV	477158	777251	12.74%	1.890%
8	7.981	844	849	853	rBV2	15058	23527	0.39%	0.057%
9	8.340	903	910	922	rBV	377039	607953	9.97%	1.478%
10	8.787	978	986	997	rBV	502610	833319	13.66%	2.026%
11	8.946	1009	1013	1020	rVB9	6421	9967	0.16%	0.024%
12	9.505	1102	1108	1120	rBV	389613	624353	10.24%	1.518%
13	9.916	1172	1178	1183	rBV9	3336	7187	0.12%	0.017%
14	10.034	1191	1198	1209	rBV	625413	1049234	17.20%	2.552%
15	10.410	1254	1262	1271	rBV	704971	1186514	19.46%	2.885%
16	10.557	1280	1287	1302	rBV	537469	918538	15.06%	2.234%
17	12.004	1525	1533	1544	rBV3	10989	21361	0.35%	0.052%
18	13.181	1726	1733	1738	rBV5	8859	16007	0.26%	0.039%
19	13.698	1814	1821	1835	rBV	1294668	1810939	29.69%	4.404%
20	13.969	1861	1867	1878	rBV	1474844	2204889	36.15%	5.362%
21	14.281	1913	1920	1929	rBV	1209926	1755517	28.79%	4.269%
22	14.492	1948	1956	1970	rBV	117737	234334	3.84%	0.570%
23	15.034	2044	2048	2053	rBV3	5464	8753	0.14%	0.021%
24	15.116	2058	2062	2068	rVB2	6946	10411	0.17%	0.025%
25	15.275	2082	2089	2098	rBV	2031530	2858484	46.87%	6.951%
26	15.398	2104	2110	2123	rBV	544270	741580	12.16%	1.803%
27	15.516	2126	2130	2133	rVB4	8769	10791	0.18%	0.026%
28	16.057	2220	2222	2227	rVB5	5873	7169	0.12%	0.017%
29	16.822	2346	2352	2355	rBV4	3284	7203	0.12%	0.018%
30	17.028	2379	2387	2397	rBV	1591372	2279209	37.37%	5.543%
31	17.128	2398	2404	2419	rVV	2470668	3546214	58.15%	8.624%
32	17.928	2535	2540	2544	rBV5	27517	38075	0.62%	0.093%
33	18.222	2586	2590	2594	rVB6	5100	10157	0.17%	0.025%
34	18.992	2717	2721	2726	rVB2	32636	42943	0.70%	0.104%
35	19.063	2729	2733	2738	rBV	28853	42184	0.69%	0.103%
36	19.216	2756	2759	2763	rBV6	16004	21593	0.35%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031092.D
Acq On : 21 Apr 2024 03:21
Operator : MA/JU
Sample : P2159-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R91

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	19.433	2790	2796	2804	rBV	3427379	4559242	74.76%	11.087%
38	21.263	3101	3107	3116	rBV	2178842	3132938	51.37%	7.619%
39	23.968	3558	3567	3585	rVB2	2632979	6098538	100.00%	14.831%
40	24.168	3592	3601	3615	rVB	1575106	3870259	63.46%	9.412%




Sum of corrected areas: 41121319

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031092.D
Acq On : 21 Apr 2024 03:21
Operator : MA/JU
Sample : P2159-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

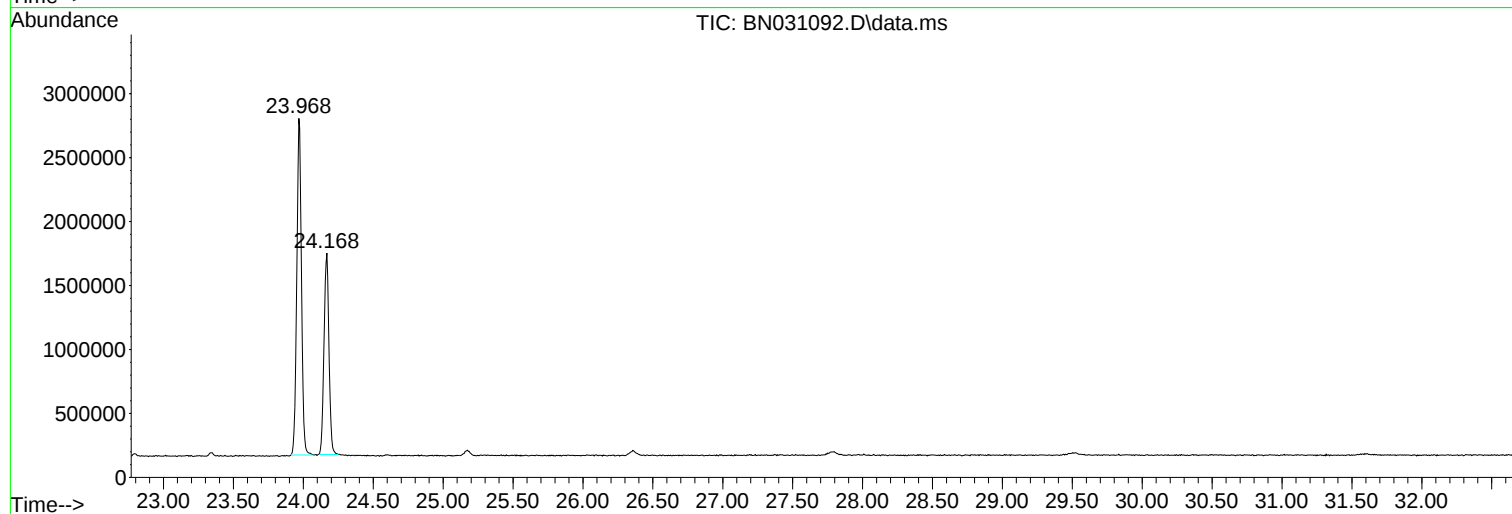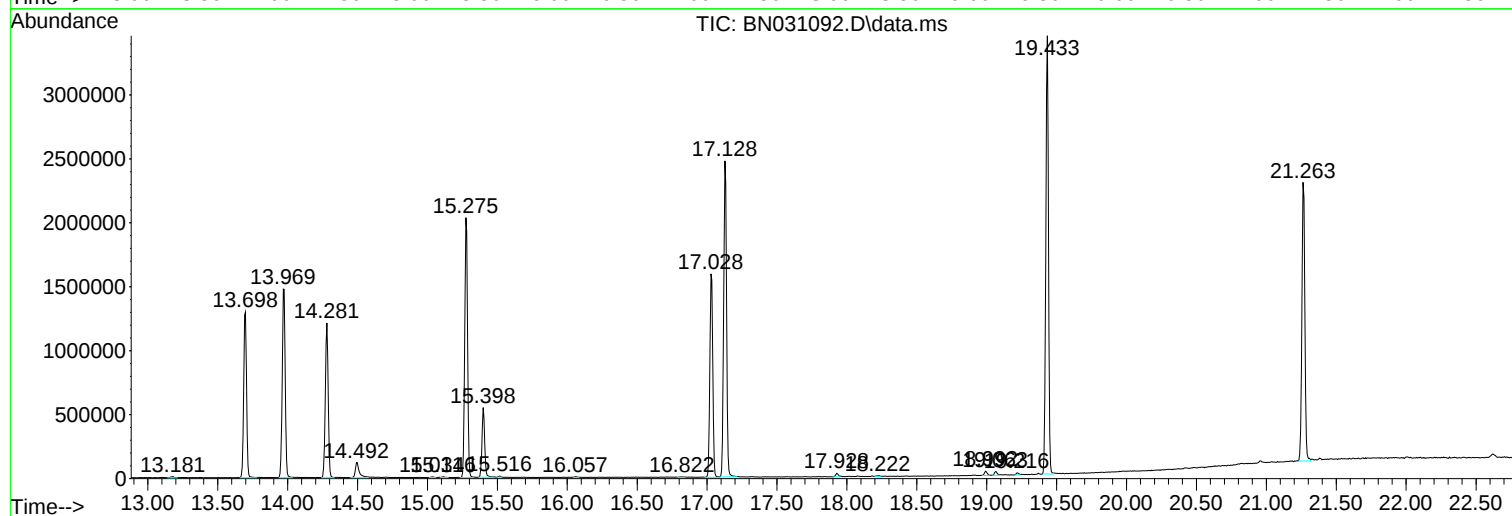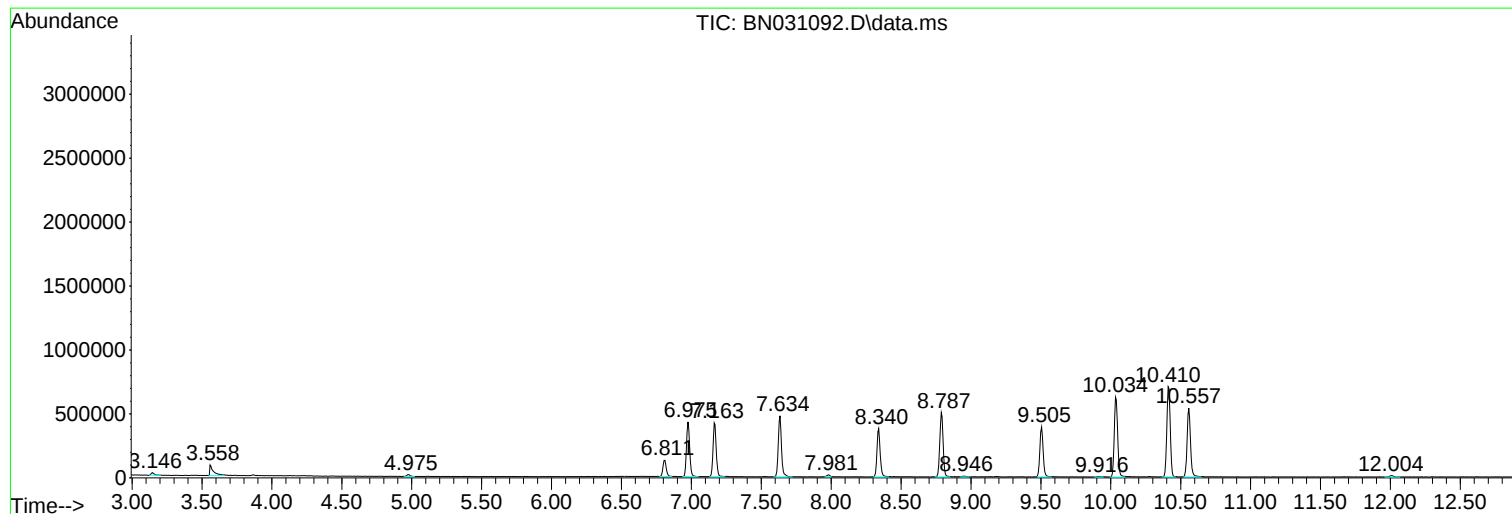

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031092.D
Acq On : 21 Apr 2024 03:21
Operator : MA/JU
Sample : P2159-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031092.D
Acq On : 21 Apr 2024 03:21
Operator : MA/JU
Sample : P2159-13
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R91

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------