

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031099.D
 Acq On : 21 Apr 2024 08:35
 Operator : MA/JU
 Sample : PB160363BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK363

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	36	rVB	24287	37380	0.70%	0.091%
2	3.552	94	96	116	rBV	269044	489567	9.21%	1.196%
3	3.864	147	149	153	rVB4	5718	6290	0.12%	0.015%
4	6.805	643	649	661	rBV	515747	818934	15.41%	2.000%
5	6.975	672	678	689	rVB	423358	653752	12.30%	1.597%
6	7.163	702	710	718	rBV	517161	812275	15.28%	1.984%
7	7.634	783	790	799	rBV	441236	703848	13.24%	1.719%
8	8.334	901	909	923	rBV	654672	1066269	20.06%	2.604%
9	8.787	978	986	997	rBV	519261	825616	15.53%	2.017%
10	8.951	1008	1014	1017	rBV6	5842	10393	0.20%	0.025%
11	9.504	1101	1108	1122	rBV	407251	659820	12.41%	1.612%
12	10.034	1191	1198	1209	rBV	678728	1114313	20.96%	2.722%
13	10.410	1255	1262	1272	rBV	694054	1126724	21.20%	2.752%
14	10.557	1277	1287	1302	rBV	514454	885276	16.65%	2.162%
15	12.004	1529	1533	1539	rBV	10462	16408	0.31%	0.040%
16	13.175	1726	1732	1738	rBV2	11915	18599	0.35%	0.045%
17	13.692	1813	1820	1827	rBV	1314836	1777638	33.44%	4.342%
18	13.969	1860	1867	1878	rBV	1512606	2193786	41.27%	5.359%
19	14.281	1911	1920	1928	rBV	1151469	1675146	31.51%	4.092%
20	14.486	1948	1955	1972	rBV	547972	940584	17.69%	2.297%
21	15.275	2082	2089	2104	rBV	2042779	2812475	52.91%	6.870%
22	15.398	2104	2110	2122	rBV	509840	691585	13.01%	1.689%
23	15.510	2127	2129	2135	rVB4	9494	12360	0.23%	0.030%
24	16.063	2217	2223	2226	rBV6	6875	9010	0.17%	0.022%
25	17.028	2381	2387	2398	rBV	1581196	2203379	41.45%	5.382%
26	17.128	2398	2404	2416	rBV	2272186	3209527	60.38%	7.840%
27	17.927	2537	2540	2545	rVB7	4380	5600	0.11%	0.014%
28	18.992	2716	2721	2728	rBV2	29218	42203	0.79%	0.103%
29	19.063	2730	2733	2738	rVB2	24880	34347	0.65%	0.084%
30	19.433	2790	2796	2804	rBV	3092364	4208429	79.17%	10.280%
31	21.263	3101	3107	3117	rBV	2122388	2994706	56.34%	7.315%
32	23.968	3558	3567	3578	rBV2	2213436	5315727	100.00%	12.984%
33	24.168	3592	3601	3615	rVB2	1456536	3567705	67.12%	8.715%




Sum of corrected areas: 40939671

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031099.D
Acq On : 21 Apr 2024 08:35
Operator : MA/JU
Sample : PB160363BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

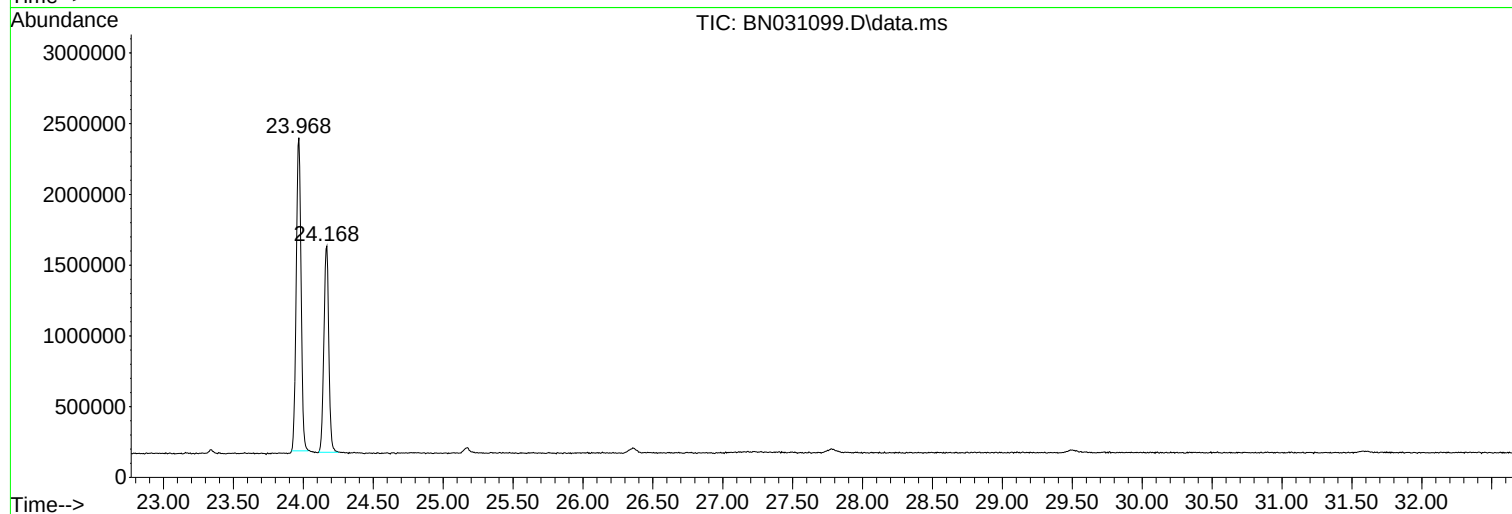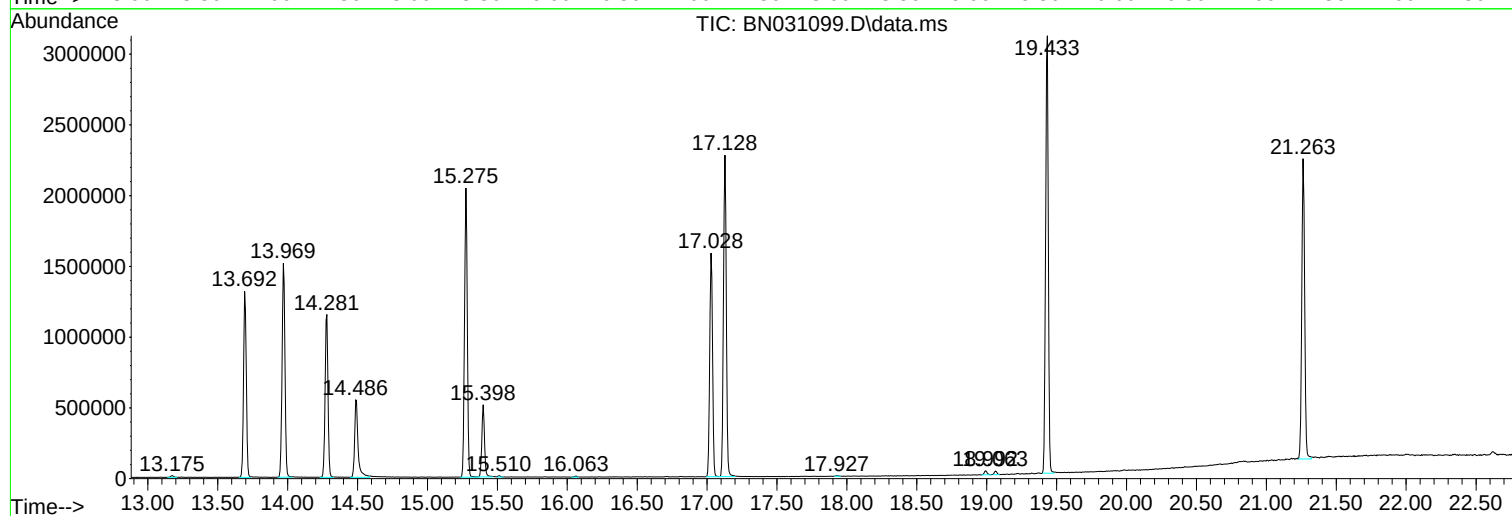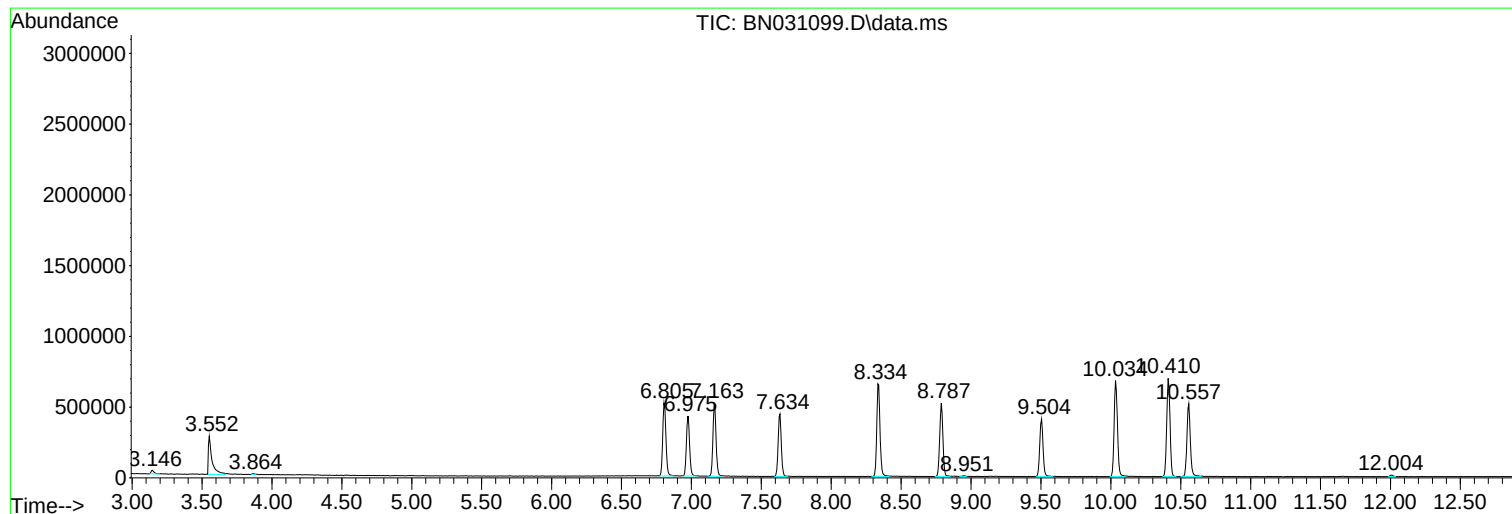

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031099.D
Acq On : 21 Apr 2024 08:35
Operator : MA/JU
Sample : PB160363BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031099.D
Acq On : 21 Apr 2024 08:35
Operator : MA/JU
Sample : PB160363BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK363

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------