

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031100.D
 Acq On : 21 Apr 2024 09:14
 Operator : MA/JU
 Sample : PB160364BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK364

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	37	rBV	31464	47963	0.73%	0.091%
2	3.552	93	96	119	rBV	337151	592344	9.00%	1.128%
3	3.863	146	149	154	rVB3	8036	10913	0.17%	0.021%
4	6.804	643	649	662	rVB	648648	1014115	15.40%	1.932%
5	6.975	672	678	691	rVB	542100	831484	12.63%	1.584%
6	7.163	703	710	720	rBV	641472	1018798	15.47%	1.941%
7	7.634	783	790	801	rBV	601886	960143	14.58%	1.829%
8	8.334	901	909	923	rBV	820015	1334167	20.26%	2.542%
9	8.787	978	986	997	rBV	636823	1026690	15.59%	1.956%
10	8.951	1008	1014	1019	rVB9	4950	8715	0.13%	0.017%
11	9.504	1101	1108	1118	rBV	503647	822597	12.49%	1.567%
12	10.034	1191	1198	1209	rBV	840225	1390096	21.11%	2.648%
13	10.410	1255	1262	1272	rBV	947385	1539763	23.39%	2.933%
14	10.557	1279	1287	1303	rBV	624878	1078401	16.38%	2.054%
15	12.010	1529	1534	1540	rBV	13213	22635	0.34%	0.043%
16	13.175	1727	1732	1737	rVB4	9554	13678	0.21%	0.026%
17	13.692	1814	1820	1830	rBV	1620851	2208223	33.54%	4.207%
18	13.969	1860	1867	1876	rBV2	1827458	2737015	41.57%	5.214%
19	14.281	1913	1920	1934	rBV	1573669	2264482	34.39%	4.314%
20	14.492	1947	1956	1979	rBV	738593	1236588	18.78%	2.356%
21	15.275	2082	2089	2099	rBV	2448064	3455138	52.48%	6.582%
22	15.398	2104	2110	2122	rVV	681799	917764	13.94%	1.748%
23	15.516	2126	2130	2136	rVB3	11393	18554	0.28%	0.035%
24	16.063	2219	2223	2226	rBV4	7387	9707	0.15%	0.018%
25	17.027	2380	2387	2397	rBV	2182532	2977354	45.22%	5.672%
26	17.127	2397	2404	2419	rVV2	2861958	4022637	61.10%	7.663%
27	17.927	2536	2540	2544	rBV4	10190	14860	0.23%	0.028%
28	18.992	2717	2721	2726	rVB2	36659	49505	0.75%	0.094%
29	19.063	2729	2733	2738	rBV	34311	46676	0.71%	0.089%
30	19.221	2756	2760	2763	rBV6	9616	12970	0.20%	0.025%
31	19.368	2782	2785	2789	rBV3	8469	10287	0.16%	0.020%
32	19.433	2789	2796	2810	rBV	3771455	5219224	79.27%	9.943%
33	21.262	3101	3107	3117	rBV	2804047	4037737	61.33%	7.692%
34	23.968	3558	3567	3582	rVB2	2815637	6584140	100.00%	12.543%
35	24.168	3591	3601	3615	rBV	1969713	4957623	75.30%	9.444%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031100.D
Acq On : 21 Apr 2024 09:14
Operator : MA/JU
Sample : PB160364BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK364

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 52492986

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031100.D
Acq On : 21 Apr 2024 09:14
Operator : MA/JU
Sample : PB160364BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK364

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

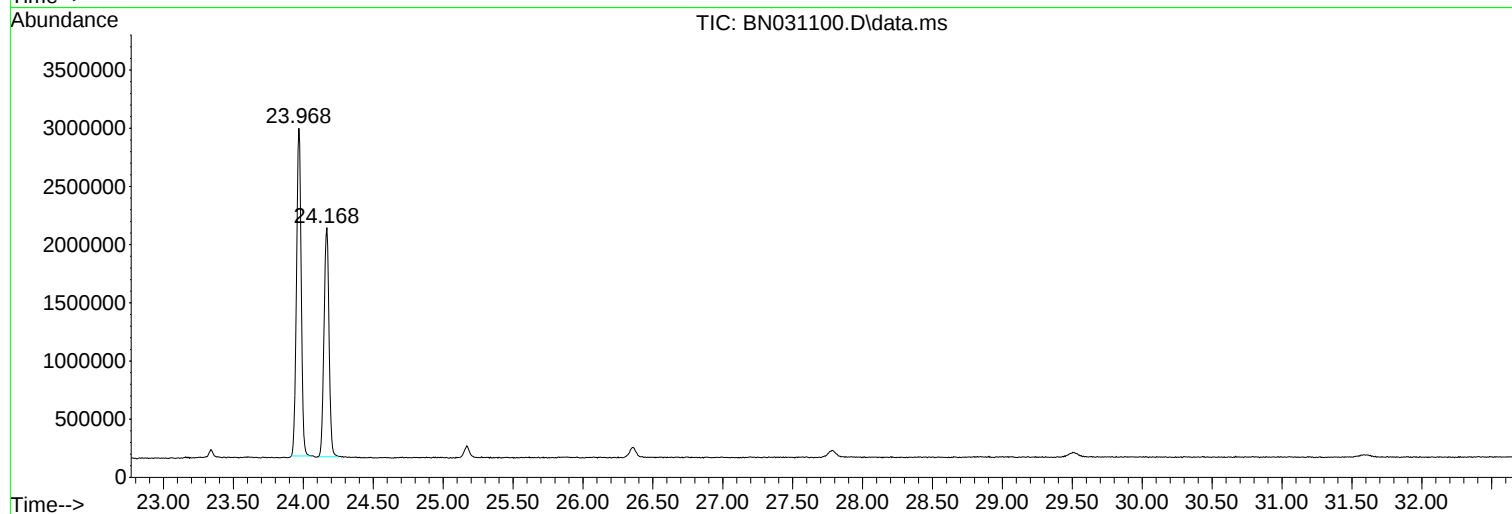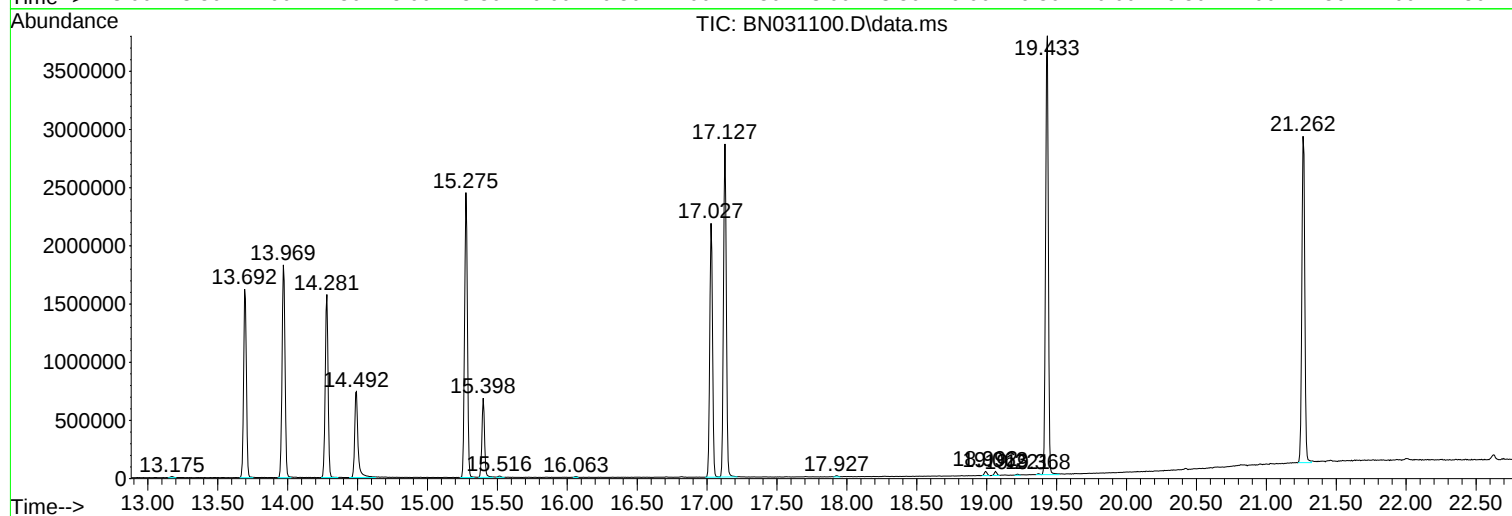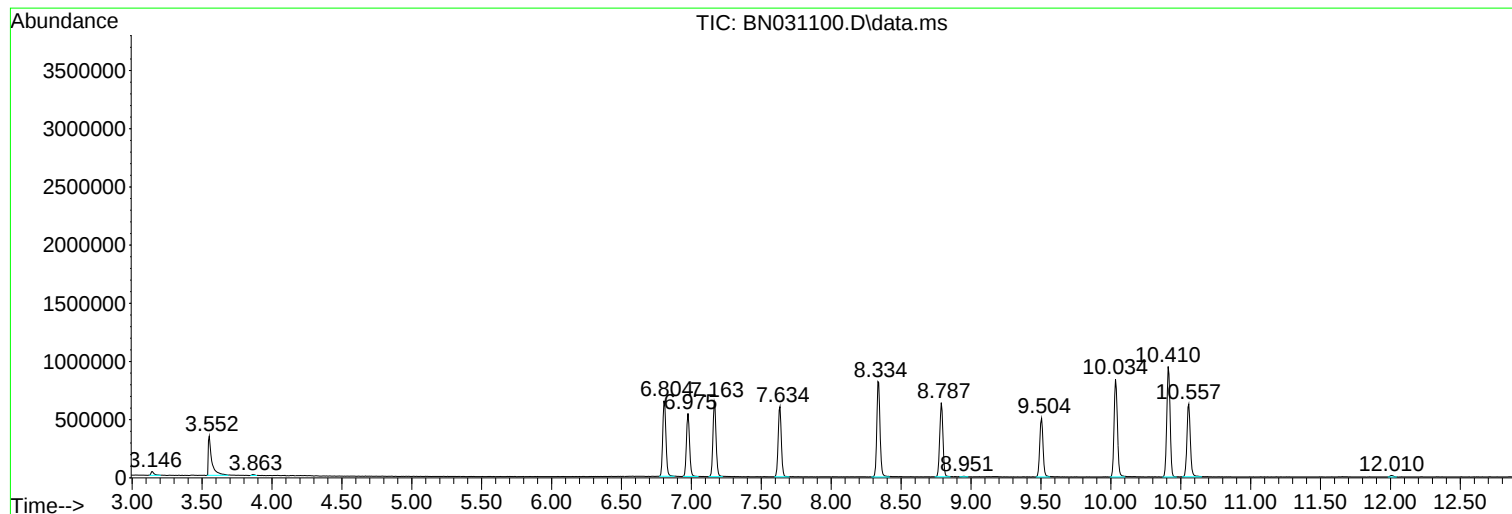

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031100.D
Acq On : 21 Apr 2024 09:14
Operator : MA/JU
Sample : PB160364BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK364

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031100.D
Acq On : 21 Apr 2024 09:14
Operator : MA/JU
Sample : PB160364BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK364

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------