

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
 Data File : BN031102.D
 Acq On : 21 Apr 2024 10:32
 Operator : MA/JU
 Sample : P2159-18
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	32	rVB	18302	23224	0.33%	0.043%
2	3.558	95	97	113	rBV	107116	192034	2.69%	0.356%
3	3.864	147	149	155	rVB3	7957	10365	0.15%	0.019%
4	4.975	335	338	345	rVB6	3952	7309	0.10%	0.014%
5	6.805	644	649	658	rVB	109728	177590	2.49%	0.329%
6	6.975	671	678	692	rBV	541879	848548	11.89%	1.572%
7	7.163	702	710	721	rBV	495638	777053	10.89%	1.440%
8	7.634	783	790	806	rBV	719026	1181479	16.56%	2.189%
9	8.334	902	909	921	rBV	367399	603792	8.46%	1.119%
10	8.787	977	986	1000	rBV	662462	1067278	14.96%	1.978%
11	8.952	1010	1014	1020	rVB8	5311	8037	0.11%	0.015%
12	9.181	1049	1053	1059	rVB3	4896	8731	0.12%	0.016%
13	9.504	1100	1108	1121	rBV	499313	812292	11.39%	1.505%
14	10.034	1192	1198	1211	rBV	783287	1260417	17.67%	2.336%
15	10.275	1233	1239	1245	rBV	96275	151018	2.12%	0.280%
16	10.410	1252	1262	1271	rBV	1134030	1844992	25.86%	3.419%
17	10.557	1280	1287	1300	rBV	565411	986069	13.82%	1.827%
18	10.793	1320	1327	1336	rVB2	32480	55774	0.78%	0.103%
19	11.669	1472	1476	1482	rVB6	4101	7881	0.11%	0.015%
20	12.004	1526	1533	1540	rBV3	13951	27332	0.38%	0.051%
21	13.063	1710	1713	1718	rBV2	9595	13904	0.19%	0.026%
22	13.175	1725	1732	1737	rVB2	12721	19785	0.28%	0.037%
23	13.692	1814	1820	1831	rBV	1691640	2350643	32.95%	4.356%
24	13.969	1859	1867	1881	rBV2	1889635	2786761	39.06%	5.164%
25	14.281	1913	1920	1935	rBV	1790915	2648464	37.12%	4.908%
26	14.492	1951	1956	1967	rBV	94043	188510	2.64%	0.349%
27	14.587	1970	1972	1978	rVB5	6450	9886	0.14%	0.018%
28	15.275	2082	2089	2102	rBV	2665712	3710525	52.01%	6.876%
29	15.398	2104	2110	2125	rVV	742904	999657	14.01%	1.852%
30	15.510	2125	2129	2135	rVB4	11537	19932	0.28%	0.037%
31	15.998	2209	2212	2218	rVB8	5252	7483	0.10%	0.014%
32	16.063	2218	2223	2227	rVB5	7897	10715	0.15%	0.020%
33	17.028	2381	2387	2397	rBV	2376201	3392278	47.55%	6.286%
34	17.128	2397	2404	2424	rVB2	3180893	4595962	64.42%	8.516%
35	17.704	2498	2502	2505	rVB6	9099	10824	0.15%	0.020%
36	17.928	2535	2540	2549	rBV	84346	118235	1.66%	0.219%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031102.D
Acq On : 21 Apr 2024 10:32
Operator : MA/JU
Sample : P2159-18
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORD5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	18.992	2717	2721	2728	rBV3	44850	58945	0.83%	0.109%
38	19.063	2728	2733	2737	rBV	39232	56229	0.79%	0.104%
39	19.127	2742	2744	2748	rBV5	5371	7336	0.10%	0.014%
40	19.216	2755	2759	2764	rBV2	42422	56393	0.79%	0.104%
41	19.369	2782	2785	2789	rBV4	9852	10642	0.15%	0.020%
42	19.433	2789	2796	2803	rBV	4247649	5789671	81.15%	10.728%
43	20.957	3052	3055	3065	rBV4	53642	83738	1.17%	0.155%
44	21.263	3101	3107	3116	rBV2	3106804	4563956	63.97%	8.457%
45	23.968	3557	3567	3580	rBV2	2930341	7134116	100.00%	13.220%
46	24.168	3592	3601	3613	rVB	2131326	5270755	73.88%	9.767%




Sum of corrected areas: 53966560

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031102.D
Acq On : 21 Apr 2024 10:32
Operator : MA/JU
Sample : P2159-18
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

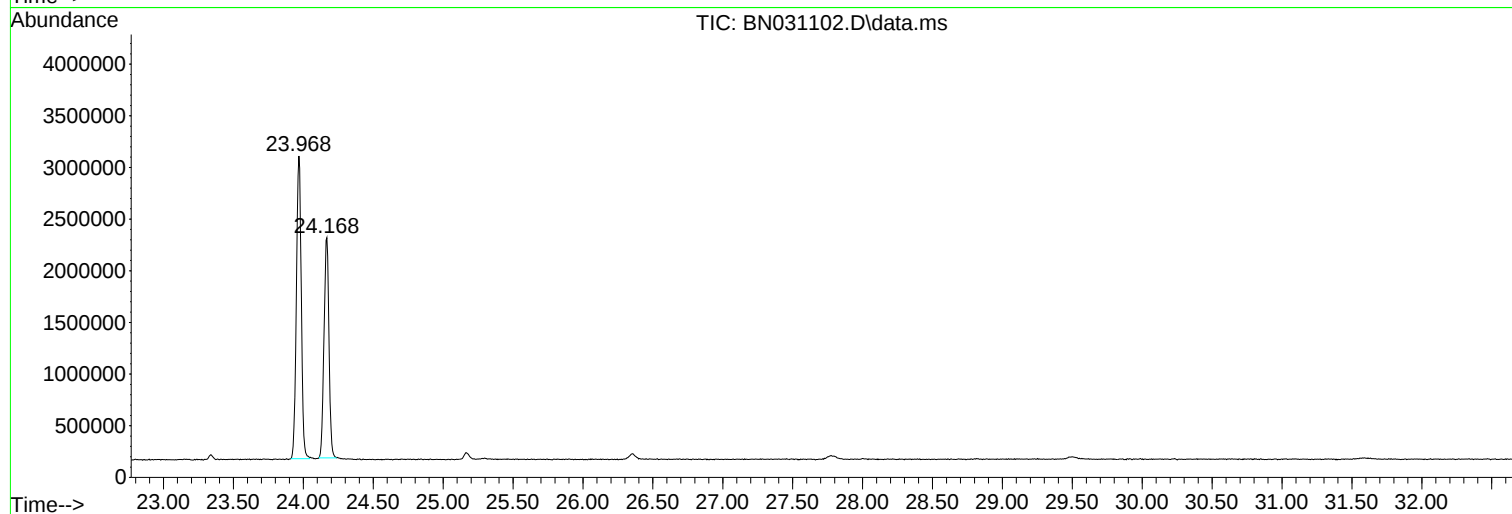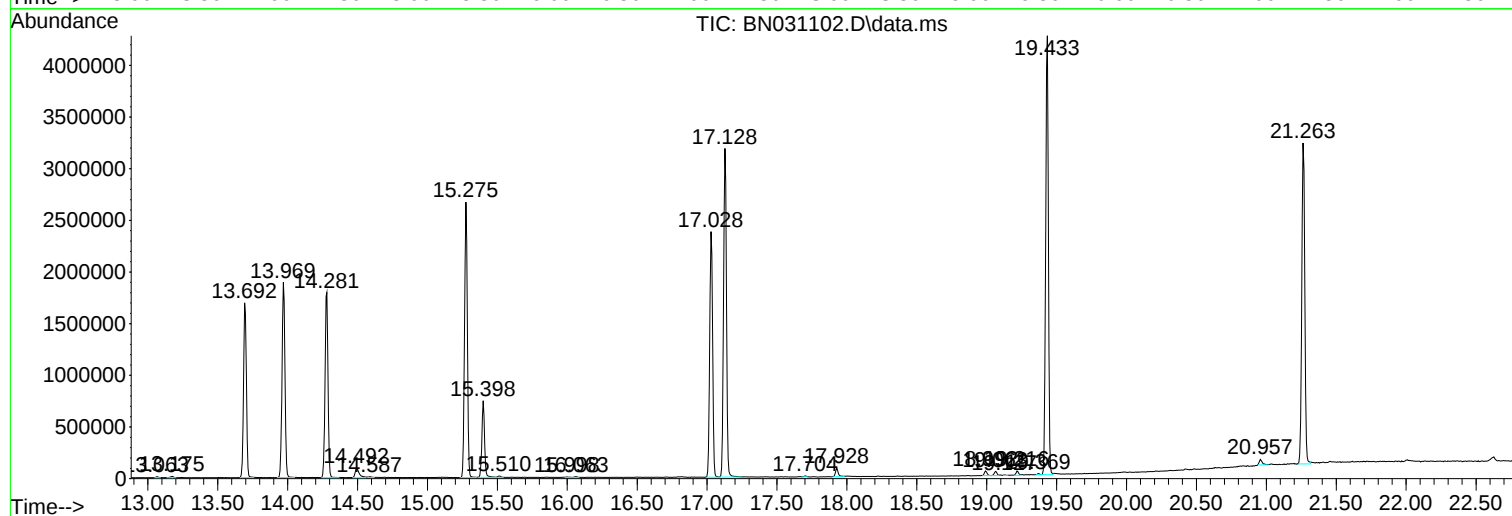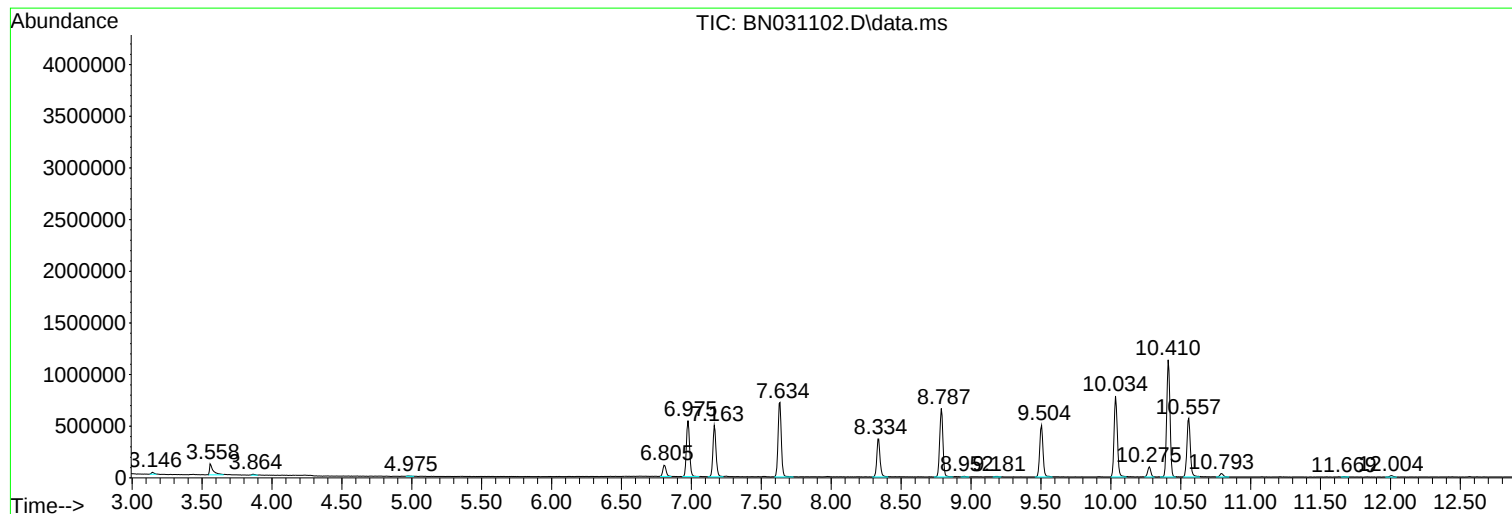

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031102.D
Acq On : 21 Apr 2024 10:32
Operator : MA/JU
Sample : P2159-18
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041924\
Data File : BN031102.D
Acq On : 21 Apr 2024 10:32
Operator : MA/JU
Sample : P2159-18
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------