
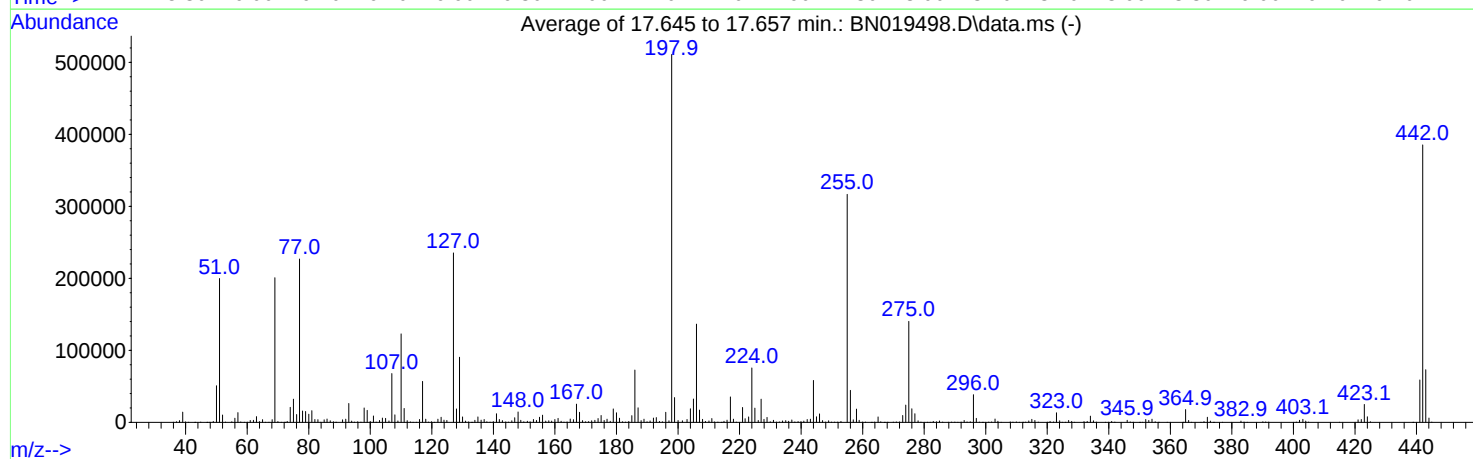


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042022\
 Data File : BN019498.D
 Acq On : 19 Apr 2022 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 04 17:40:00 2022

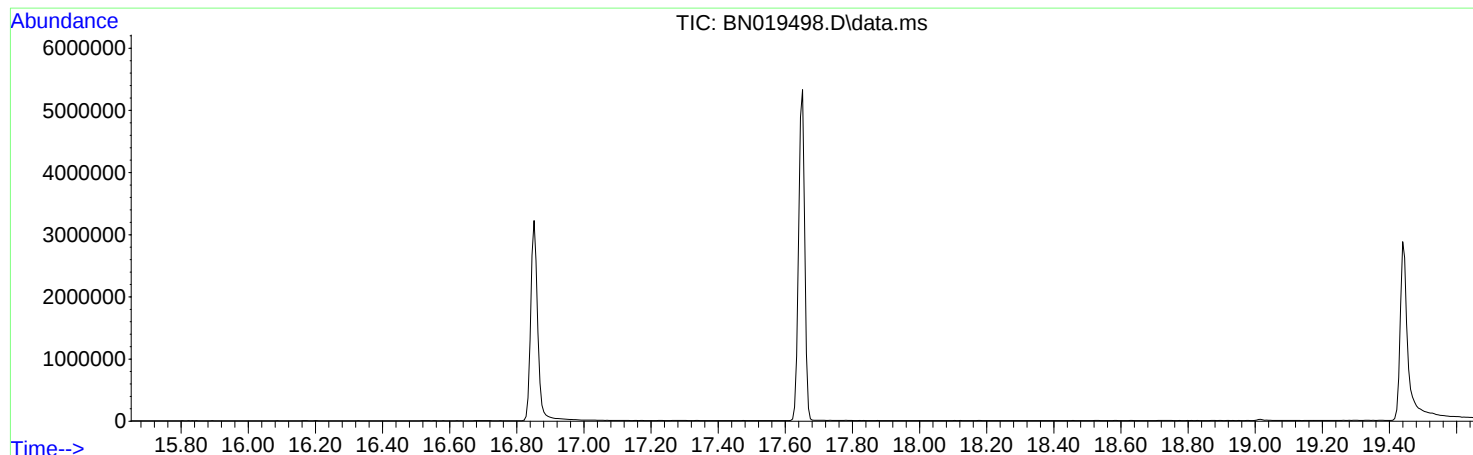




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	199866	PASS
68	69	0.00	2	1.8	3703	PASS
69	198	0.00	100	39.3	200933	PASS
70	69	0.00	2	0.6	1160	PASS
127	198	10	80	46.1	235371	PASS
197	198	0.00	2	0.4	2253	PASS
198	198	100	100	100.0	510976	PASS
199	198	5	9	6.7	34379	PASS
275	198	10	60	27.5	140291	PASS
365	198	1	100	3.5	17910	PASS
441	198	0.01	100	11.5	58965	PASS
442	442	50	100	100.0	385301	PASS
443	442	15	24	19.0	73056	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042022\
 Data File : BN019498.D
 Acq On : 19 Apr 2022 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 20 06:50:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

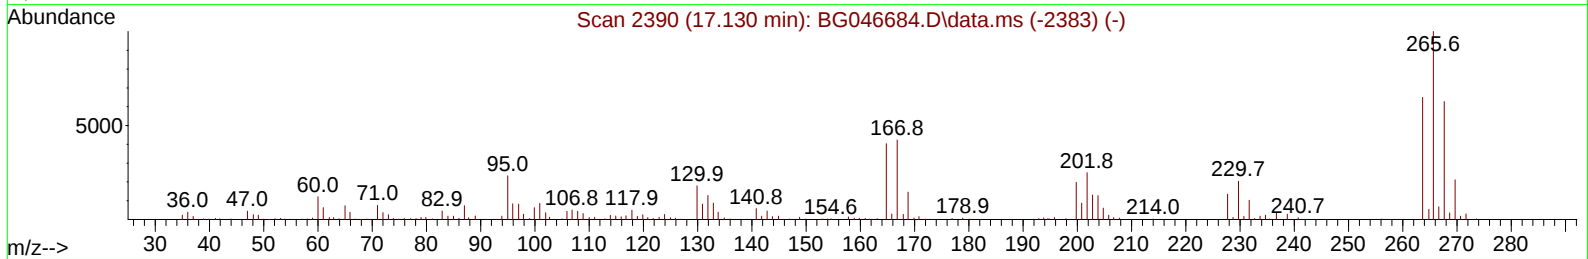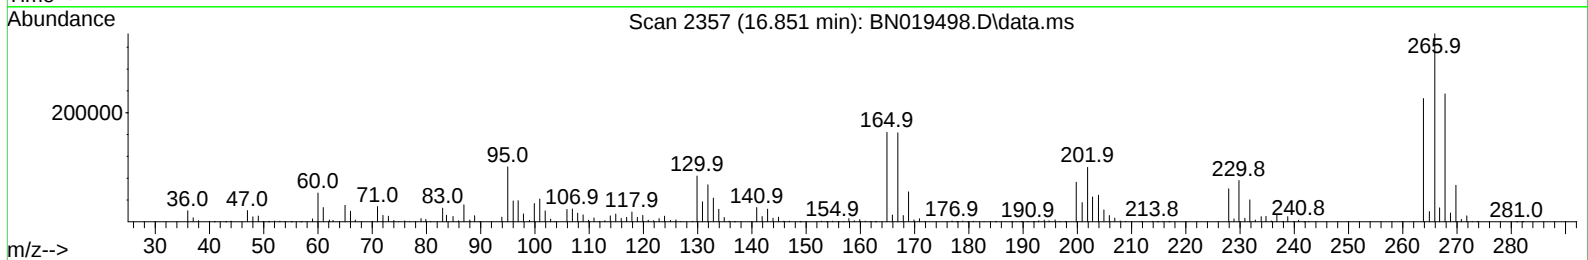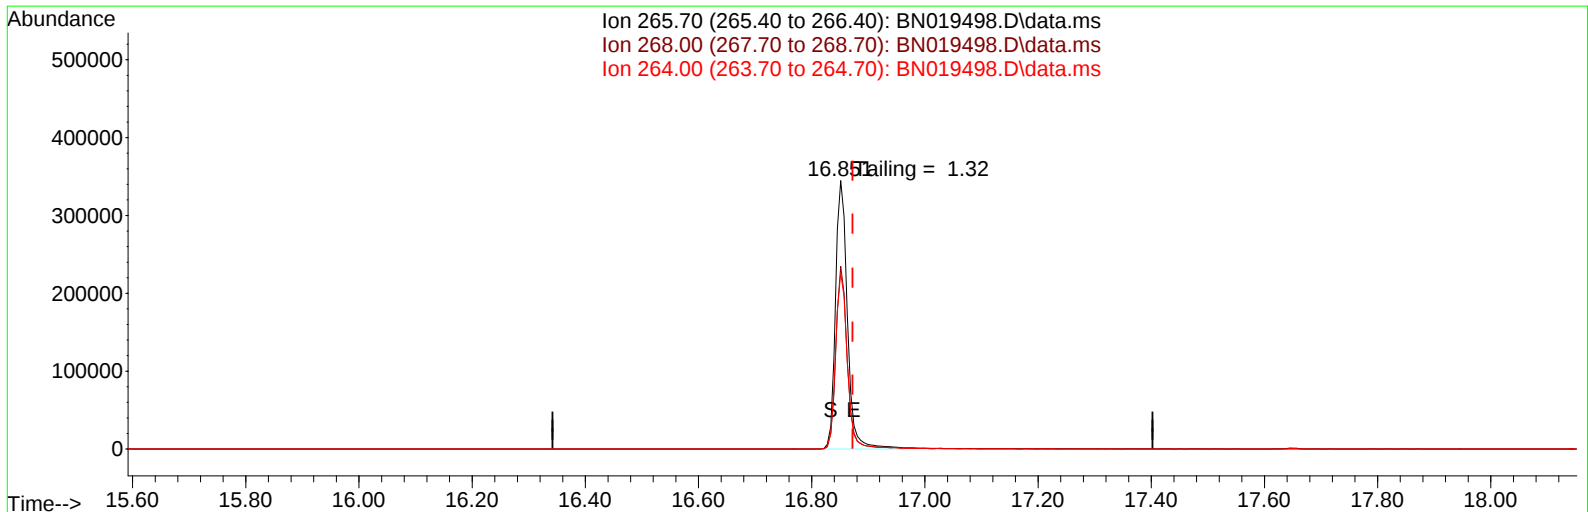

TIC: BN019498.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.021) 16388.84 ng




response 511118

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.02
264.00	61.60	65.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042022\
Data File : BN019498.D
Acq On : 19 Apr 2022 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 20 06:50:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

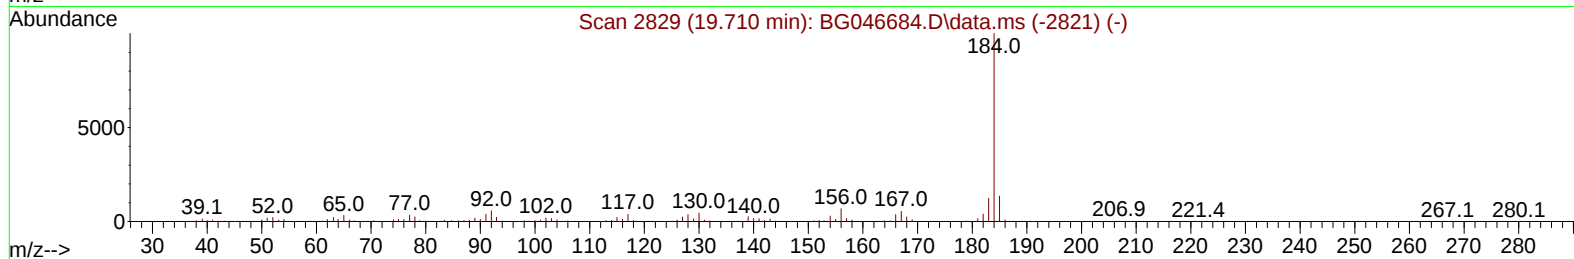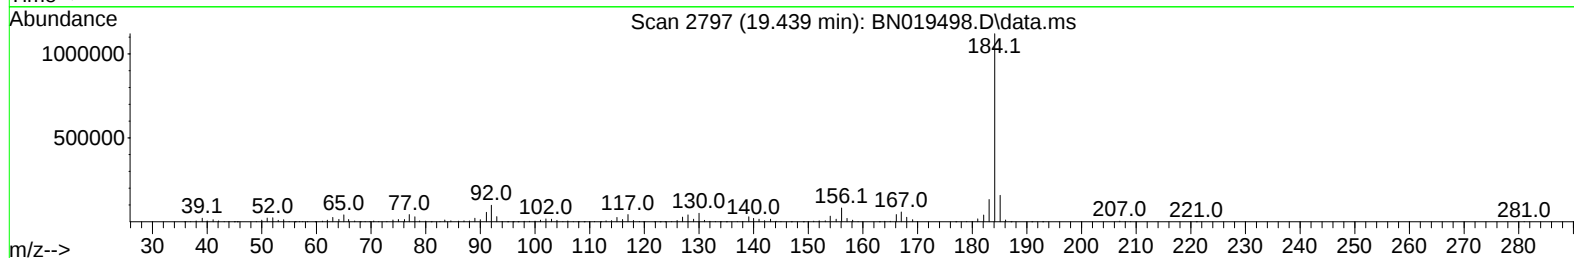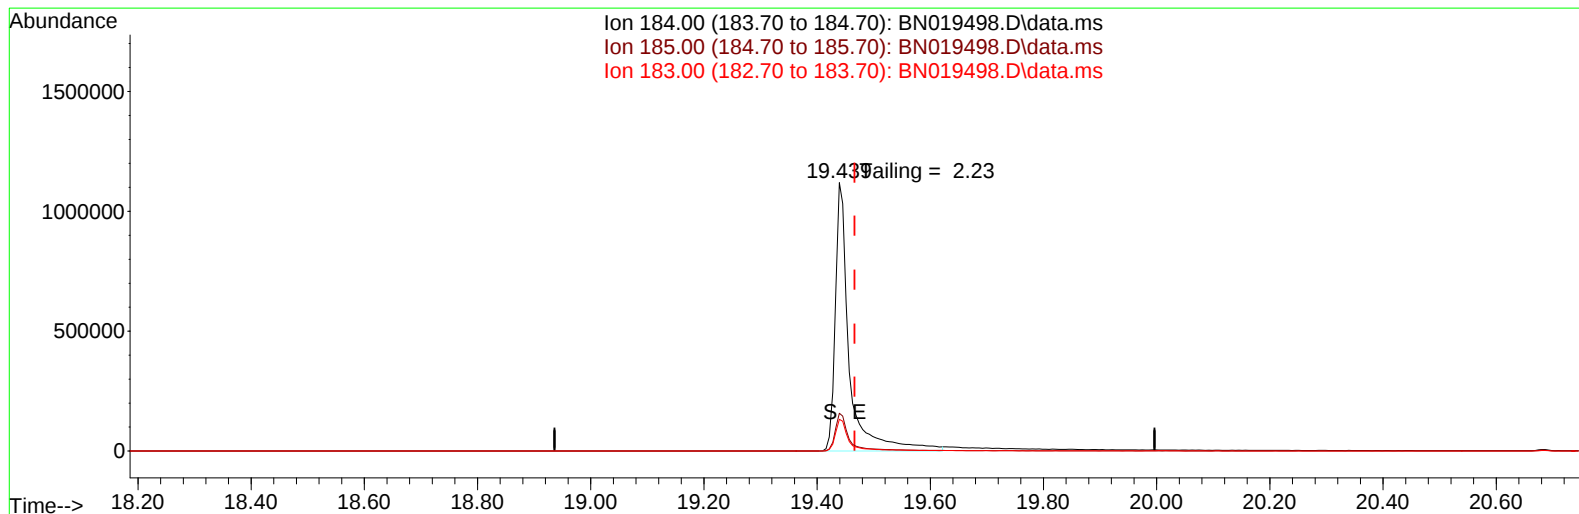

TIC: BN019498.D\data.ms

(77) Benzidine

19.439min (-0.027) 0.00 ng

response 2031215

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/20/2022	BNA_N	<u>BN019498.D</u>
Compound Name	Response	Retention Time
DDT	1434006	20.686
DDD	59688	20.245
DDE	3459	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
63147	1497153	4.22

Instrument :
BNA_N
ClientSampleId :
DFTPP