

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042023\
 Data File : BN025039.D
 Acq On : 20 Apr 2023 17:26
 Operator : CG/JU
 Sample : PB152216BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 21 04:26:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	8742	0.400	ng/ul	0.00
4) Naphthalene-d8	10.737	136	27518	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.575	164	16294	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	35161	0.400	ng/ul	0.00
17) Chrysene-d12	21.523	240	24729	0.400	ng/ul	0.00
23) Perylene-d12	23.949	264	24777	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	58263	6.437	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	12108	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.354	212	28230	0.433	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.716	202	4424	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.794	252	8160	0.098	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042023\
Data File : BN025039.D
Acq On : 20 Apr 2023 17:26
Operator : CG/JU
Sample : PB152216BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Apr 21 04:26:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration

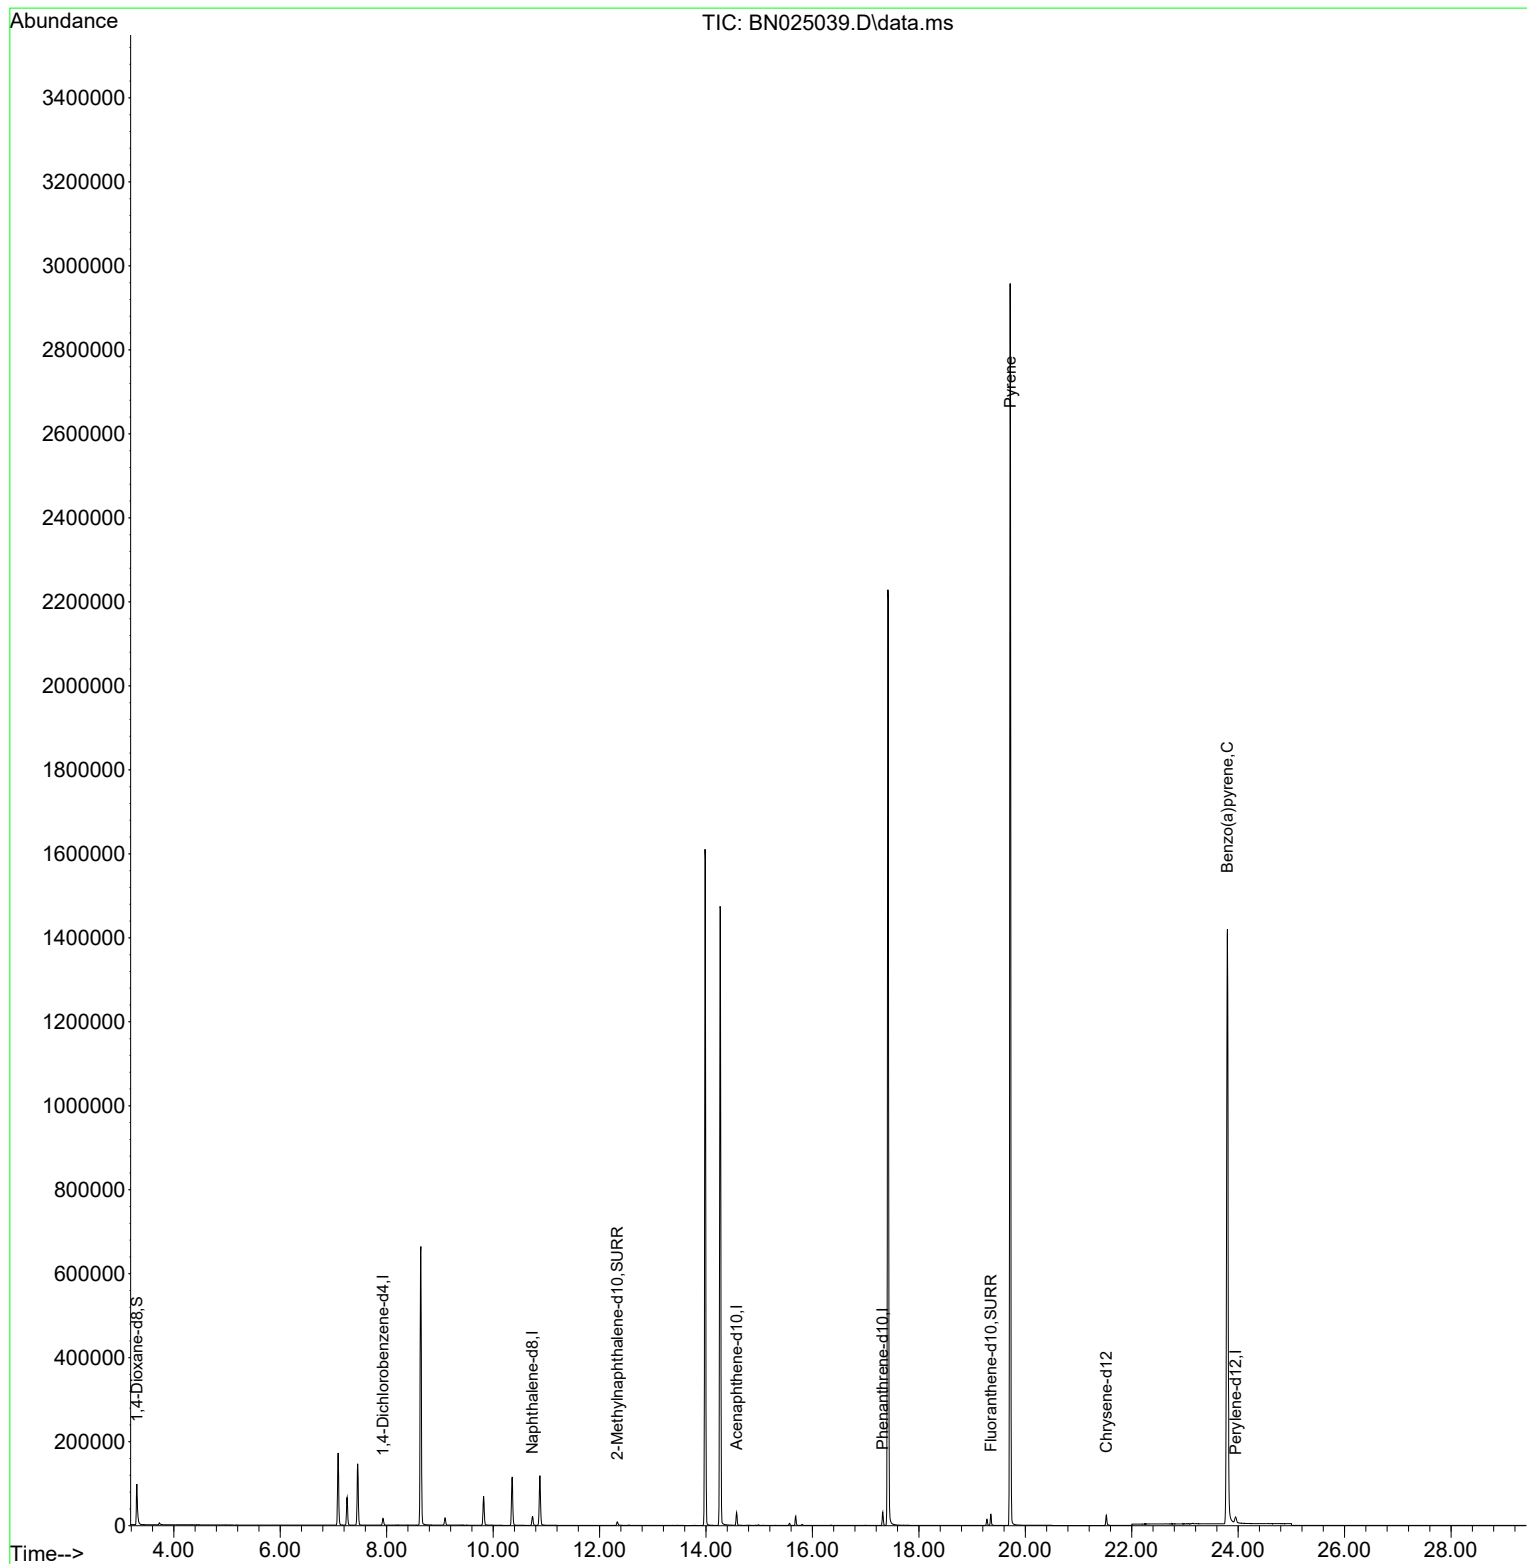



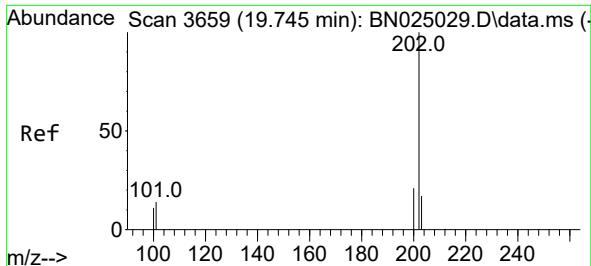


#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.716 min Scan# 3653
Delta R.T. -0.029 min
Lab File: BN025039.D
Acq: 20 Apr 2023 17:26


Instrument :
BNA_N
ClientSampleId :

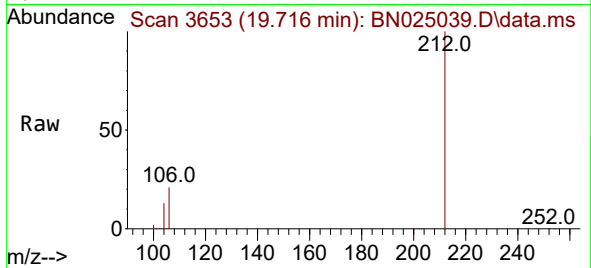

Tgt Ion:202 Resp: 4424
Ion Ratio Lower Upper
202 100
101 177.8 11.3 16.9#
100 1339.5 9.2 13.8#

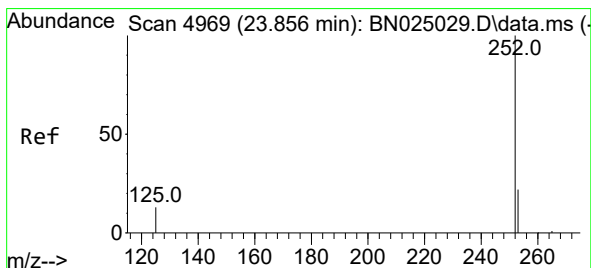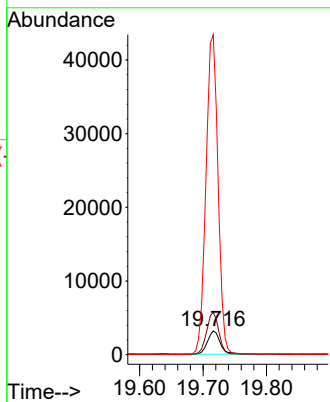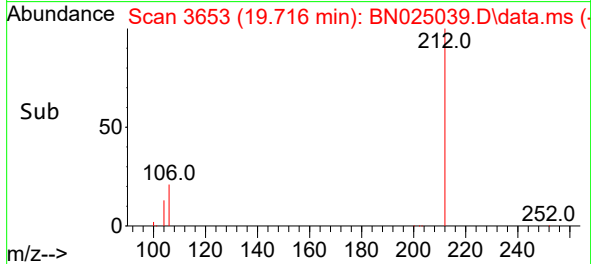

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 23.794 min Scan# 4948
Delta R.T. -0.062 min
Lab File: BN025039.D
Acq: 20 Apr 2023 17:26

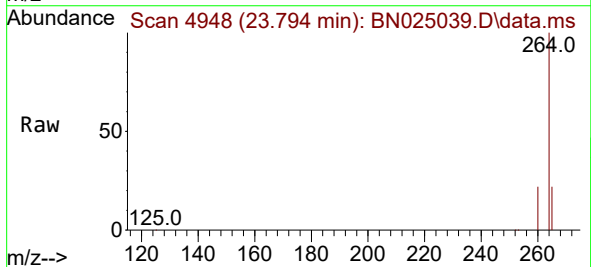

Tgt Ion:252 Resp: 8160
Ion Ratio Lower Upper
252 100
253 42.4 21.4 32.2#
125 36.8 14.6 22.0#

