

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042120\
 Data File : BN010564.D
 Acq On : 21 Apr 2020 13:44
 Operator : CG/JU
 Sample : L2338-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-DUP01-20200414

Quant Time: Apr 21 14:41:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN041320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 21 13:19:17 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	3484	0.40	ng	0.00
7) Naphthalene-d8	10.35	136	13782	0.40	ng	0.00
13) Acenaphthene-d10	14.22	164	8442	0.40	ng	0.01
19) Phenanthrene-d10	16.96	188	18830	0.40	ng	0.00
27) Chrysene-d12	21.17	240	16249	0.40	ng	0.00
34) Perylene-d12	23.35	264	15060	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.24	112	1676	0.22	ng	0.00
5) Phenol-d6	6.79	99	1350	0.14	ng	0.00
8) Nitrobenzene-d5	8.73	82	3774	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	11.95	152	8128	0.36	ng	0.00
14) 2,4,6-Tribromophenol	15.72	330	1658	0.42	ng	0.00
15) 2-Fluorobiphenyl	12.84	172	14771	0.48	ng	0.00
25) Fluoranthene-d10	19.01	212	20990	0.37	ng	0.00
29) Terphenyl-d14	19.62	244	27199	0.73	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.11	149	904	0.033	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042120\
Data File : BN010564.D
Acq On : 21 Apr 2020 13:44
Operator : CG/JU
Sample : L2338-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-DUP01-20200414

Quant Time: Apr 21 14:41:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN041320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 13:19:17 2020
Response via : Initial Calibration

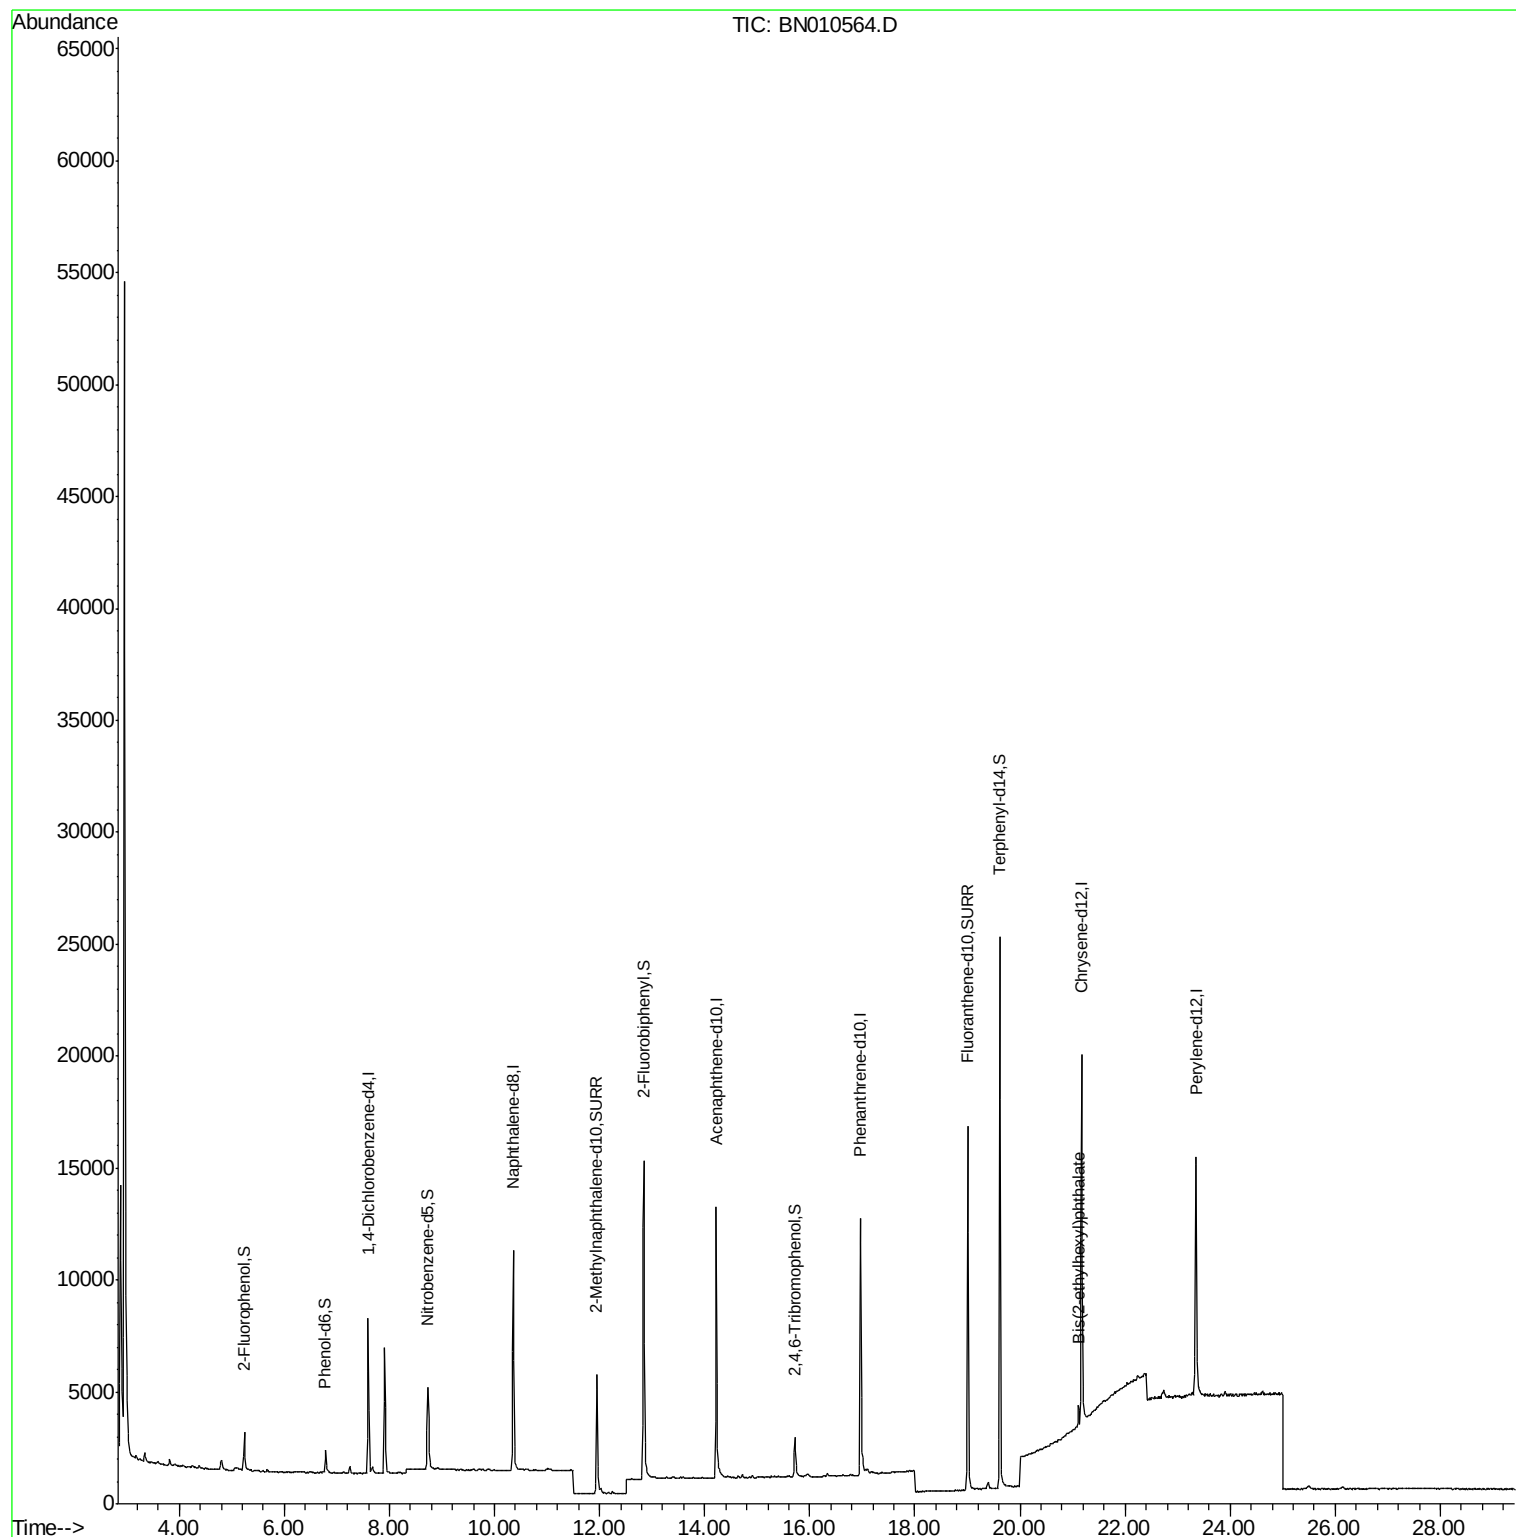




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.60 min Scan# 592
Delta R.T. 0.00 min
Lab File: BN010564.D
Acq: 21 Apr 2020 13:44

Instrument :
BNA_N
ClientSampleId :
BP-DUP01-20200414

Tot Ion:152 Resp: 3484
Ion Ratio Lower Upper
152 100
150 154.6 121.8 182.6
115 59.5 45.5 68.3

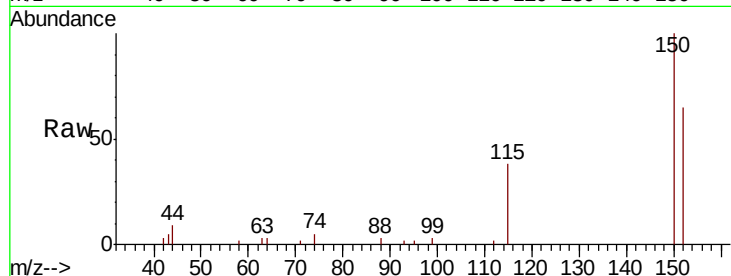


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

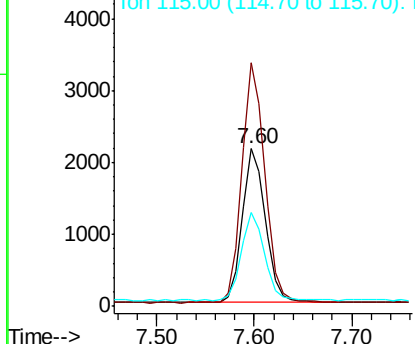



#4


2-Fluorophenol
Concen: 0.220 ng
RT: 5.24 min Scan# 299
Delta R.T. 0.00 min
Lab File: BN010564.D
Acq: 21 Apr 2020 13:44

Tgt Ion:112 Resp: 1676
Ion Ratio Lower Upper
112 100
64 44.5 35.8 53.8
63 24.9 19.9 29.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

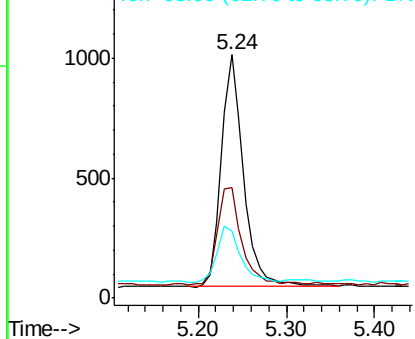



#5

Phenol-d6

Concen: 0.135 ng

RT: 6.79 min Scan# 492

Delta R.T. 0.01 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Instrument :

BNA_N

ClientSampleId :

BP-DUP01-20200414


Tot Ion: 99 Resp: 1350

Ion Ratio Lower Upper




99 100

42 16.1 9.8 14.6#

71 35.6 27.8 41.8

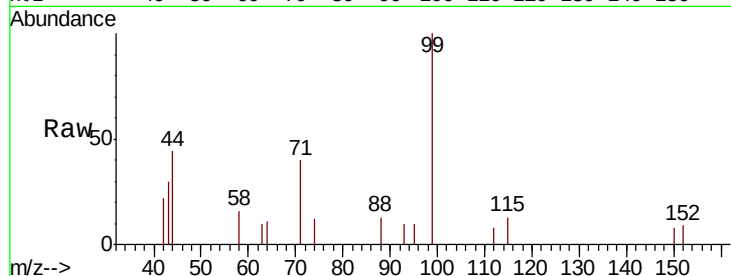

Abundance Ion 99.00 (98.70 to 99.70): BN010564.D (-479) (-)

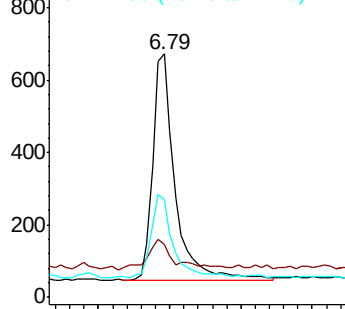

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.35 min Scan# 842

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Tgt Ion: 136 Resp: 13782


Ion Ratio Lower Upper

136 100



137 11.4 8.9 13.3


54 3.9 2.6 4.0

68 4.9 3.4 5.2



Abundance Ion 136.00 (135.70 to 136.70): BN010564.D (-826) (-)

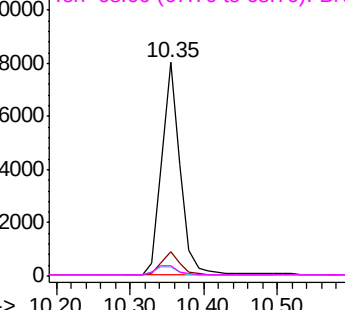



#8

Nitrobenzene-d5

Concen: 0.392 ng

RT: 8.73 min Scan# 714

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Instrument :

BNA_N

ClientSampleId :

BP-DUP01-20200414


Tot Ion: 82 Resp: 3774

Ion Ratio Lower Upper

82 100

128 41.7 41.3 61.9




54 34.1 23.4 35.0

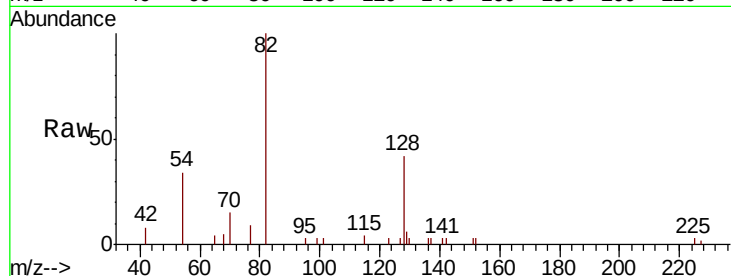

Abundance Ion 82.00 (81.70 to 82.70): BN010564.D (-706) (-)

Ion 128.00 (127.70 to 128.70): BN010564.D (-706) (-)

Ion 54.00 (53.70 to 54.70): BN010564.D (-706) (-)

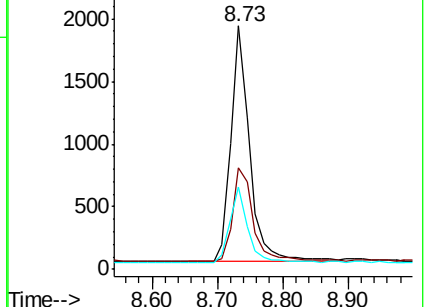

#11

2-Methylnaphthalene-d10

Concen: 0.359 ng

RT: 11.95 min Scan# 1032

Delta R.T. 0.00 min

Lab File: BN010564.D


Acq: 21 Apr 2020 13:44

Tgt Ion: 152 Resp: 8128

Ion Ratio Lower Upper



152 100


151 18.9 15.3 22.9



Abundance Ion 152.00 (151.70 to 152.70): BN010564.D (-987) (-)

Ion 151.00 (150.70 to 151.70): BN010564.D (-987) (-)

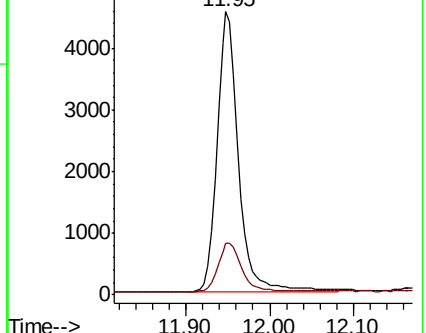

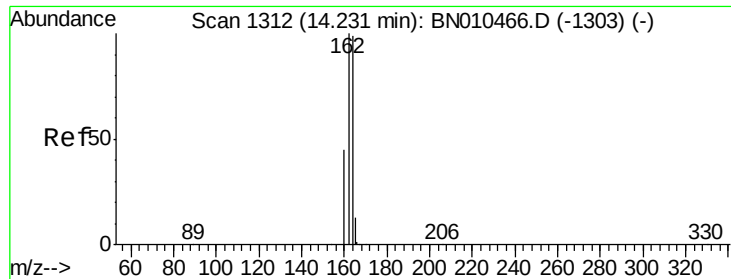

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.22 min Scan# 1312

Delta R.T. 0.01 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Instrument :

BNA_N

ClientSampleId :

BP-DUP01-20200414


Tot Ion:164 Resp: 8442

Ion Ratio Lower Upper

164 100

162 100.3 80.6 121.0




160 46.7 36.5 54.7



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

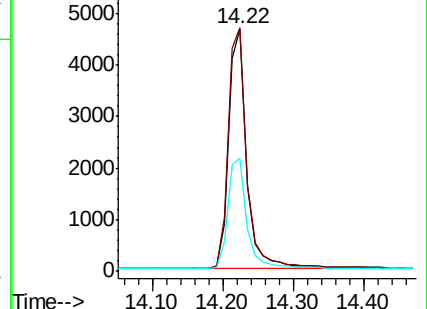

#14

2,4,6-Tribromophenol

Concen: 0.417 ng

RT: 15.72 min Scan# 1446

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44


Tgt Ion:330 Resp: 1658

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 36.2 28.1 42.1




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



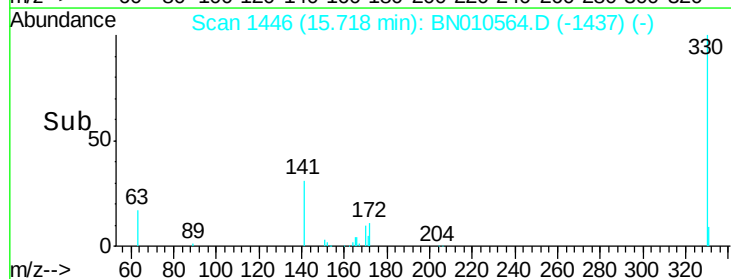
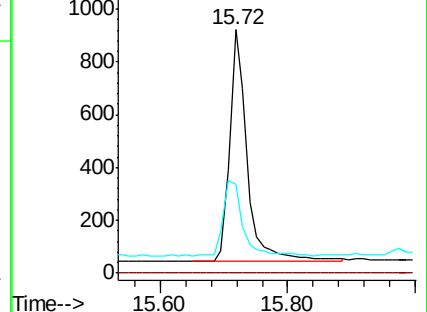




#15
2-Fluorobiphenyl
Concen: 0.481 ng
RT: 12.84 min Scan# 1188
Delta R.T. 0.00 min
Lab File: BN010564.D
Acq: 21 Apr 2020 13:44




Instrument :
BNA_N
ClientSampleId :
BP-DUP01-20200414


Tot Ion:172 Resp: 14771
Ion Ratio Lower Upper
172 100
171 34.6 28.2 42.2
170 23.0 18.4 27.6

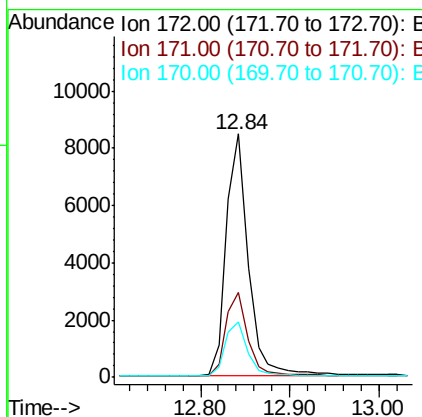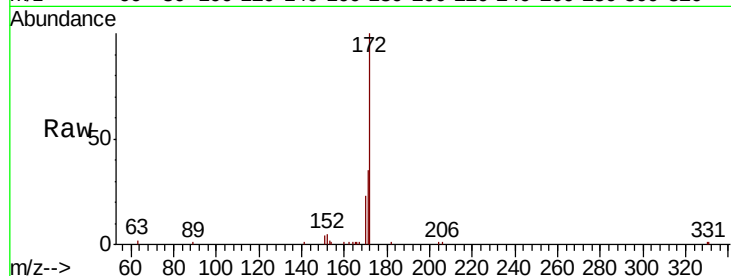

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.96 min Scan# 1562
Delta R.T. 0.00 min
Lab File: BN010564.D
Acq: 21 Apr 2020 13:44

Tgt Ion:188 Resp: 18830
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.6 5.0 7.6#

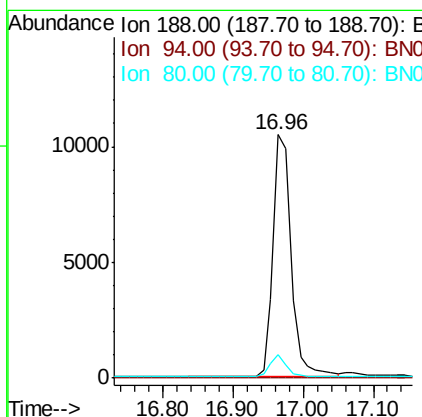

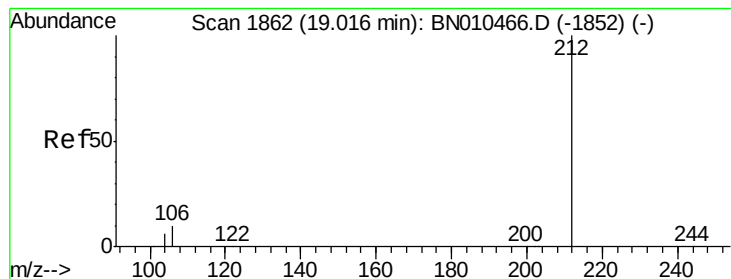

#25

Fluoranthene-d10

Concen: 0.368 ng

RT: 19.01 min Scan# 1862

Delta R.T. 0.01 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Instrument :

BNA_N

ClientSampleId :

BP-DUP01-20200414


Tot Ion:212 Resp: 20990

Ion Ratio Lower Upper

212 100

106 9.6 7.8 11.6




104 5.6 4.5 6.7



Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

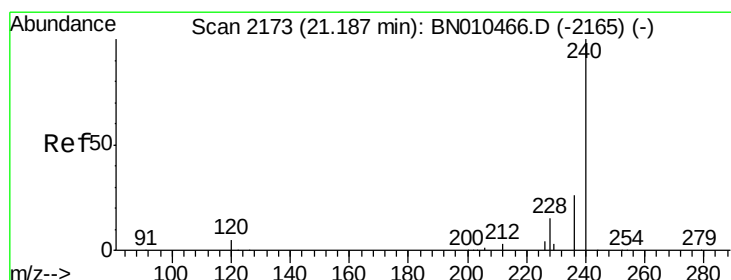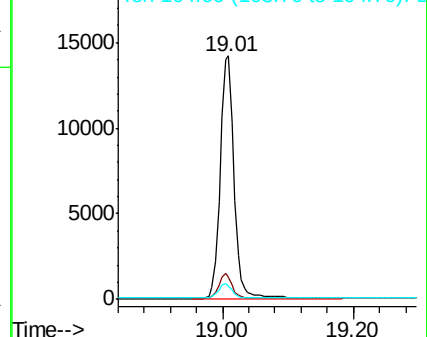

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.17 min Scan# 2173

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44


Tgt Ion:240 Resp: 16249

Ion Ratio Lower Upper

240 100

120 7.9 4.8 7.2#



236 27.3 21.4 32.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

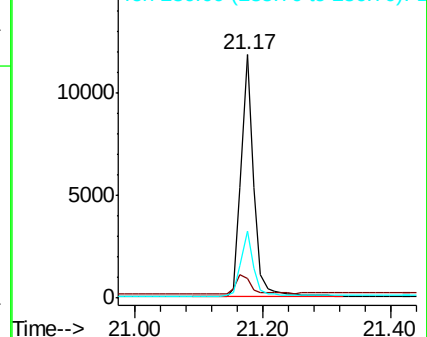

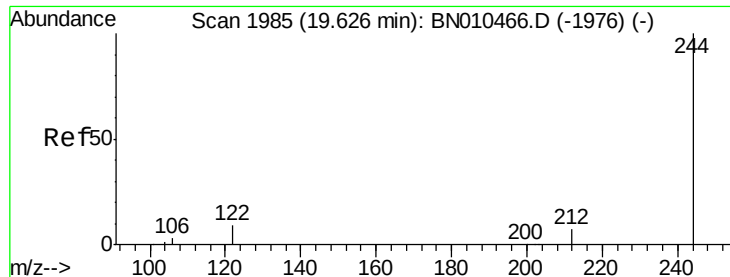

#29

Terphenyl-d14

Concen: 0.731 ng

RT: 19.62 min Scan# 1985

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Instrument :

BNA_N

ClientSampleId :

BP-DUP01-20200414


Tot Ion:244 Resp: 27199

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.4

122 8.9 7.8 11.8

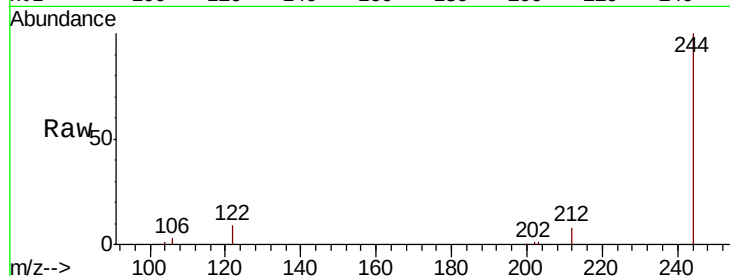


Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

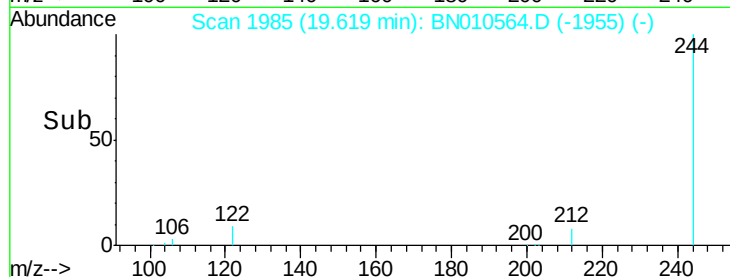

Time-->

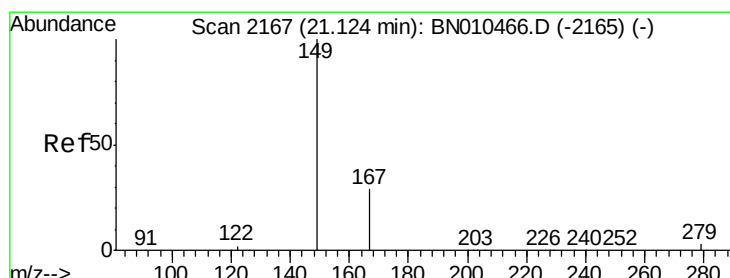

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.033 ng

RT: 21.11 min Scan# 2167

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44


Tgt Ion:149 Resp: 904

Ion Ratio Lower Upper

149 100

167 27.2 23.4 35.0

279 6.7 4.0 6.0#

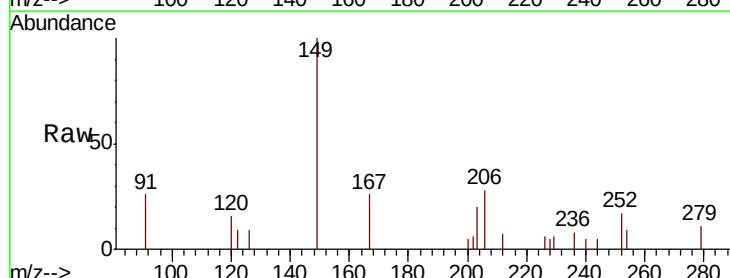


Abundance Ion 149.00 (148.70 to 149.70): E




Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

Time-->

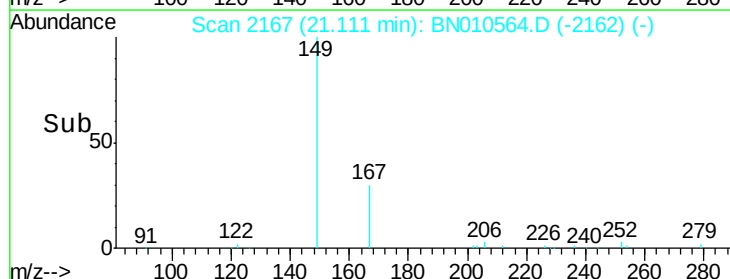

Time-->

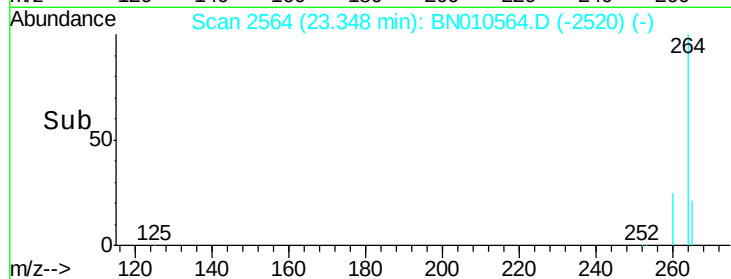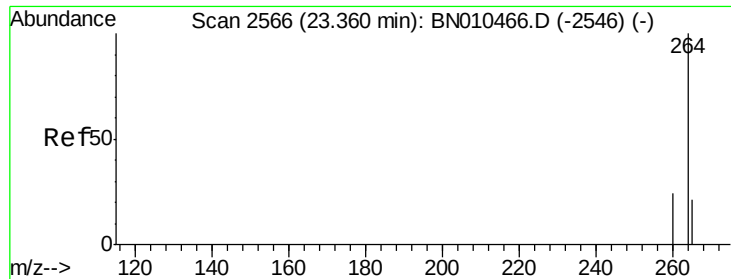

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.35 min Scan# 2564

Delta R.T. 0.00 min

Lab File: BN010564.D

Acq: 21 Apr 2020 13:44

Instrument :

BNA_N

ClientSampleId :

BP-DUP01-20200414

Tot Ion: 264 Resp: 15060

Ion Ratio Lower Upper

264 100

260 25.1 19.8 29.8

265 62.6 42.3 63.5

