


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042120\
 Data File : BN010559.D
 Acq On : 21 Apr 2020 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 21 13:19:17 2020

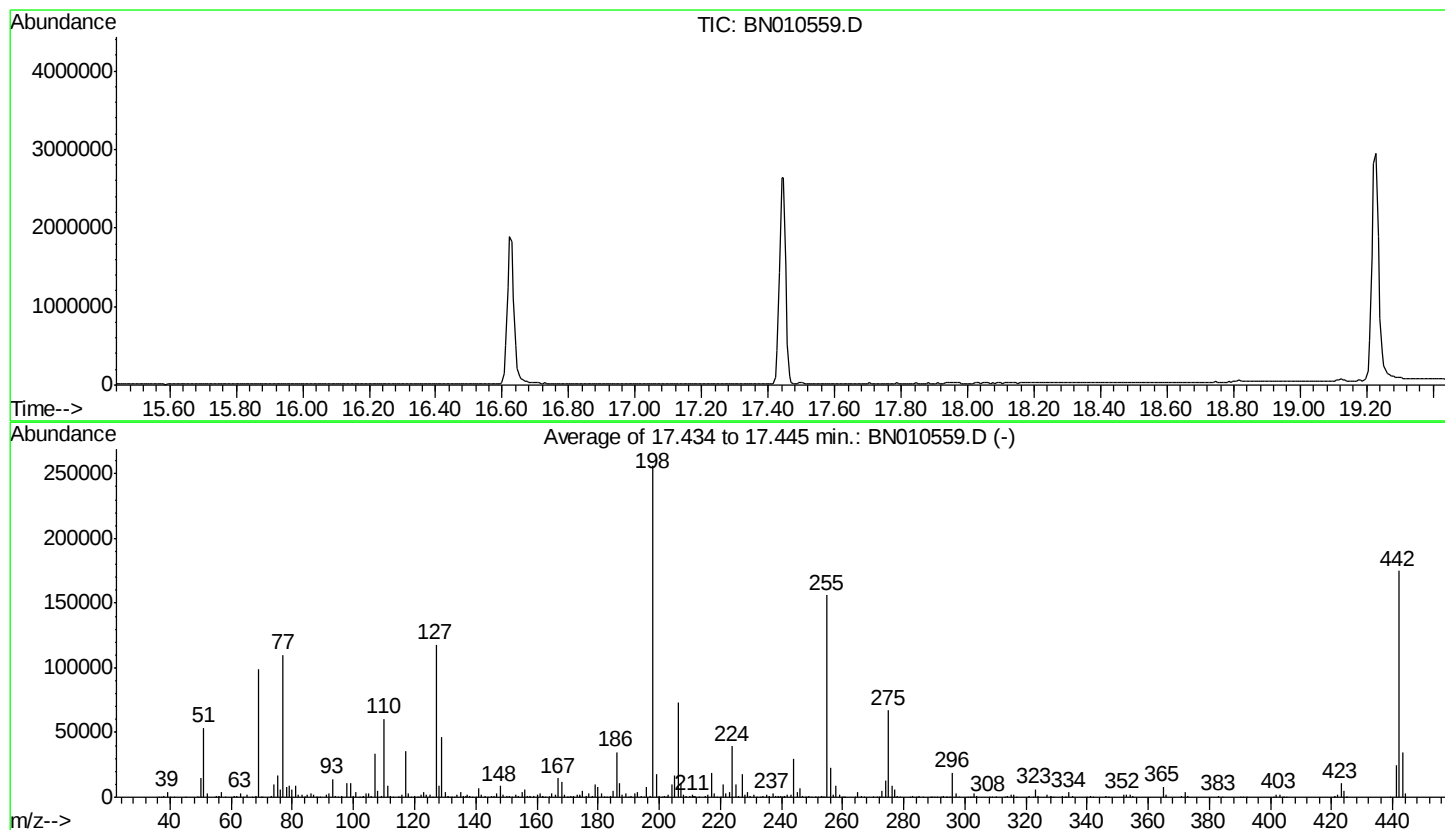

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	53736	PASS
68	69	0.00	2	1.3	1325	PASS
69	198	0.00	100	38.7	99090	PASS
70	69	0.00	2	0.2	242	PASS
127	198	10	80	46.0	117904	PASS
197	198	0.00	2	0.4	974	PASS
198	198	100	100	100.0	256320	PASS
199	198	5	9	7.0	18014	PASS
275	198	10	60	26.1	66962	PASS
365	198	1	100	3.3	8385	PASS
441	198	0.01	100	9.9	25262	PASS
442	198	50	100	68.3	175098	PASS
443	442	15	24	19.8	34625	PASS