

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
 Data File : BN025048.D
 Acq On : 21 Apr 2023 10:29
 Operator : CG/JU
 Sample : PB152233BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK233

Quant Time: Apr 22 00:15:48 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	7723	0.400	ng/ul	0.00
4) Naphthalene-d8	10.737	136	24910	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.575	164	14679	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	31120	0.400	ng/ul	0.00
17) Chrysene-d12	21.517	240	21497	0.400	ng/ul	0.00
23) Perylene-d12	23.958	264	21998	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	52658	6.585	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	10981	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	23464	0.414	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.565	166	3943	0.077	ng/ul#	13
20) Pyrene	19.712	202	3828	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.806	252	7545	0.102	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
Data File : BN025048.D
Acq On : 21 Apr 2023 10:29
Operator : CG/JU
Sample : PB152233BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK233

Quant Time: Apr 22 00:15:48 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration




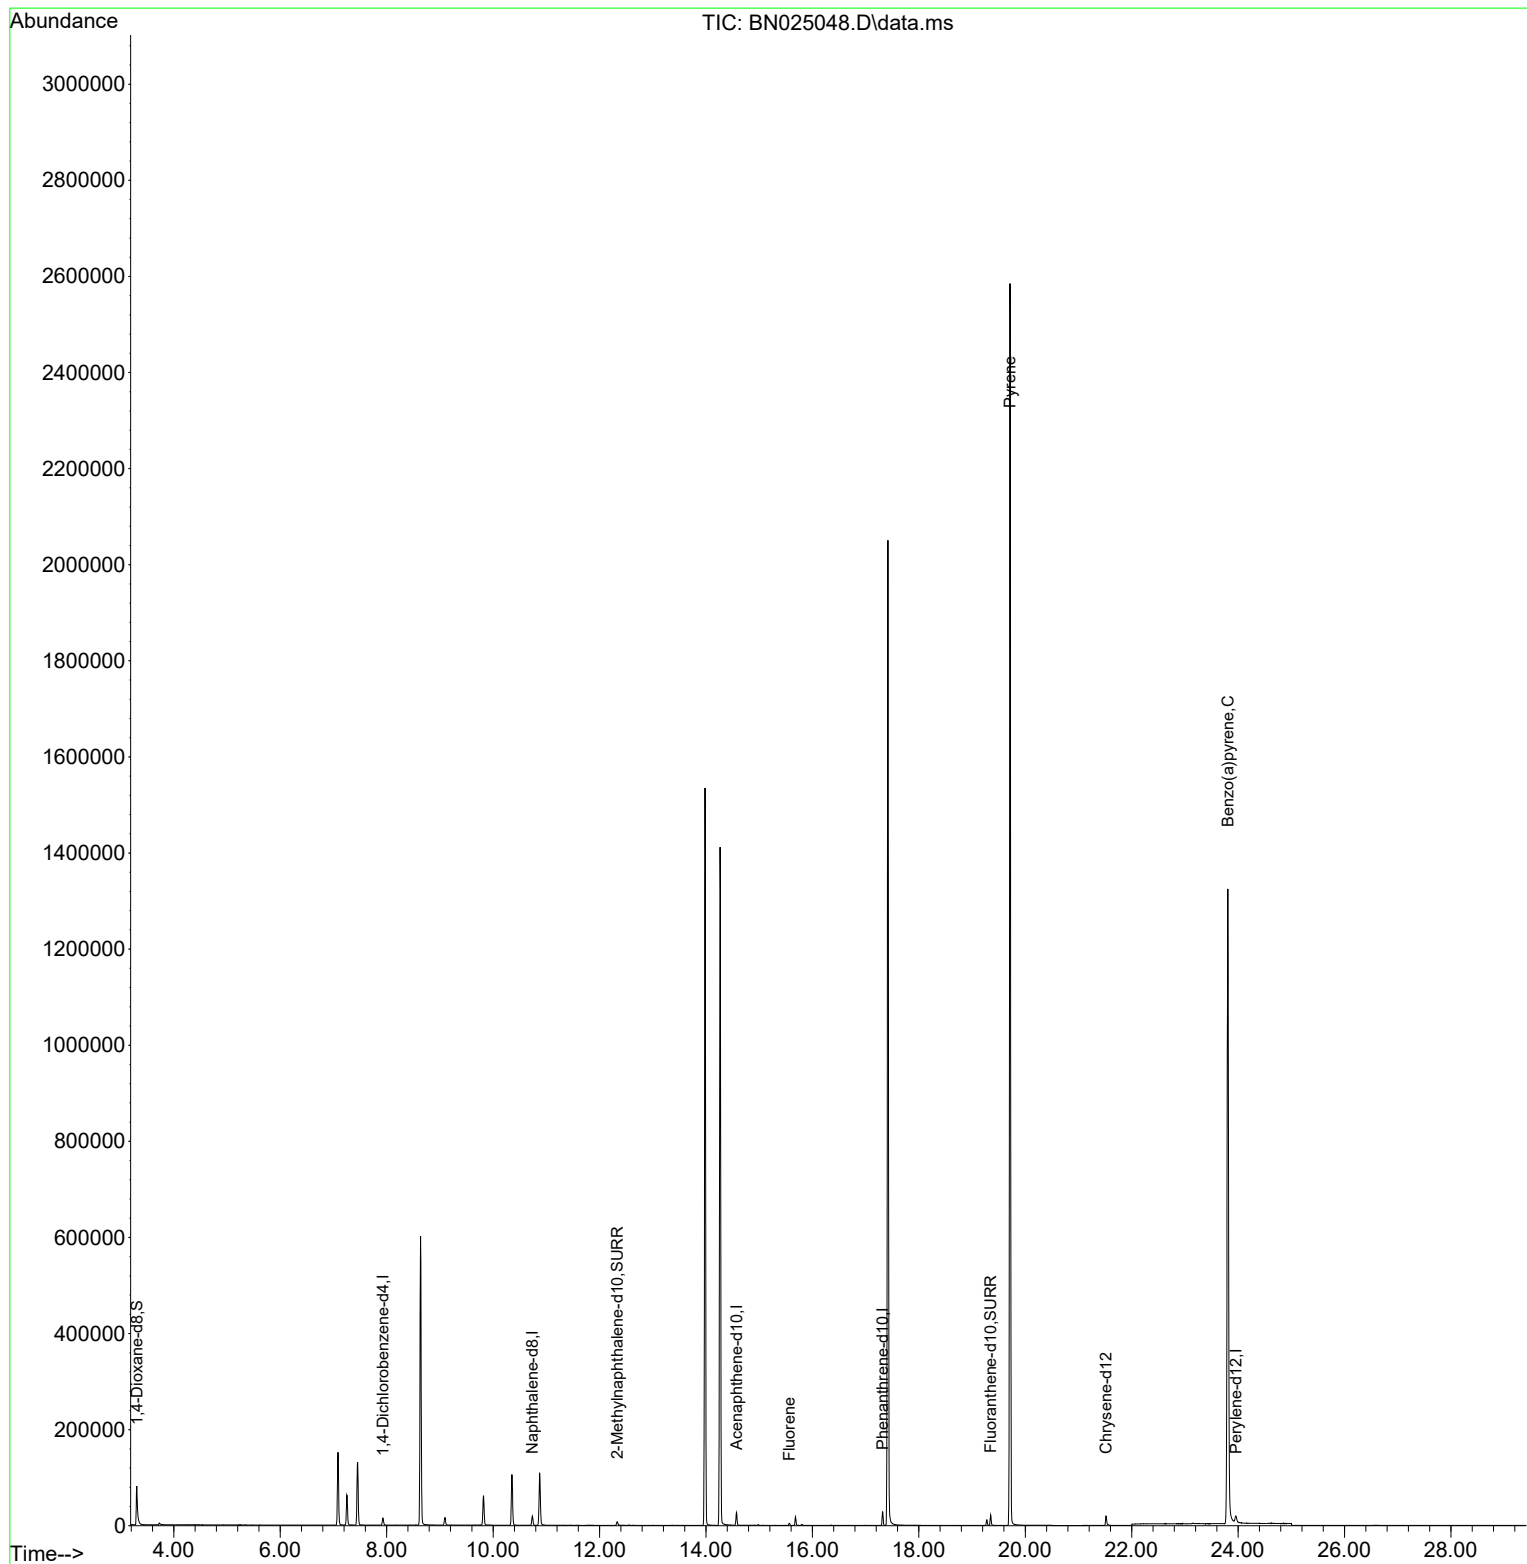


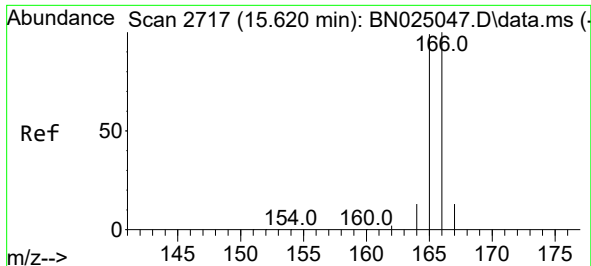

#12
Fluorene
Concen: 0.077 ng/ul
RT: 15.565 min Scan# 21
Delta R.T. -0.061 min
Lab File: BN025048.D
Acq: 21 Apr 2023 10:29




Instrument :
BNA_N
ClientSampleId :
SBLK233


Tgt Ion:166 Resp: 3943
Ion Ratio Lower Upper
166 100
165 6.7 78.1 117.1#
167 33.8 11.0 16.6#

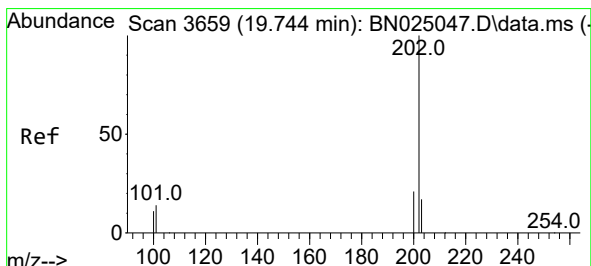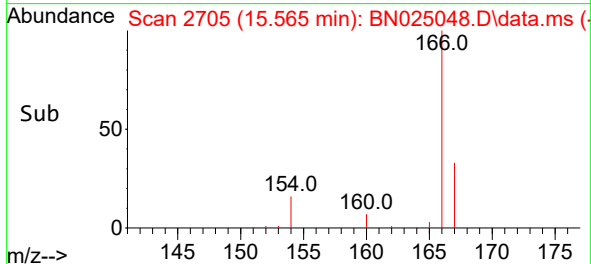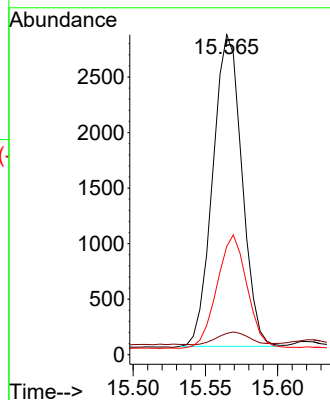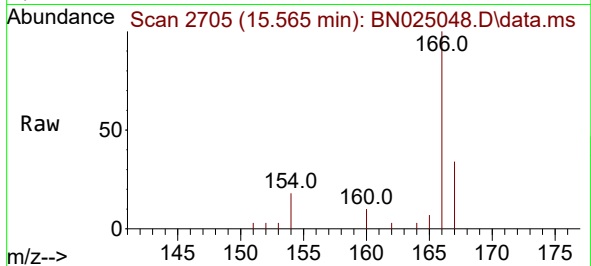

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.712 min Scan# 3652
Delta R.T. -0.033 min
Lab File: BN025048.D
Acq: 21 Apr 2023 10:29


Tgt Ion:202 Resp: 3828
Ion Ratio Lower Upper
202 100
101 184.3 11.3 16.9#
100 1411.8 9.2 13.8#

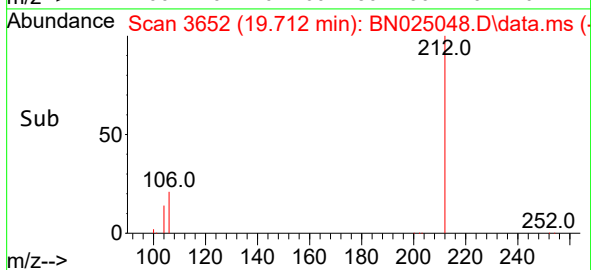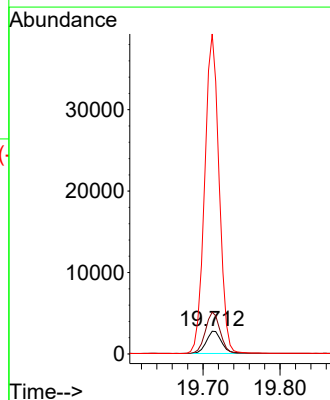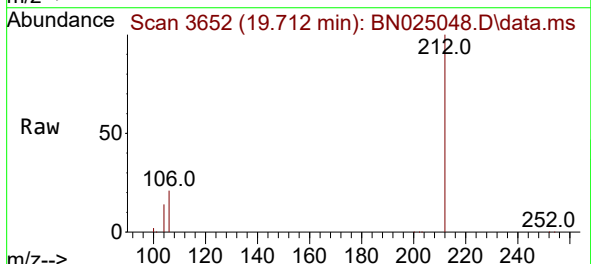

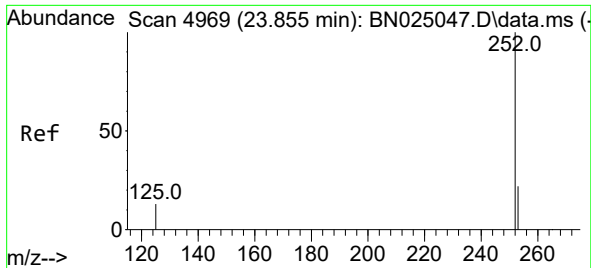

#26
 Benzo(a)pyrene
 Concen: 0.102 ng/ul
 RT: 23.806 min Scan# 4952
 Delta R.T. -0.050 min
 Lab File: BN025048.D
 Acq: 21 Apr 2023 10:29

Instrument :
 BNA_N
 ClientSampleId :
 SBLK233

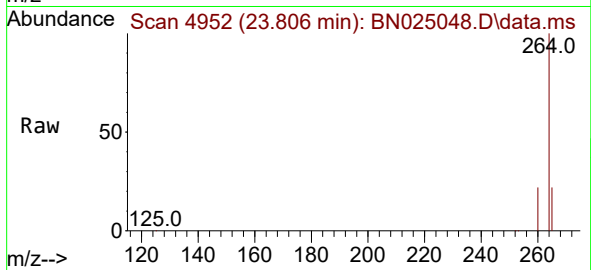

Tgt Ion:252 Resp: 7545
 Ion Ratio Lower Upper
 252 100
 253 43.7 21.4 32.2#
 125 37.4 14.6 22.0#

