

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
 Data File : BN025054.D
 Acq On : 21 Apr 2023 14:03
 Operator : CG/JU
 Sample : 02340-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE19

Quant Time: Apr 22 00:16:31 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	7103	0.400	ng/ul	0.00
4) Naphthalene-d8	10.736	136	22356	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.574	164	13750	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	30188	0.400	ng/ul	0.00
17) Chrysene-d12	21.513	240	22329	0.400	ng/ul	0.00
23) Perylene-d12	23.954	264	21546	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	43113	5.862	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.331	152	13042	0.454	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	37145	0.631	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	8948	1.130	ng/ul	94
20) Pyrene	19.716	202	5360	0.065	ng/ul#	1
26) Benzo(a)pyrene	23.805	252	9466	0.131	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
Data File : BN025054.D
Acq On : 21 Apr 2023 14:03
Operator : CG/JU
Sample : 02340-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE19

Quant Time: Apr 22 00:16:31 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration




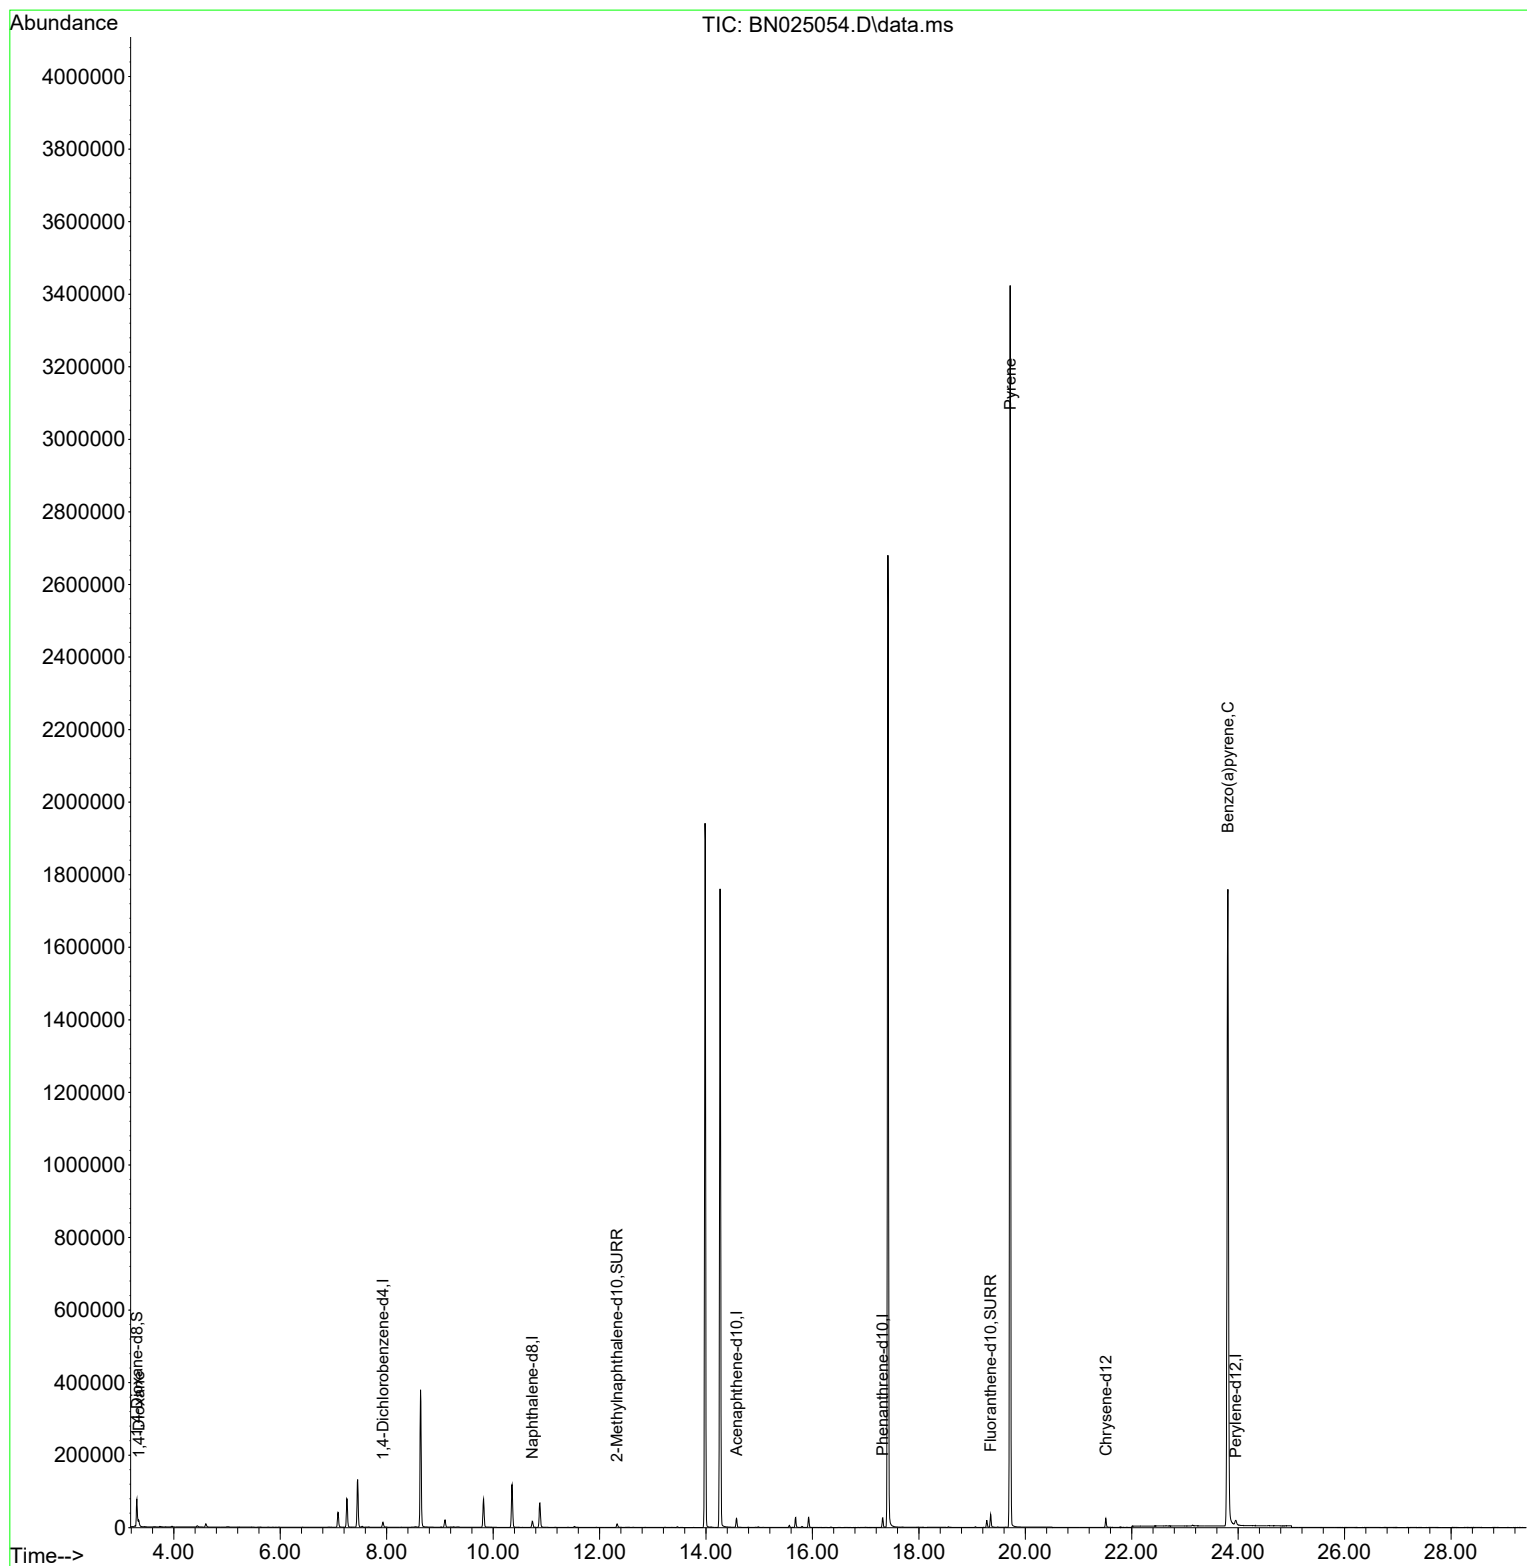


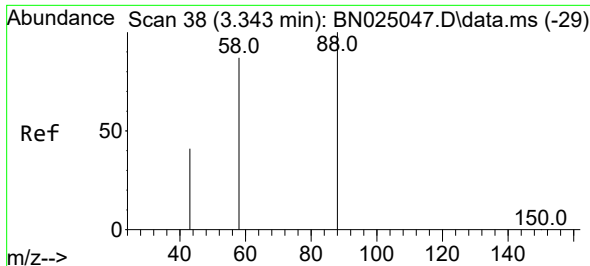

#2
1,4-Dioxane
Concen: 1.130 ng/ul
RT: 3.343 min Scan# 38
Delta R.T. 0.000 min
Lab File: BN025054.D
Acq: 21 Apr 2023 14:03




Instrument :
BNA_N
ClientSampleId :
BHE19


Tgt Ion: 88 Resp: 8948
Ion Ratio Lower Upper
88 100
43 44.8 37.0 55.4
58 78.8 56.9 85.3

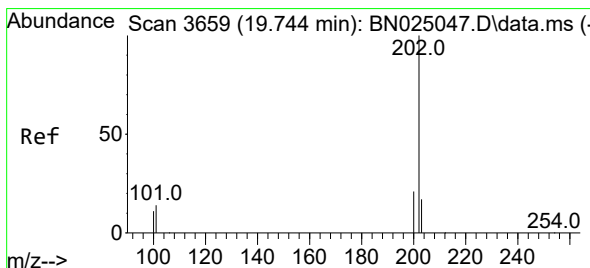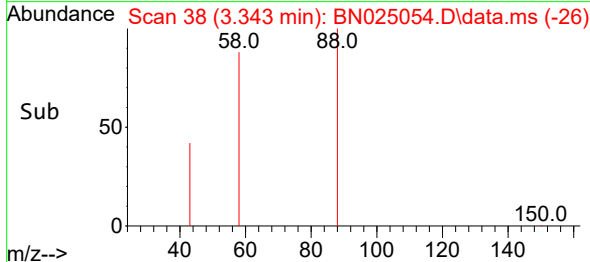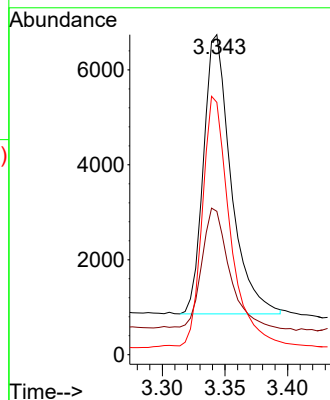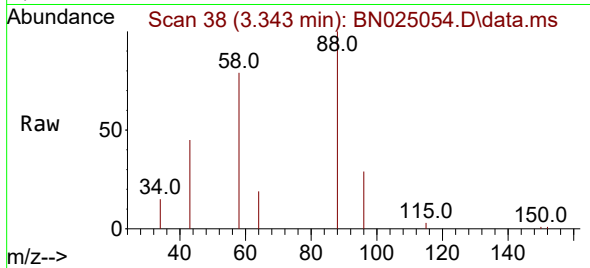

#20
Pyrene
Concen: 0.065 ng/ul
RT: 19.716 min Scan# 3653
Delta R.T. -0.029 min
Lab File: BN025054.D
Acq: 21 Apr 2023 14:03


Tgt Ion: 202 Resp: 5360
Ion Ratio Lower Upper
202 100
101 174.9 11.3 16.9#
100 1270.7 9.2 13.8#

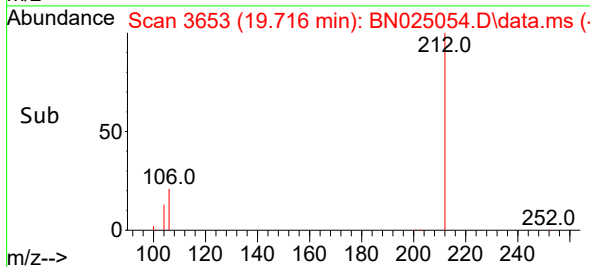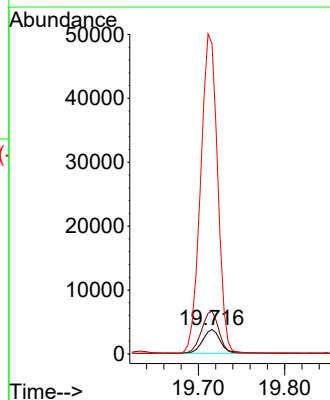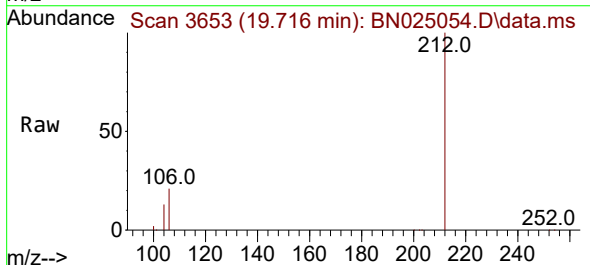

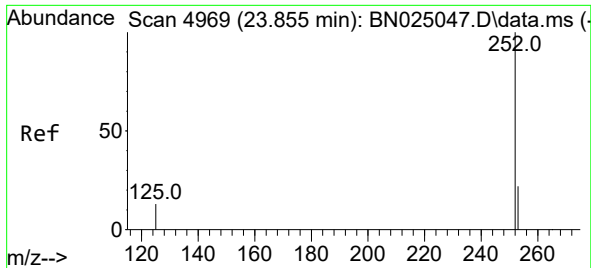

#26
Benzo(a)pyrene
Concen: 0.131 ng/ul
RT: 23.805 min Scan# 4969
Delta R.T. -0.051 min
Lab File: BN025054.D
Acq: 21 Apr 2023 14:03

Instrument :
BNA_N
ClientSampleId :
BHE19

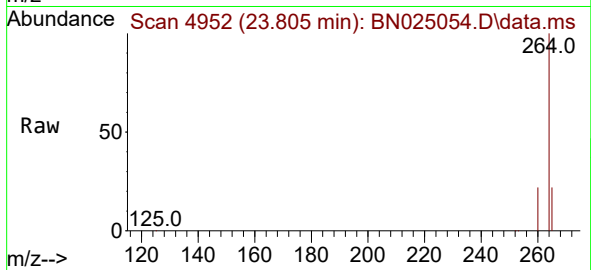

Tgt Ion:252 Resp: 9466
Ion Ratio Lower Upper
252 100
253 41.7 21.4 32.2#
125 35.8 14.6 22.0#

