

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
 Data File : BN025062.D
 Acq On : 21 Apr 2023 18:50
 Operator : CG/JU
 Sample : PB152280BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK280

Quant Time: Apr 22 00:17:45 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	6755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.737	136	21937	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.570	164	12788	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188	26604	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	17664	0.400	ng/ul	0.00
23) Perylene-d12	23.960	264	18223	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	56324	8.053	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	11629	0.413	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	24519	0.526	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.565	166	4141	0.092	ng/ul#	14
20) Pyrene	19.711	202	3903	0.059	ng/ul#	1
26) Benzo(a)pyrene	23.808	252	7020	0.115	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
Data File : BN025062.D
Acq On : 21 Apr 2023 18:50
Operator : CG/JU
Sample : PB152280BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK280

Quant Time: Apr 22 00:17:45 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration




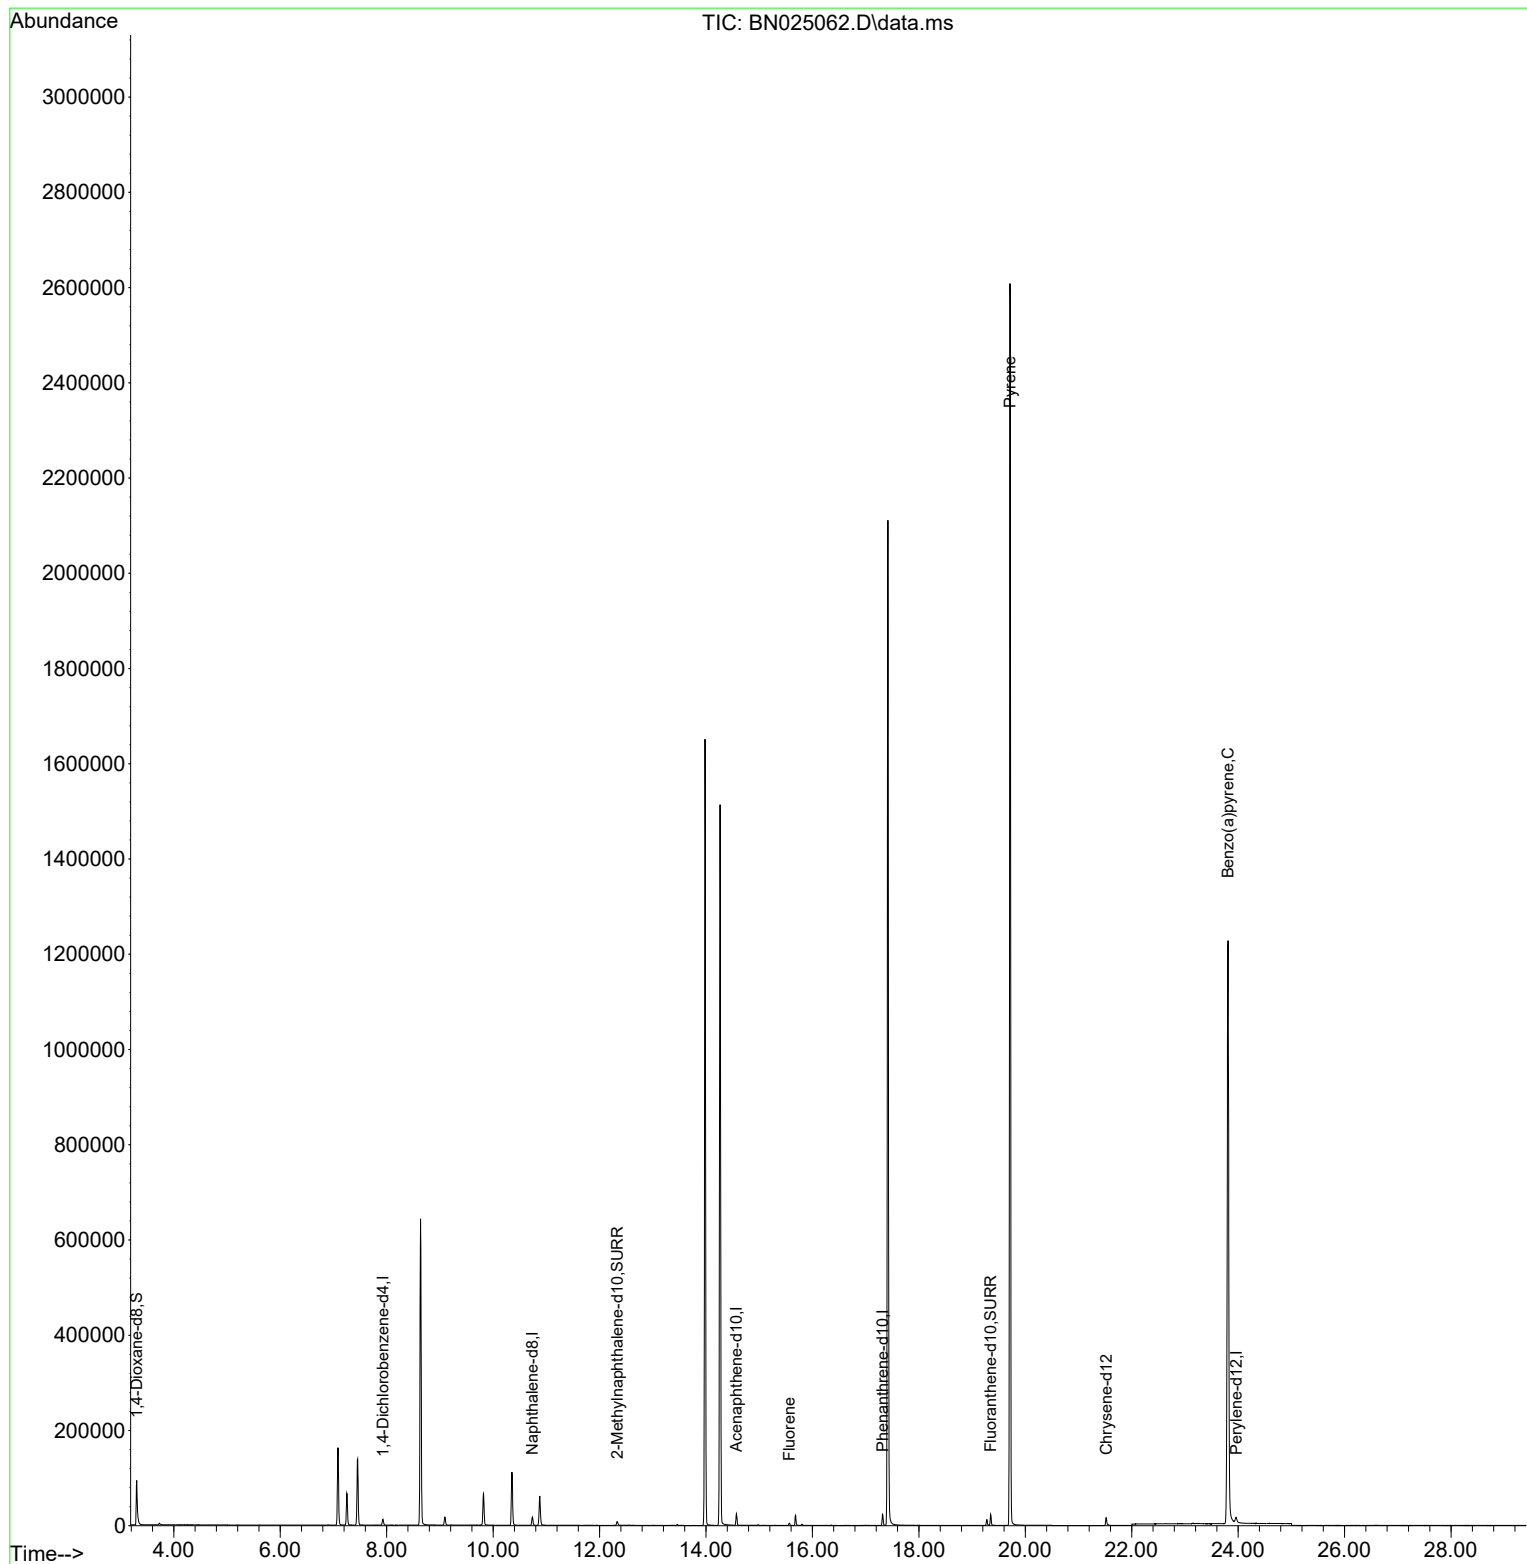


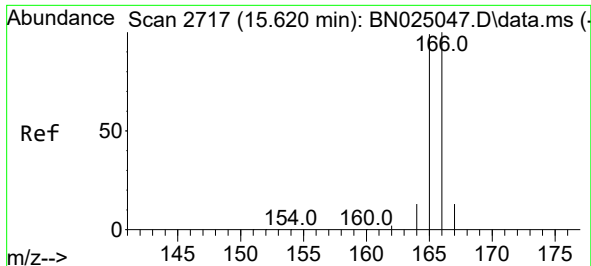

#12
Fluorene
Concen: 0.092 ng/ul
RT: 15.565 min Scan# 21
Delta R.T. -0.061 min
Lab File: BN025062.D
Acq: 21 Apr 2023 18:50




Instrument :
BNA_N
ClientSampleId :
SBLK280


Tgt Ion:166 Resp: 4141
Ion Ratio Lower Upper
166 100
165 7.0 78.1 117.1#
167 33.3 11.0 16.6#

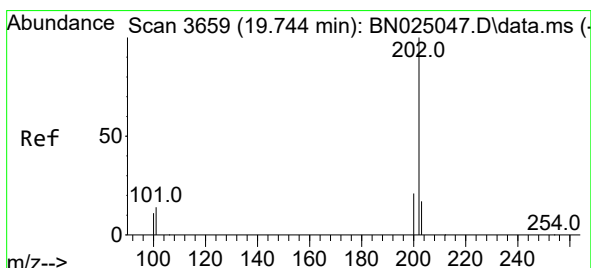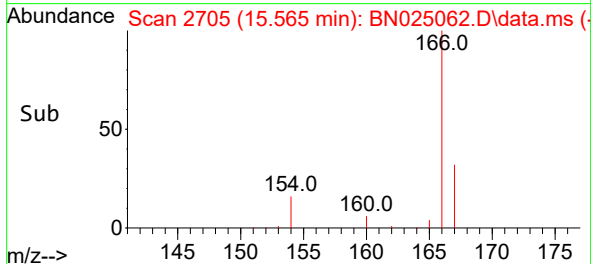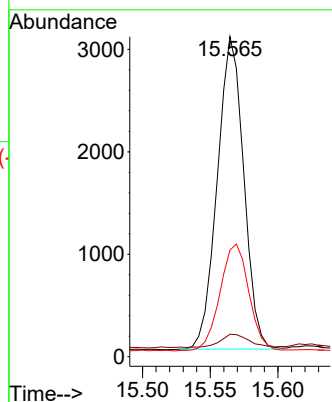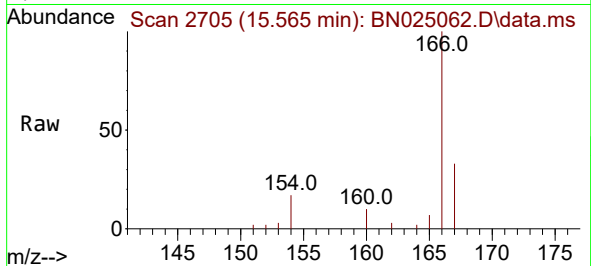

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.711 min Scan# 3652
Delta R.T. -0.033 min
Lab File: BN025062.D
Acq: 21 Apr 2023 18:50


Tgt Ion:202 Resp: 3903
Ion Ratio Lower Upper
202 100
101 184.5 11.3 16.9#
100 1414.4 9.2 13.8#

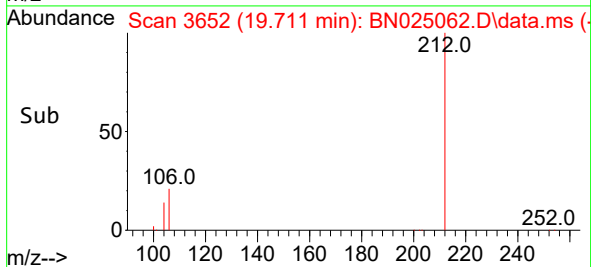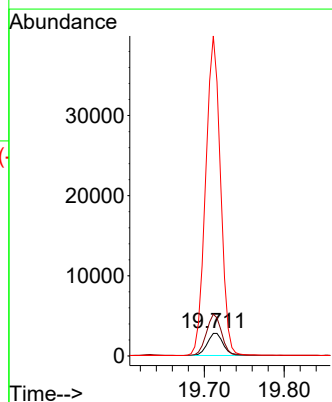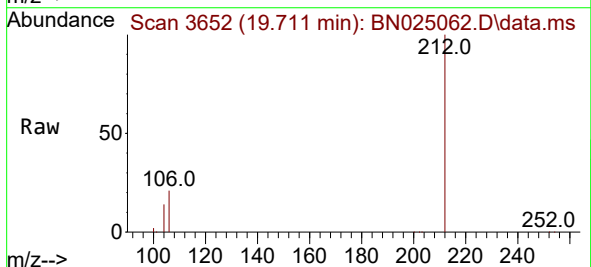

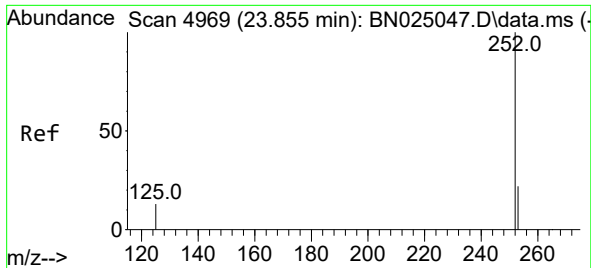

#26
 Benzo(a)pyrene
 Concen: 0.115 ng/ul
 RT: 23.808 min Scan# 4953
 Delta R.T. -0.048 min
 Lab File: BN025062.D
 Acq: 21 Apr 2023 18:50

Instrument :
 BNA_N
 ClientSampleId :
 SBLK280

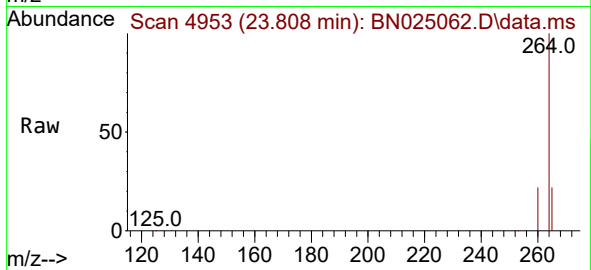

Tgt Ion:252 Resp: 7020
 Ion Ratio Lower Upper
 252 100
 253 44.1 21.4 32.2#
 125 36.9 14.6 22.0#

