

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
 Data File : BN025050.D
 Acq On : 21 Apr 2023 11:41
 Operator : CG/JU
 Sample : 02340-14
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE15

Quant Time: Apr 22 00:16:06 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	7217	0.400	ng/ul	0.00
4) Naphthalene-d8	10.736	136	23197	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.574	164	13689	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	29103	0.400	ng/ul	0.00
17) Chrysene-d12	21.516	240	21423	0.400	ng/ul	0.00
23) Perylene-d12	23.960	264	20838	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	30963	4.143	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.331	152	10189	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	24365	0.431	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	1284	0.160	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
Data File : BN025050.D
Acq On : 21 Apr 2023 11:41
Operator : CG/JU
Sample : 02340-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE15


Quant Time: Apr 22 00:16:06 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration

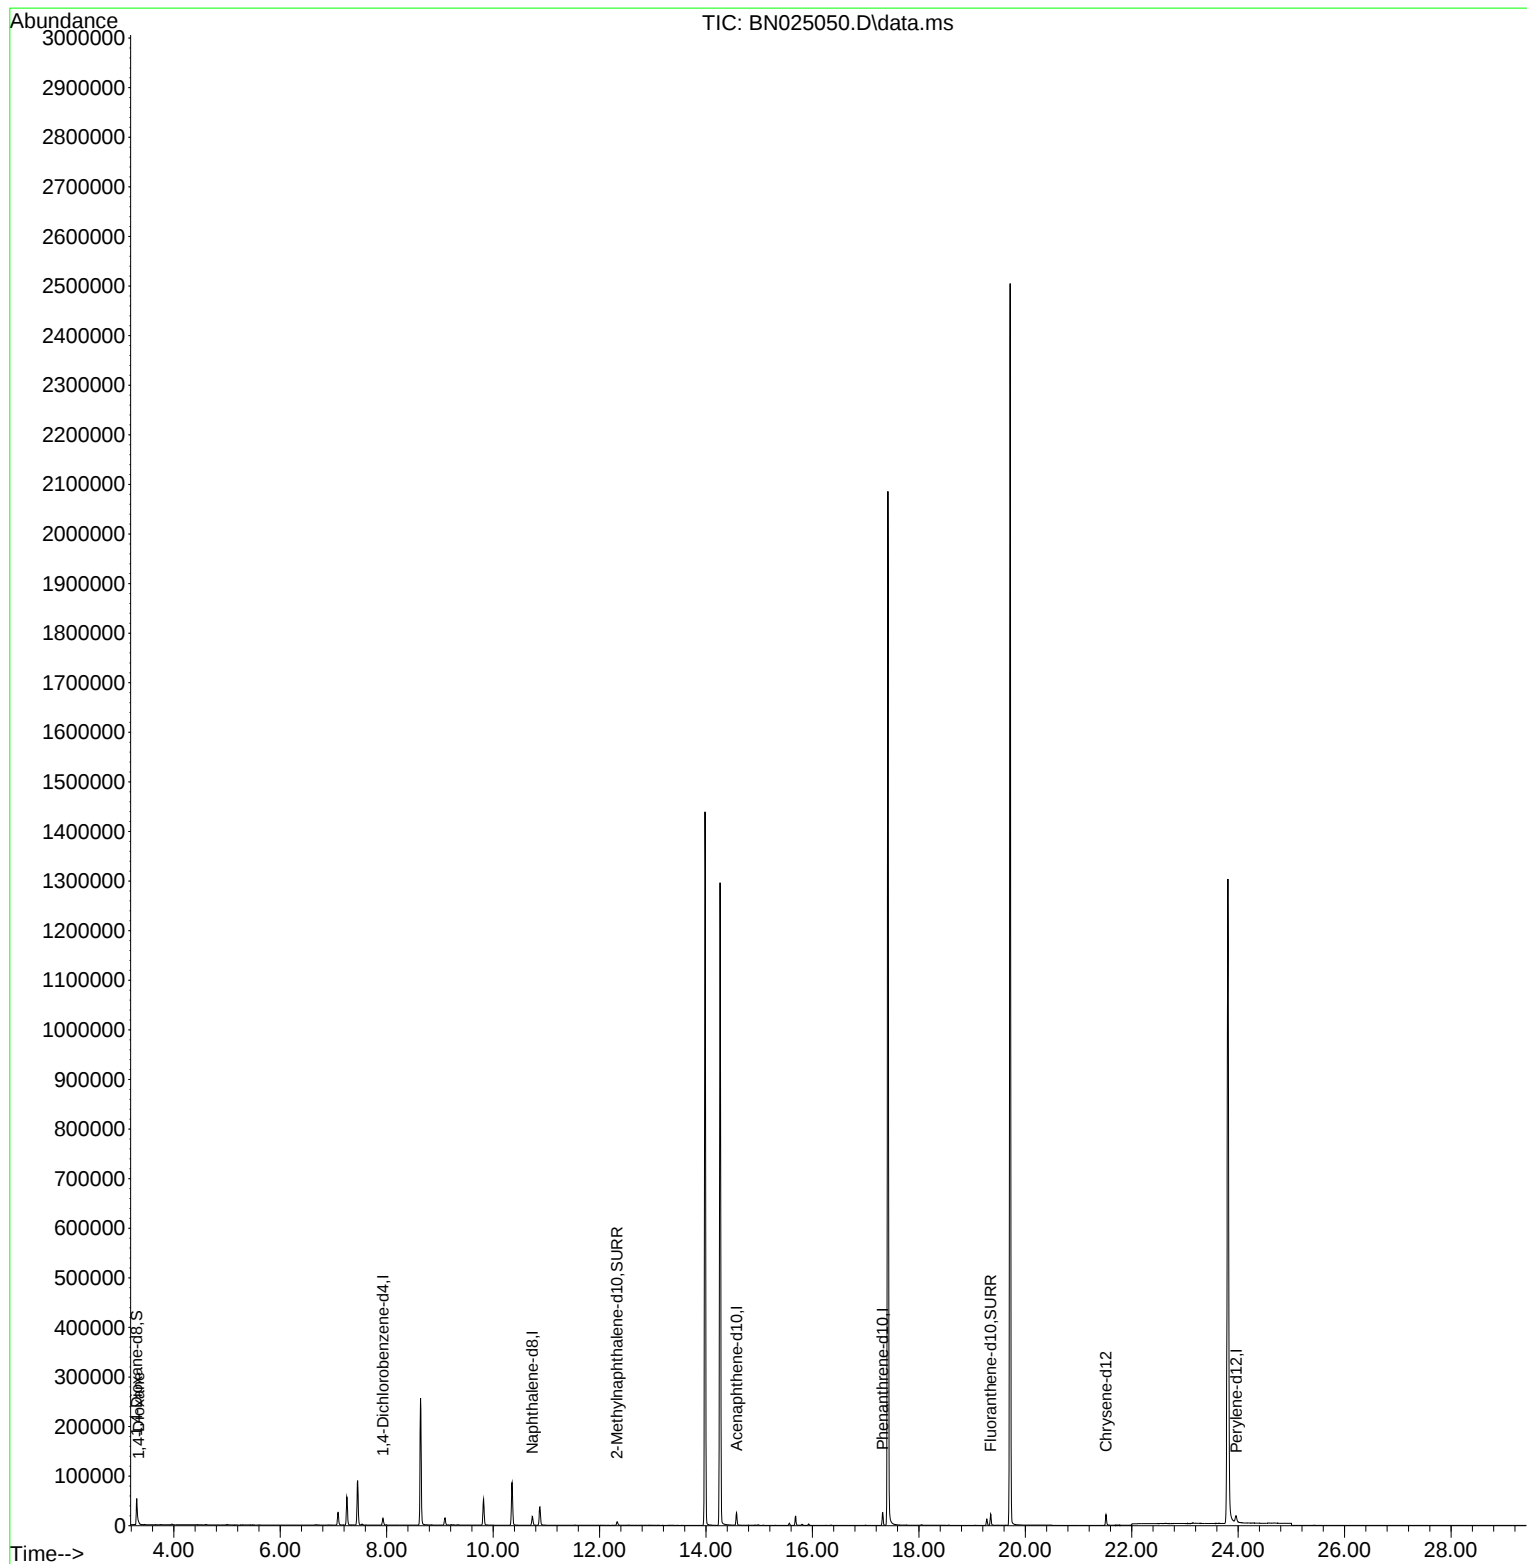

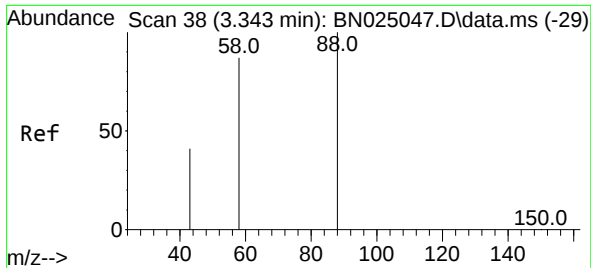

#2
 1,4-Dioxane
 Concen: 0.160 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN025050.D
 Acq: 21 Apr 2023 11:41

Instrument :
 BNA_N
 ClientSampleId :
 BHE15

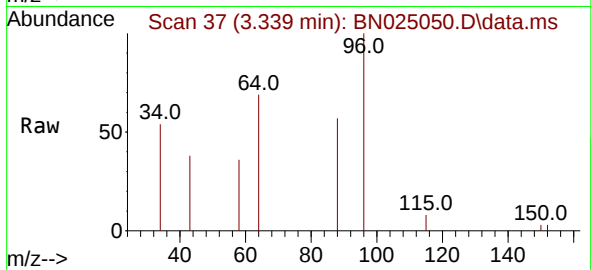

Tgt Ion: 88 Resp: 1284

Ion	Ratio	Lower	Upper
88	100		
43	67.9	37.0	55.4#
58	64.4	56.9	85.3

