

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
 Data File : BN025052.D
 Acq On : 21 Apr 2023 12:52
 Operator : CG/JU
 Sample : 02340-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE20

Quant Time: Apr 22 00:16:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	8674	0.400	ng/u1	0.00
4) Naphthalene-d8	10.737	136	27268	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.575	164	16647	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.321	188	35544	0.400	ng/u1	0.00
17) Chrysene-d12	21.514	240	26532	0.400	ng/u1	0.00
23) Perylene-d12	23.954	264	25280	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	50106	5.579	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.332	152	13976	0.399	ng/u1	0.00
18) Fluoranthene-d10	19.349	212	36188	0.517	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	17354	1.794	ng/u1	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
Data File : BN025052.D
Acq On : 21 Apr 2023 12:52
Operator : CG/JU
Sample : 02340-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE20

Quant Time: Apr 22 00:16:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration

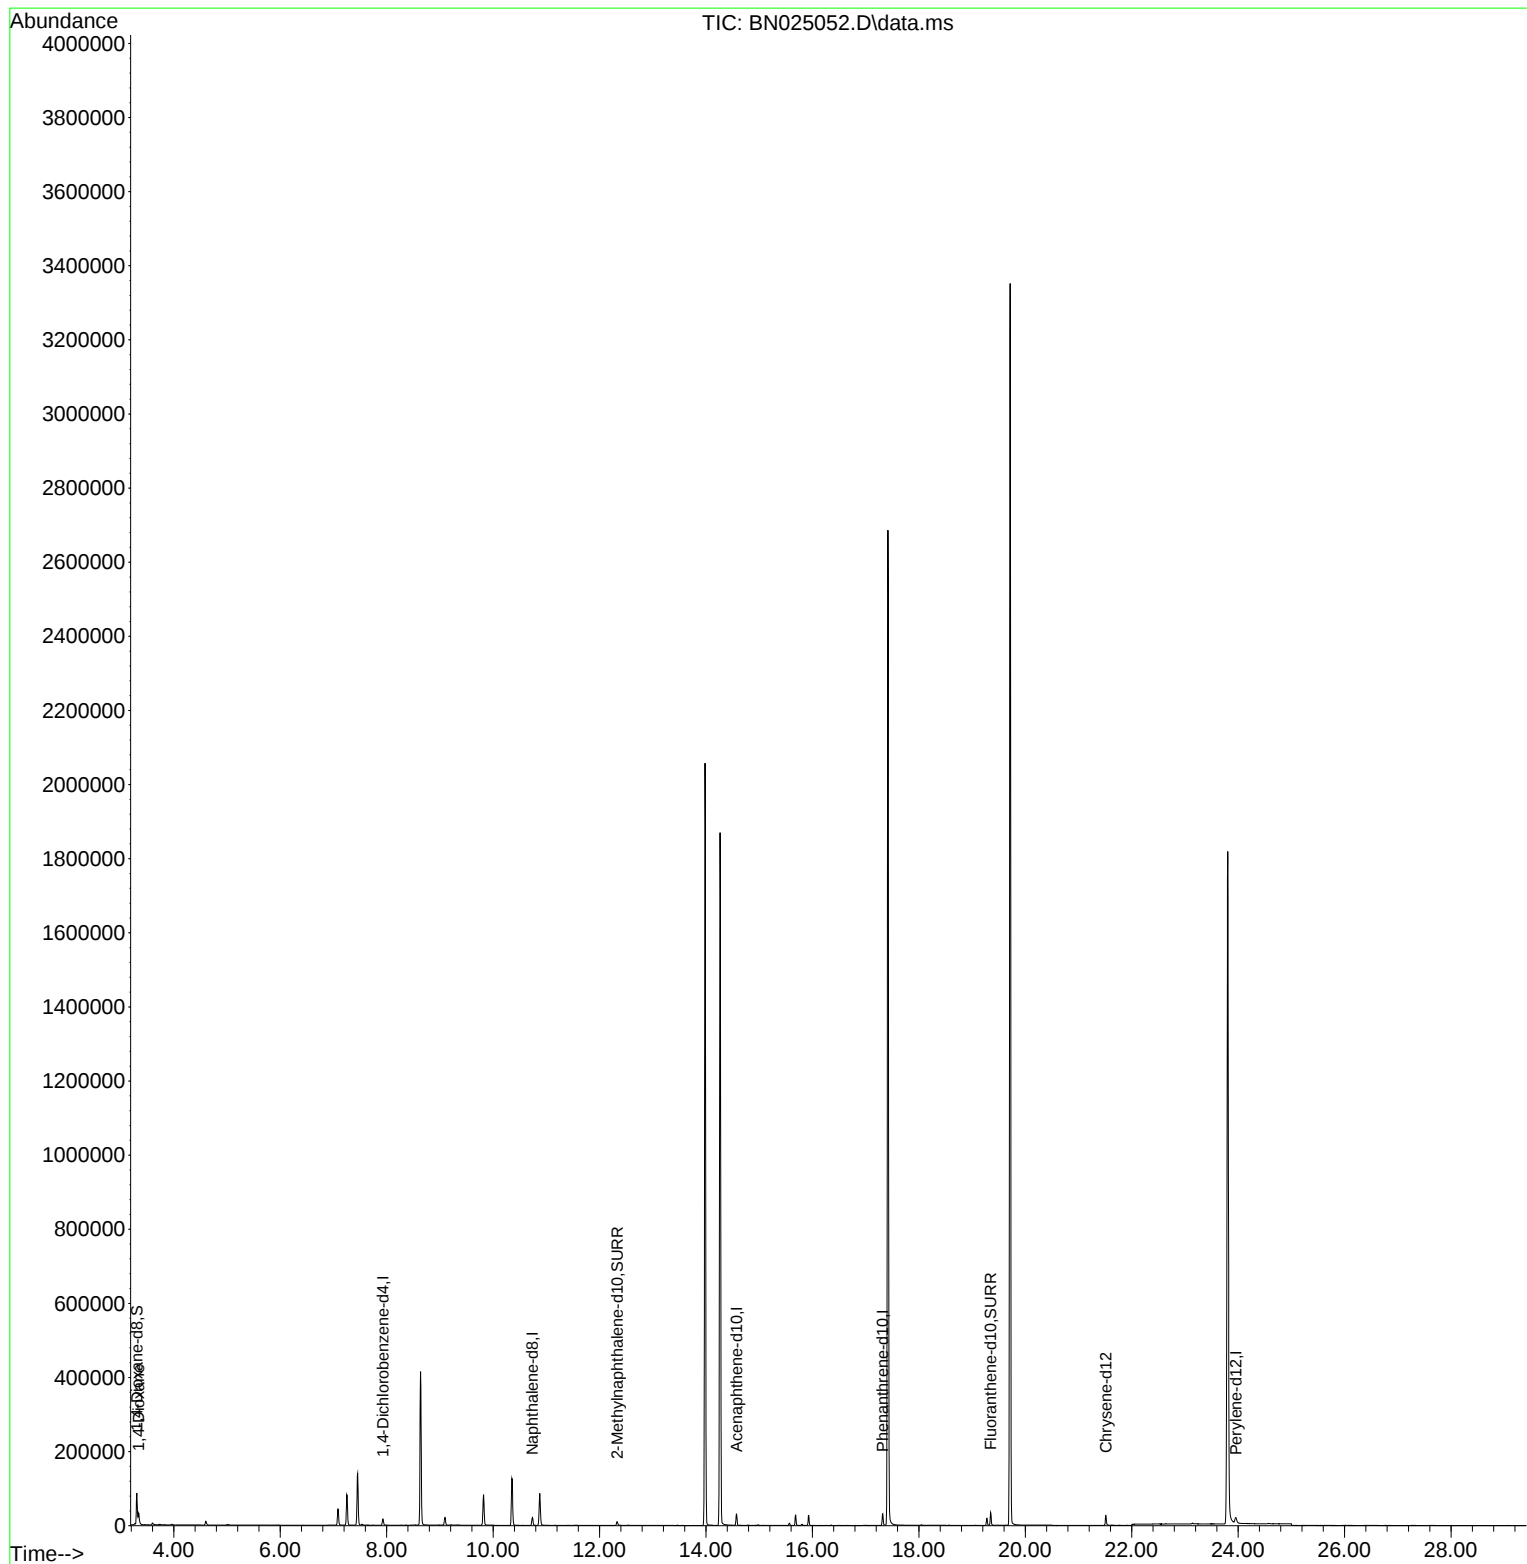

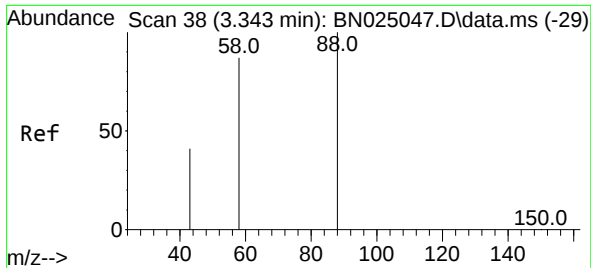

#2

1,4-Dioxane

Concen: 1.794 ng/ul

RT: 3.339 min Scan# 31

Delta R.T. -0.004 min

Lab File: BN025052.D


Acq: 21 Apr 2023 12:52

Instrument :

BNA_N

ClientSampleId :

BHE20

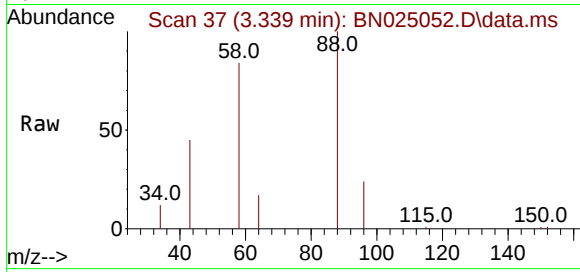

Tgt Ion: 88 Resp: 17354

Ion Ratio Lower Upper

88 100

43 44.6 37.0 55.4

58 84.4 56.9 85.3

