

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
 Data File : BN025066.D
 Acq On : 21 Apr 2023 21:48
 Operator : CG/JU
 Sample : 02392-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHE12

Quant Time: Apr 22 00:39:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 04:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	7045	0.400	ng/ul	0.00
4) Naphthalene-d8	10.737	136	22307	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.571	164	13120	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.318	188	28937	0.400	ng/ul	0.00
17) Chrysene-d12	21.506	240	22550	0.400	ng/ul	0.00
23) Perylene-d12	23.935	264	21517	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	42366	5.808	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	9963	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.346	212	27874	0.469	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	28359	3.610	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042123\
Data File : BN025066.D
Acq On : 21 Apr 2023 21:48
Operator : CG/JU
Sample : 02392-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHE12


Quant Time: Apr 22 00:39:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 04:13:07 2023
Response via : Initial Calibration

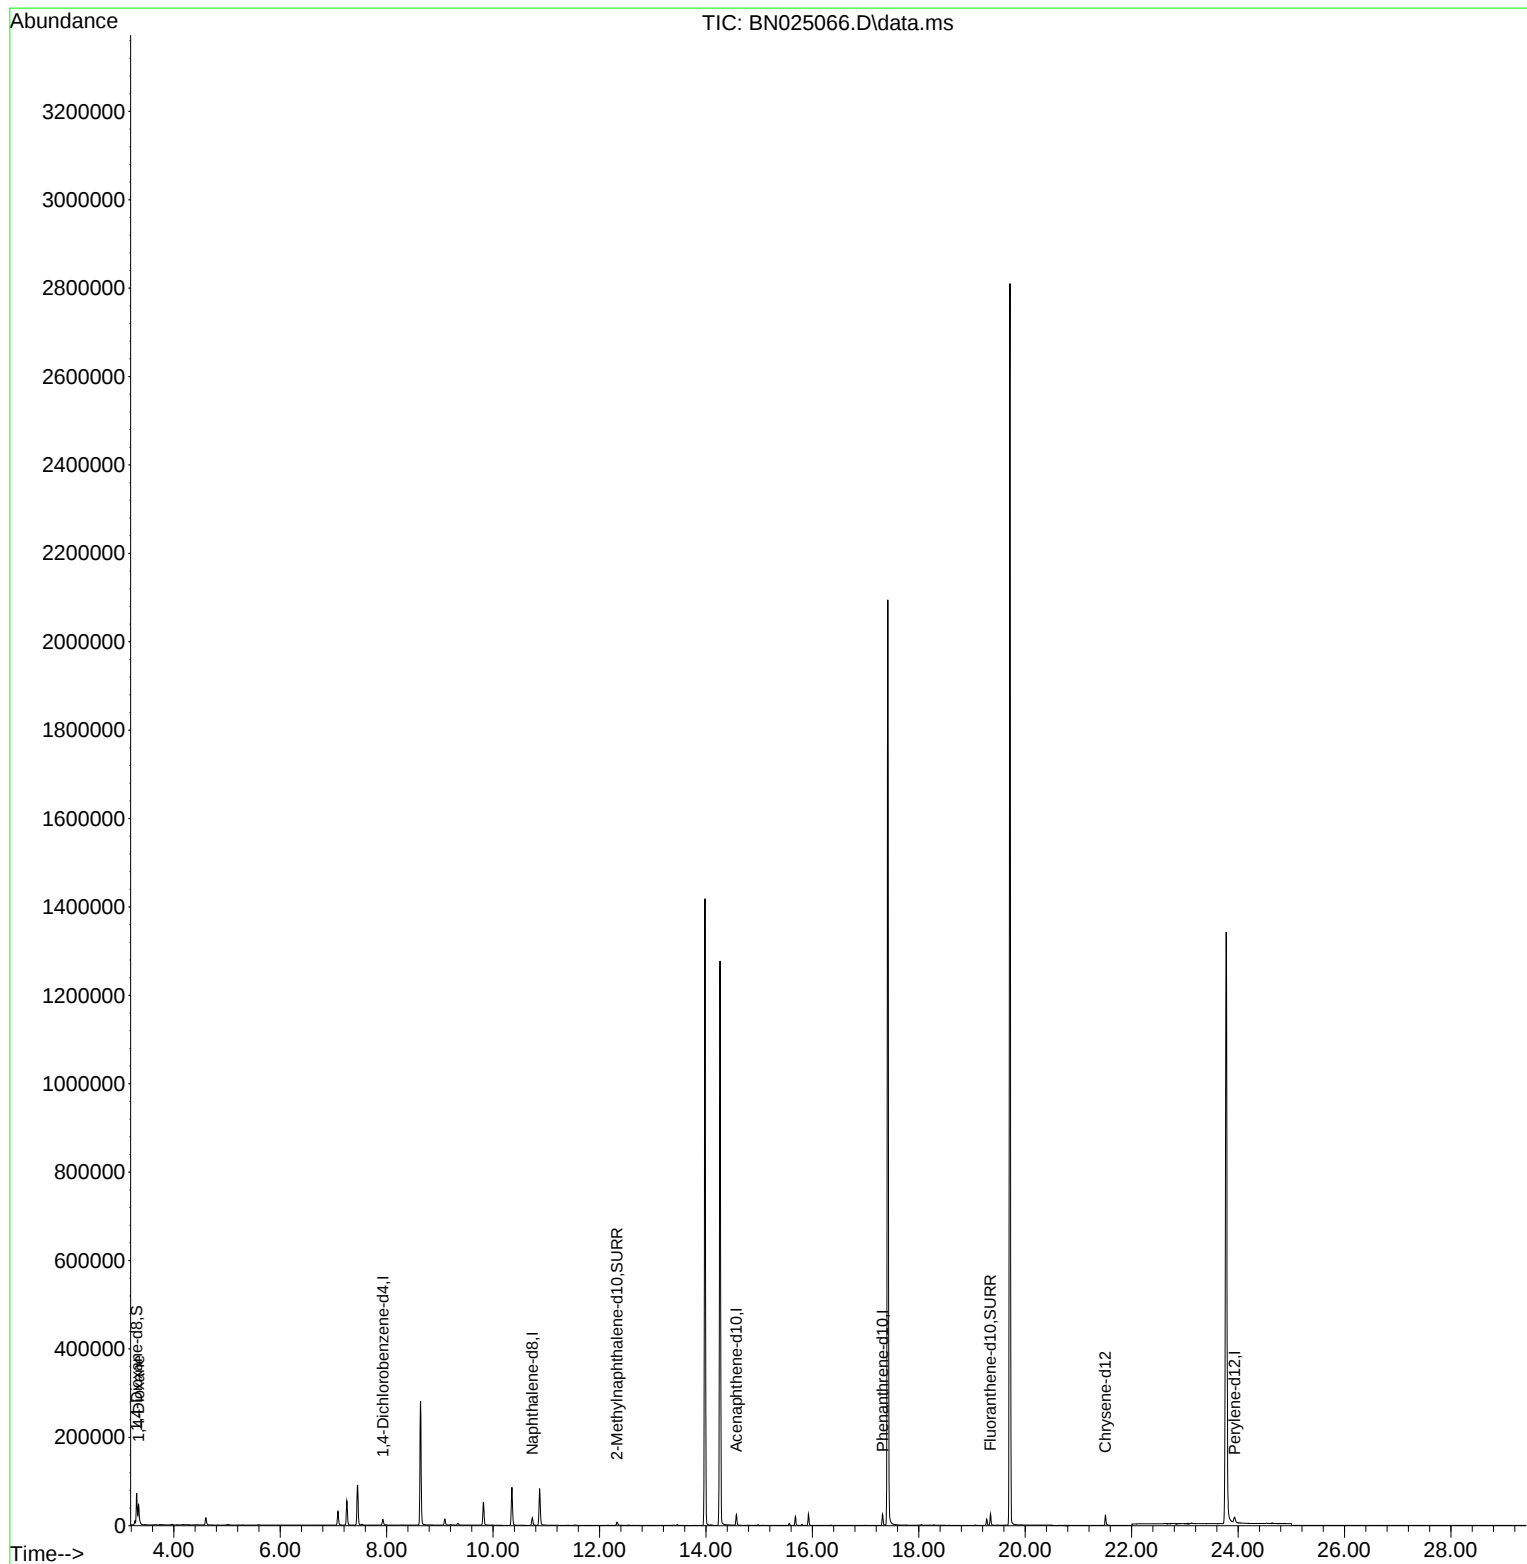

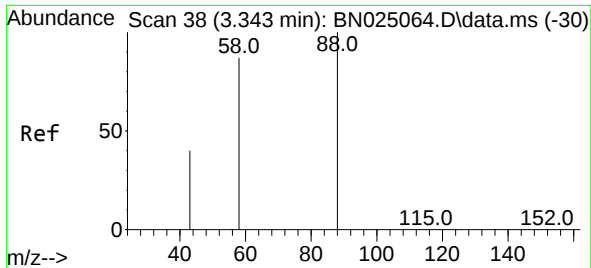

#2
 1,4-Dioxane
 Concen: 3.610 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN025066.D
 Acq: 21 Apr 2023 21:48

Instrument :
 BNA_N
 ClientSampleId :
 BHE12

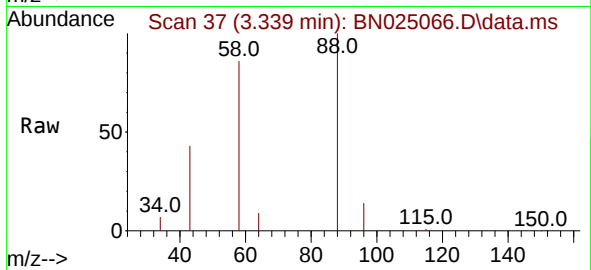

Tgt Ion:	88	Resp:	28359
Ion	Ratio	Lower	Upper
88	100		
43	43.3	37.0	55.4
58	86.5	56.9	85.3

