

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
 Data File : BN005174.D
 Acq On : 22 Apr 2019 15:12
 Operator : JU/SJ
 Sample : K2402-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHH4

Quant Time: Apr 23 03:41:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 04:25:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	393874	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1771309	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1129924	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	2586659	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	2271120	20.00	ng/ul	0.04
85) Perylene-d12	23.46	264	2266645	20.00	ng/ul	0.08

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	74793	9.17	ng/uL	0.00
5) Phenol-d5	6.77	99	899025	29.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	585631	30.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	707814	29.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	753355	31.15	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	356793	32.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	381088	34.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	759446	29.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1019545	39.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2765755	33.72	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3308165	32.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	417142	32.21	ng/ul	0.00
57) Fluorene-d10	15.23	176	2363567	34.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	332017	28.54	ng/ul	0.00
70) Anthracene-d10	17.09	188	3692725	34.05	ng/ul	0.00
78) Pyrene-d10	19.40	212	4052183	34.88	ng/ul	0.01
89) Benzo(a)pyrene-d12	23.32	264	3495666	35.29	ng/ul	0.08


Target Compounds					Qvalue
44) Dimethylphthalate	13.70	163	832976	10.192 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
Data File : BN005174.D
Acq On : 22 Apr 2019 15:12
Operator : JU/SJ
Sample : K2402-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHH4

Quant Time: Apr 23 03:41:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 04:25:06 2019
Response via : Initial Calibration

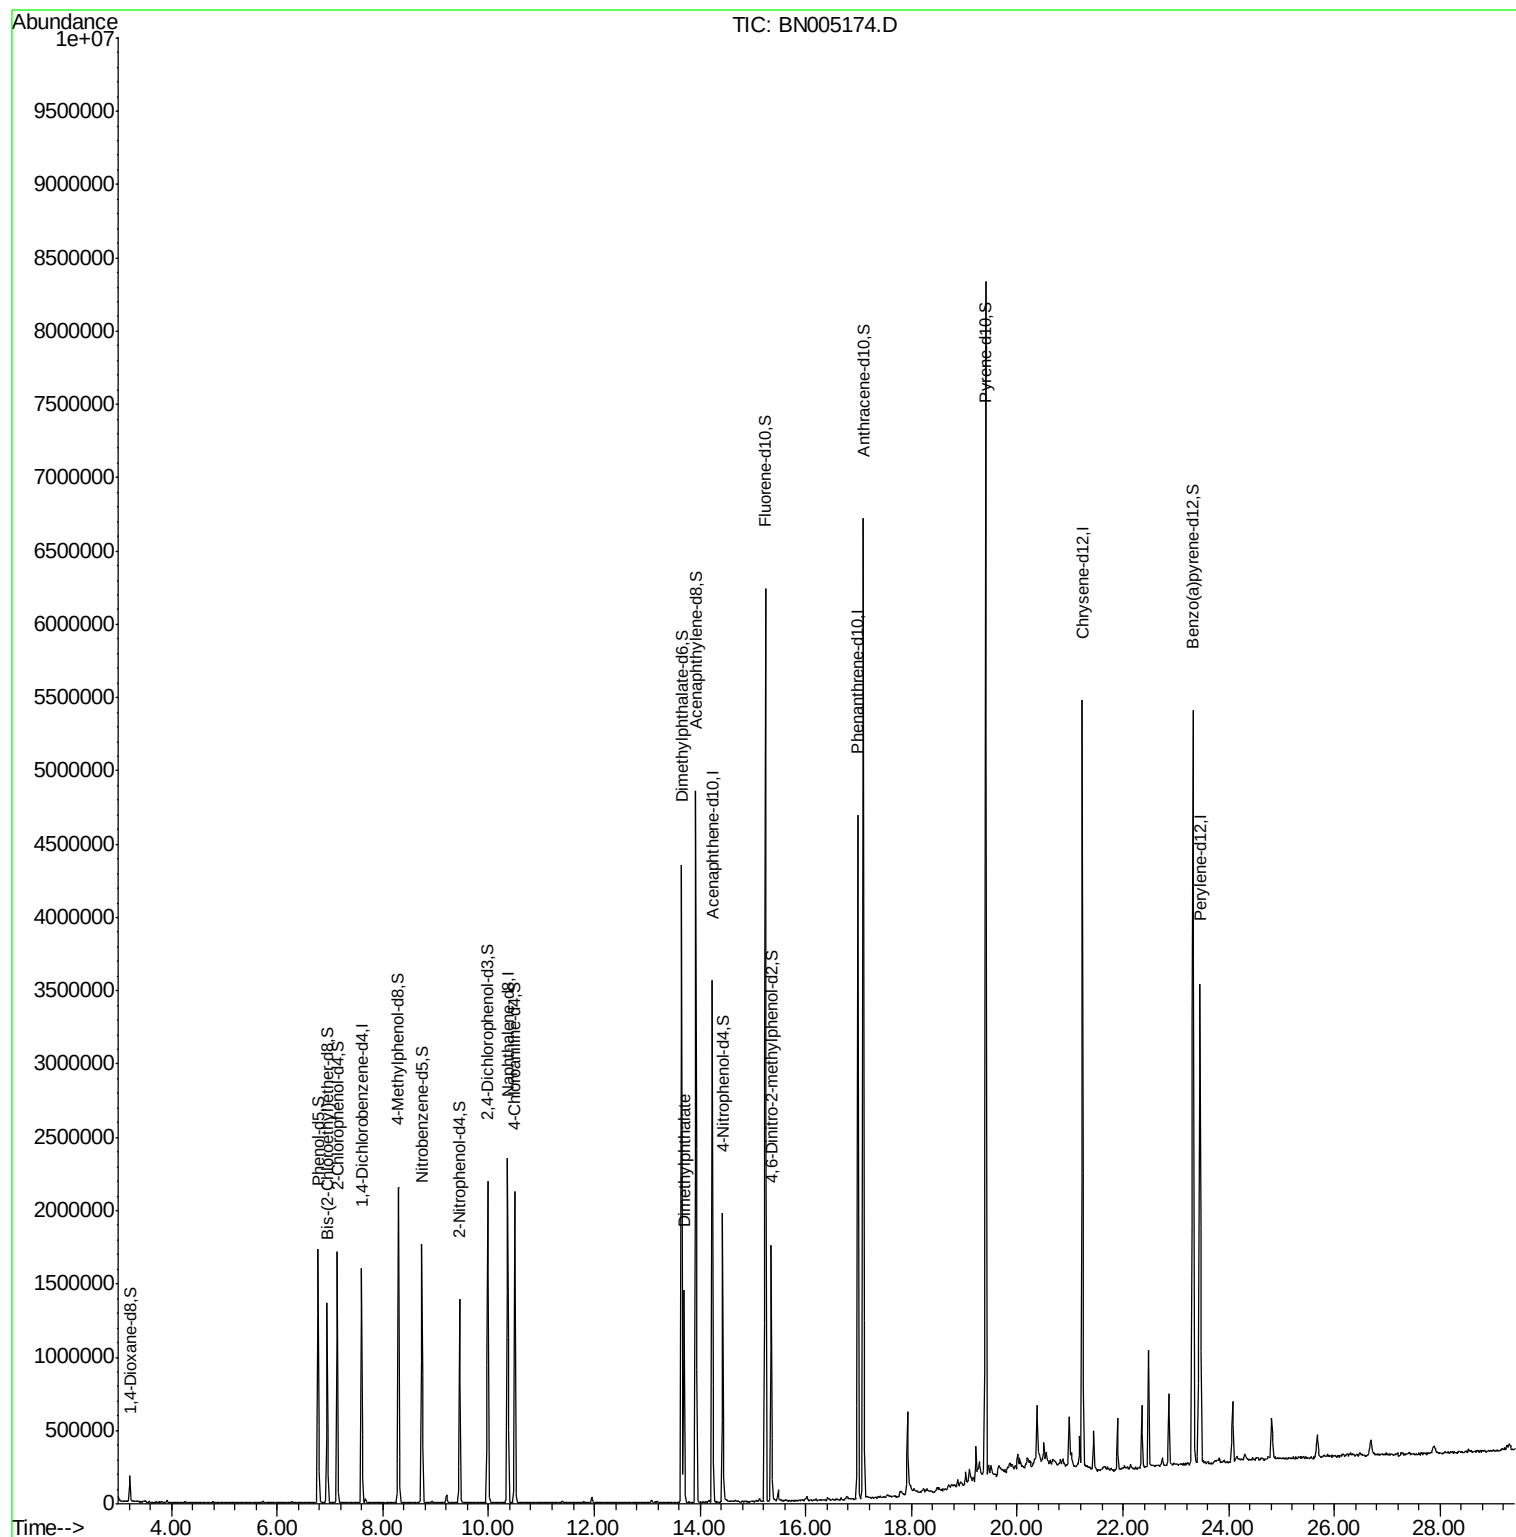

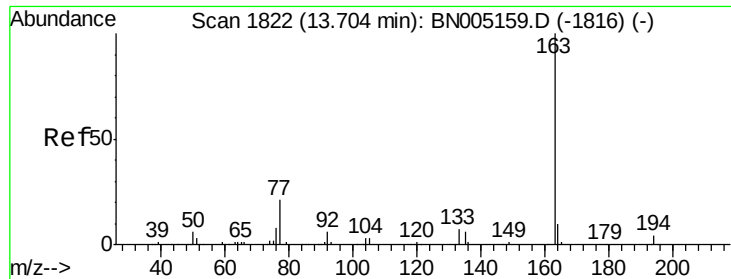

#44

Dimethylphthalate

Concen: 10.192 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BN005174.D

Acq: 22 Apr 2019 15:12

Instrument :

BNA_N

ClientSampleId :

GAHH4


Tgt Ion:163 Resp: 832976

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.2 8.1 12.1

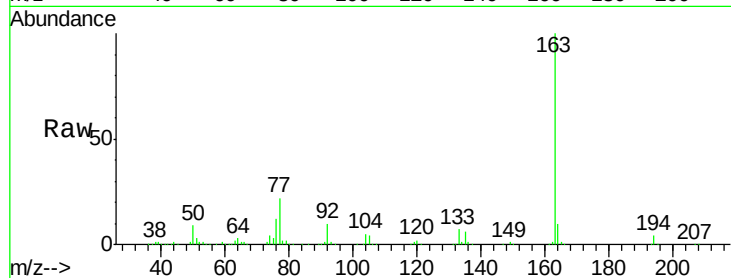

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

