

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
 Data File : BN005176.D
 Acq On : 22 Apr 2019 16:22
 Operator : JU/SJ
 Sample : K2402-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHH5

Quant Time: Apr 23 03:41:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 04:25:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	428559	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1867274	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1111339	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	2391468	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	2051993	20.00	ng/ul	0.02
85) Perylene-d12	23.43	264	2217734	20.00	ng/ul	0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	87991	9.91	ng/uL	0.00
5) Phenol-d5	6.78	99	1100541	32.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	678055	32.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	840164	32.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	890582	33.85	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	405651	35.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	446358	38.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	873731	32.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1152311	41.84	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2700235	33.47	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3328682	33.59	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	398892	31.31	ng/ul	0.00
57) Fluorene-d10	15.23	176	2248155	33.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	312806	29.08	ng/ul	0.00
70) Anthracene-d10	17.09	188	3334317	33.26	ng/ul	0.00
78) Pyrene-d10	19.40	212	3505402	33.39	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	3327979	34.34	ng/ul	0.04

Target Compounds


					Qvalue	
15) N-Nitroso-di-n-propylamine	8.30	70	24288	1.078	ng/ul#	1
44) Dimethylphthalate	13.70	163	812345	10.106	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
Data File : BN005176.D
Acq On : 22 Apr 2019 16:22
Operator : JU/SJ
Sample : K2402-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHH5

Quant Time: Apr 23 03:41:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 04:25:06 2019
Response via : Initial Calibration




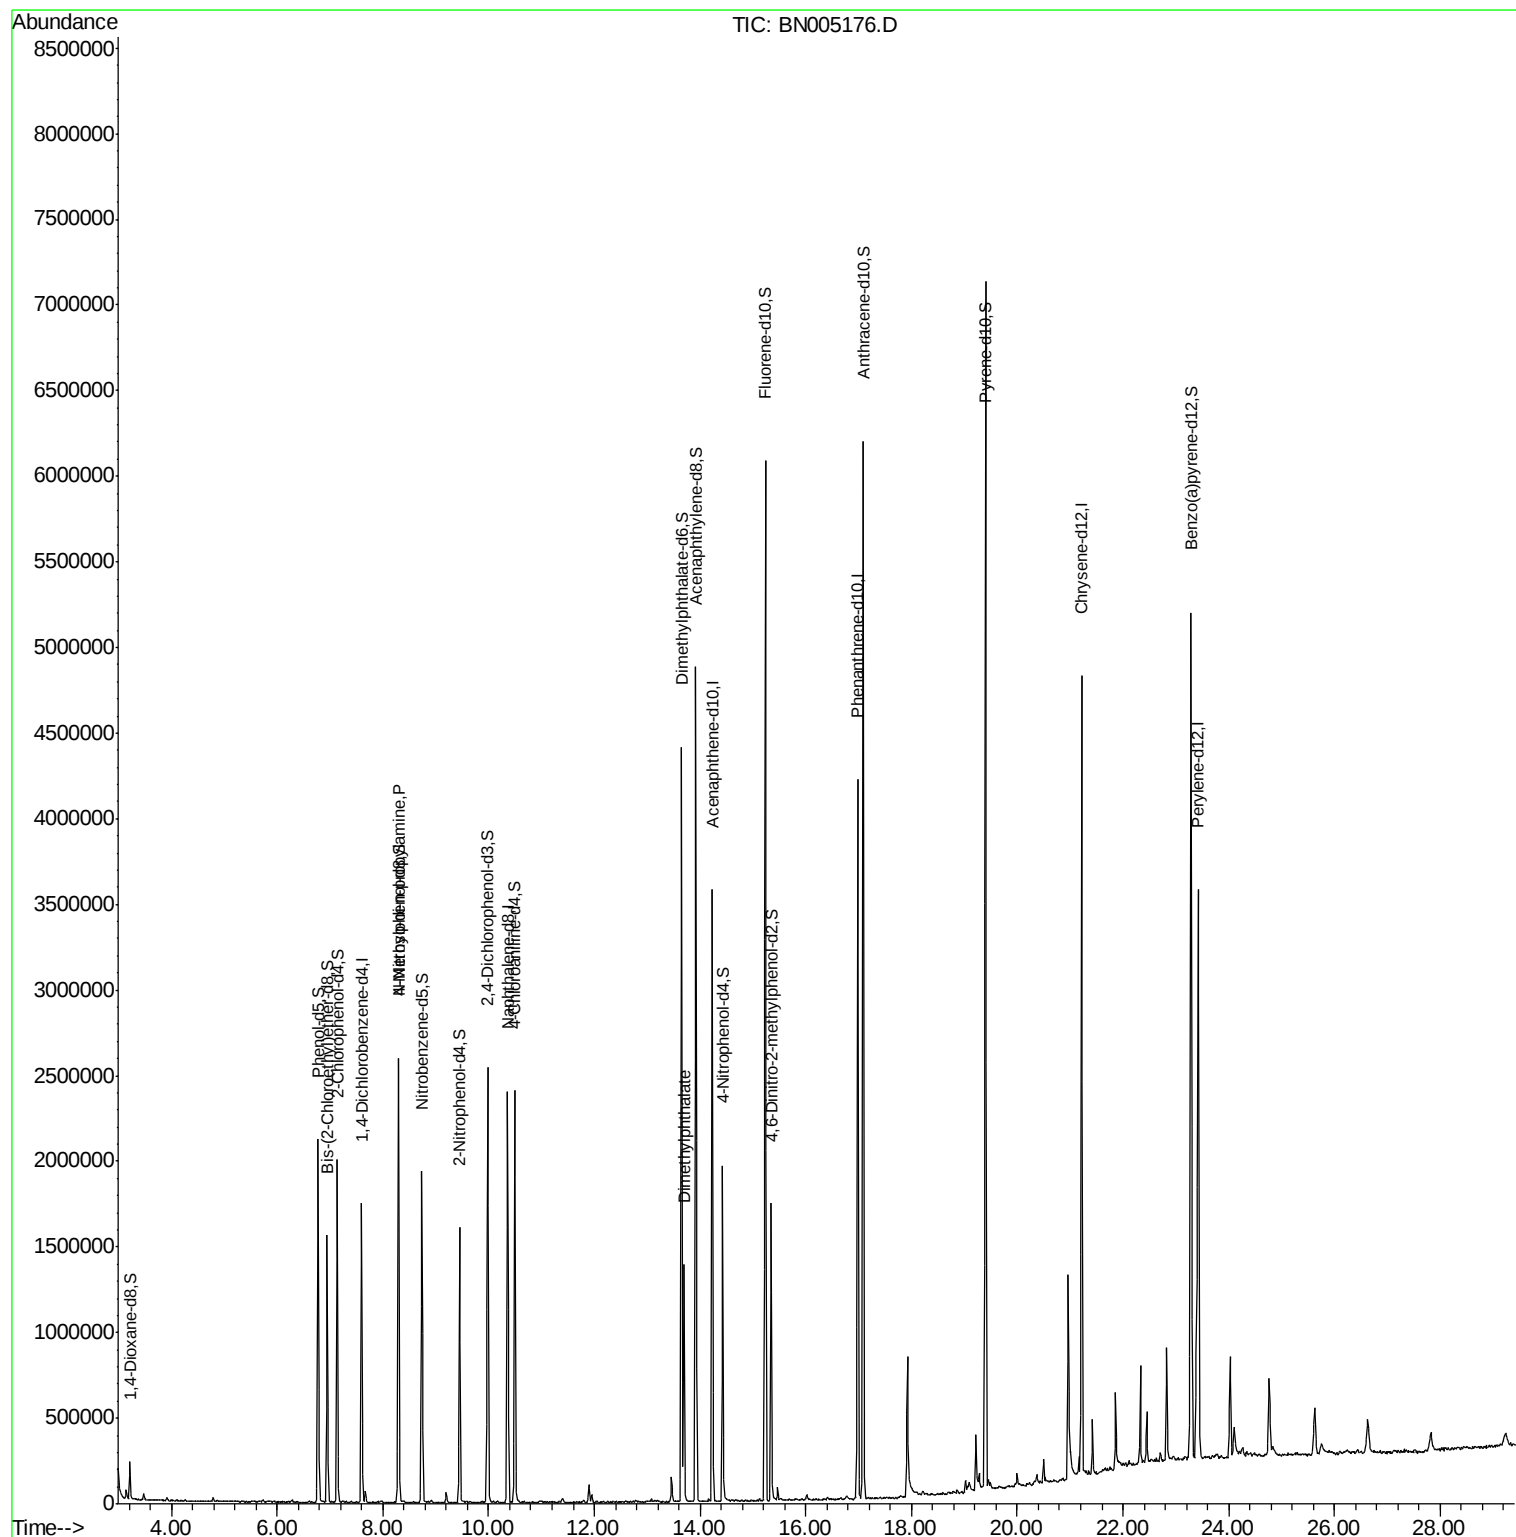


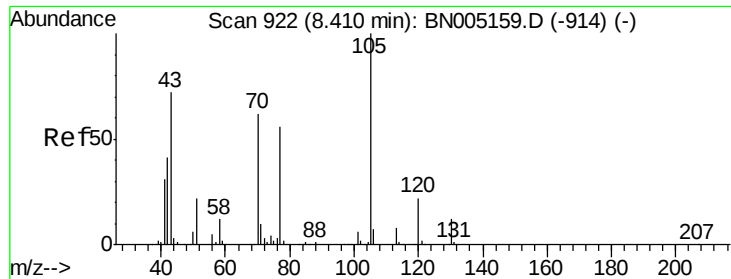

#15
N-Nitroso-di-n-propylamine
Concen: 1.078 ng/ul
RT: 8.30 min Scan# 903
Delta R.T. -0.11 min
Lab File: BN005176.D
Acq: 22 Apr 2019 16:22

Instrument :
BNA_N
ClientSampleId :
GAHH5

Tgt Ion: 70 Resp: 24288
Ion Ratio Lower Upper
70 100
42 372.7 53.8 80.8#
101 0.0 7.7 11.5#
130 0.0 15.0 22.4#

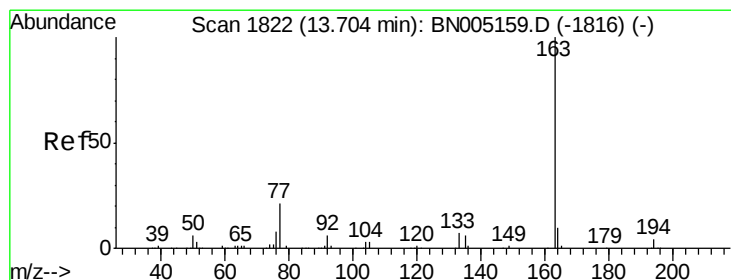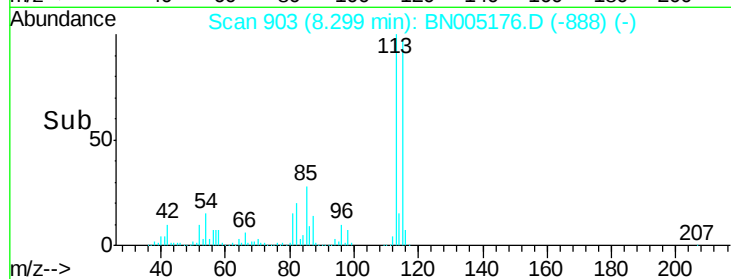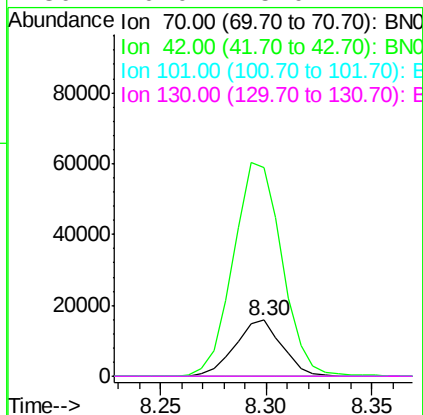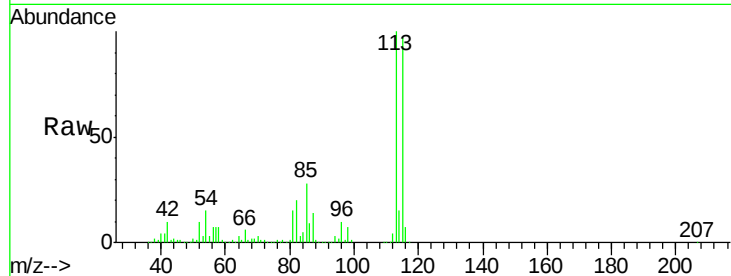

#44
Dimethylphthalate
Concen: 10.106 ng/ul
RT: 13.70 min Scan# 1821
Delta R.T. -0.01 min
Lab File: BN005176.D
Acq: 22 Apr 2019 16:22

Tgt Ion: 163 Resp: 812345
Ion Ratio Lower Upper
163 100
194 4.2 3.4 5.0
164 10.5 8.1 12.1

