

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
 Data File : BN005177.D
 Acq On : 22 Apr 2019 16:56
 Operator : JU/SJ
 Sample : K2402-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHH6

Quant Time: Apr 23 03:42:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 04:25:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	418827	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1803224	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1063594	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	2340525	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	2201423	20.00	ng/ul	0.02
85) Perylene-d12	23.43	264	2469735	20.00	ng/ul	0.05

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	75626	8.72	ng/uL	0.00
5) Phenol-d5	6.78	99	873324	26.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	555134	27.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	677845	26.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	699458	27.20	ng/ul	-0.01
19) Nitrobenzene-d5	8.74	128	326477	29.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	357670	31.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	689547	26.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	955144	35.91	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2252601	29.18	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	2711654	28.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	321621	26.38	ng/ul	0.00
57) Fluorene-d10	15.23	176	1869432	28.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	252990	24.03	ng/ul	0.00
70) Anthracene-d10	17.09	188	2847792	29.02	ng/ul	0.00
78) Pyrene-d10	19.40	212	3148797	27.96	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	3218254	29.82	ng/ul	0.05


Target Compounds					Qvalue
44) Dimethylphthalate	13.70	163	683295	8.882 ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
Data File : BN005177.D
Acq On : 22 Apr 2019 16:56
Operator : JU/SJ
Sample : K2402-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHH6

Quant Time: Apr 23 03:42:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 04:25:06 2019
Response via : Initial Calibration

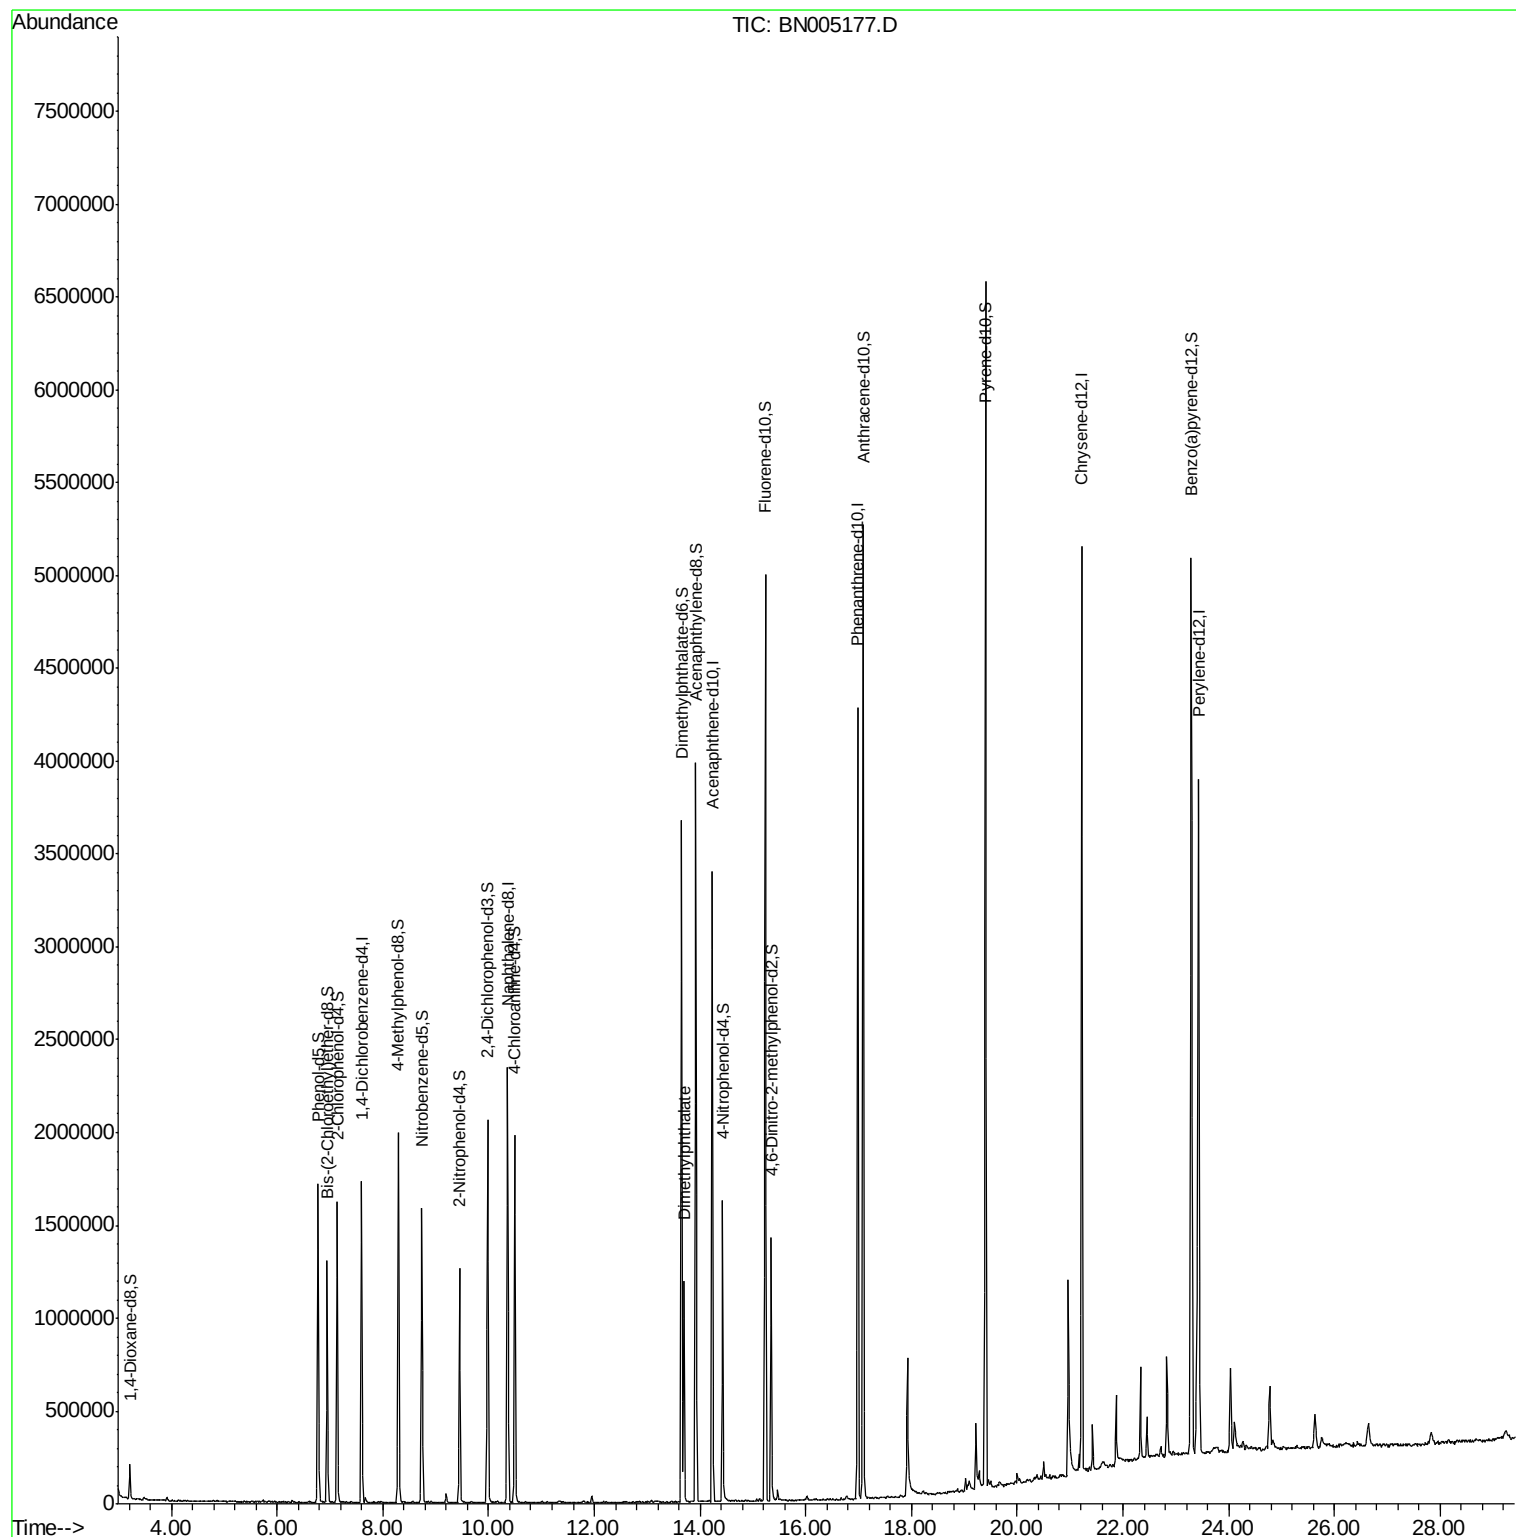

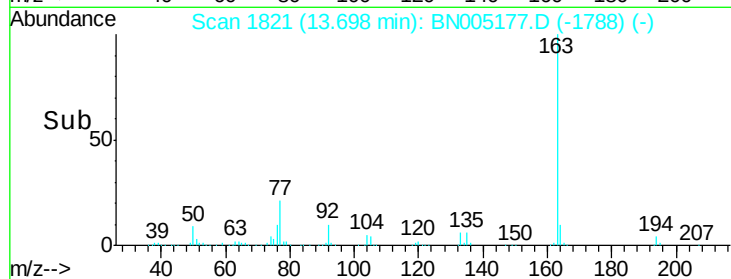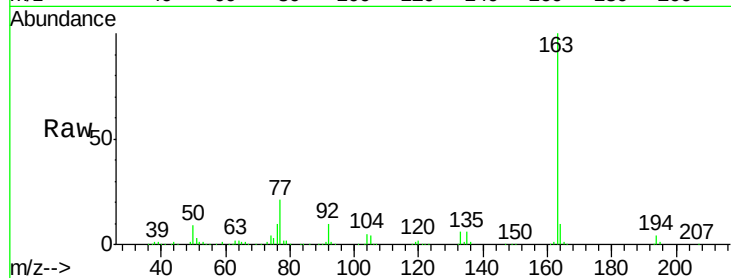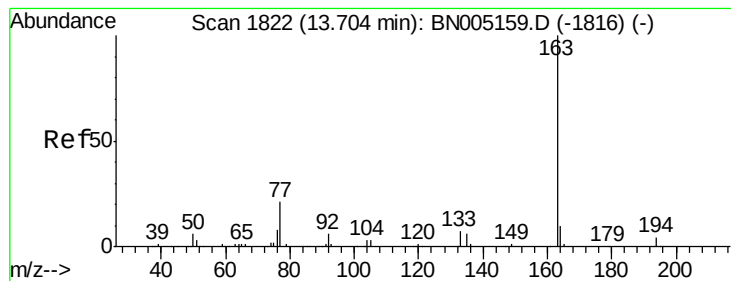

#44

Dimethylphthalate

Concen: 8.882 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BN005177.D

Acq: 22 Apr 2019 16:56

Instrument :

BNA_N

ClientSampleId :

GAHH6

Tgt Ion:163 Resp: 683295

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.3 8.1 12.1

