

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
 Data File : BN005178.D
 Acq On : 22 Apr 2019 17:31
 Operator : JU/SJ
 Sample : K2402-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHJ1

Quant Time: Apr 23 03:42:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 04:25:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	432451	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1925814	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1199906	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	2687306	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	2178428	20.00	ng/ul	0.03
85) Perylene-d12	23.45	264	2132470	20.00	ng/ul	0.06

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	82355	9.19	ng/uL	0.00
5) Phenol-d5	6.78	99	1117314	32.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	713439	33.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	862322	33.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	929746	35.02	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	440253	37.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	483290	40.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	927057	33.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1247641	43.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3115809	35.77	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3791163	35.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	484106	35.20	ng/ul	0.00
57) Fluorene-d10	15.23	176	2592735	35.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	379690	31.41	ng/ul	0.00
70) Anthracene-d10	17.09	188	3981812	35.35	ng/ul	0.00
78) Pyrene-d10	19.40	212	4202037	37.71	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	3415018	36.64	ng/ul	0.06

Target Compounds


					Qvalue	
15) N-Nitroso-di-n-propylamine	8.29	70	23958	1.054	ng/ul#	1
44) Dimethylphthalate	13.70	163	1064302	12.263	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
Data File : BN005178.D
Acq On : 22 Apr 2019 17:31
Operator : JU/SJ
Sample : K2402-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHJ1

Quant Time: Apr 23 03:42:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 04:25:06 2019
Response via : Initial Calibration

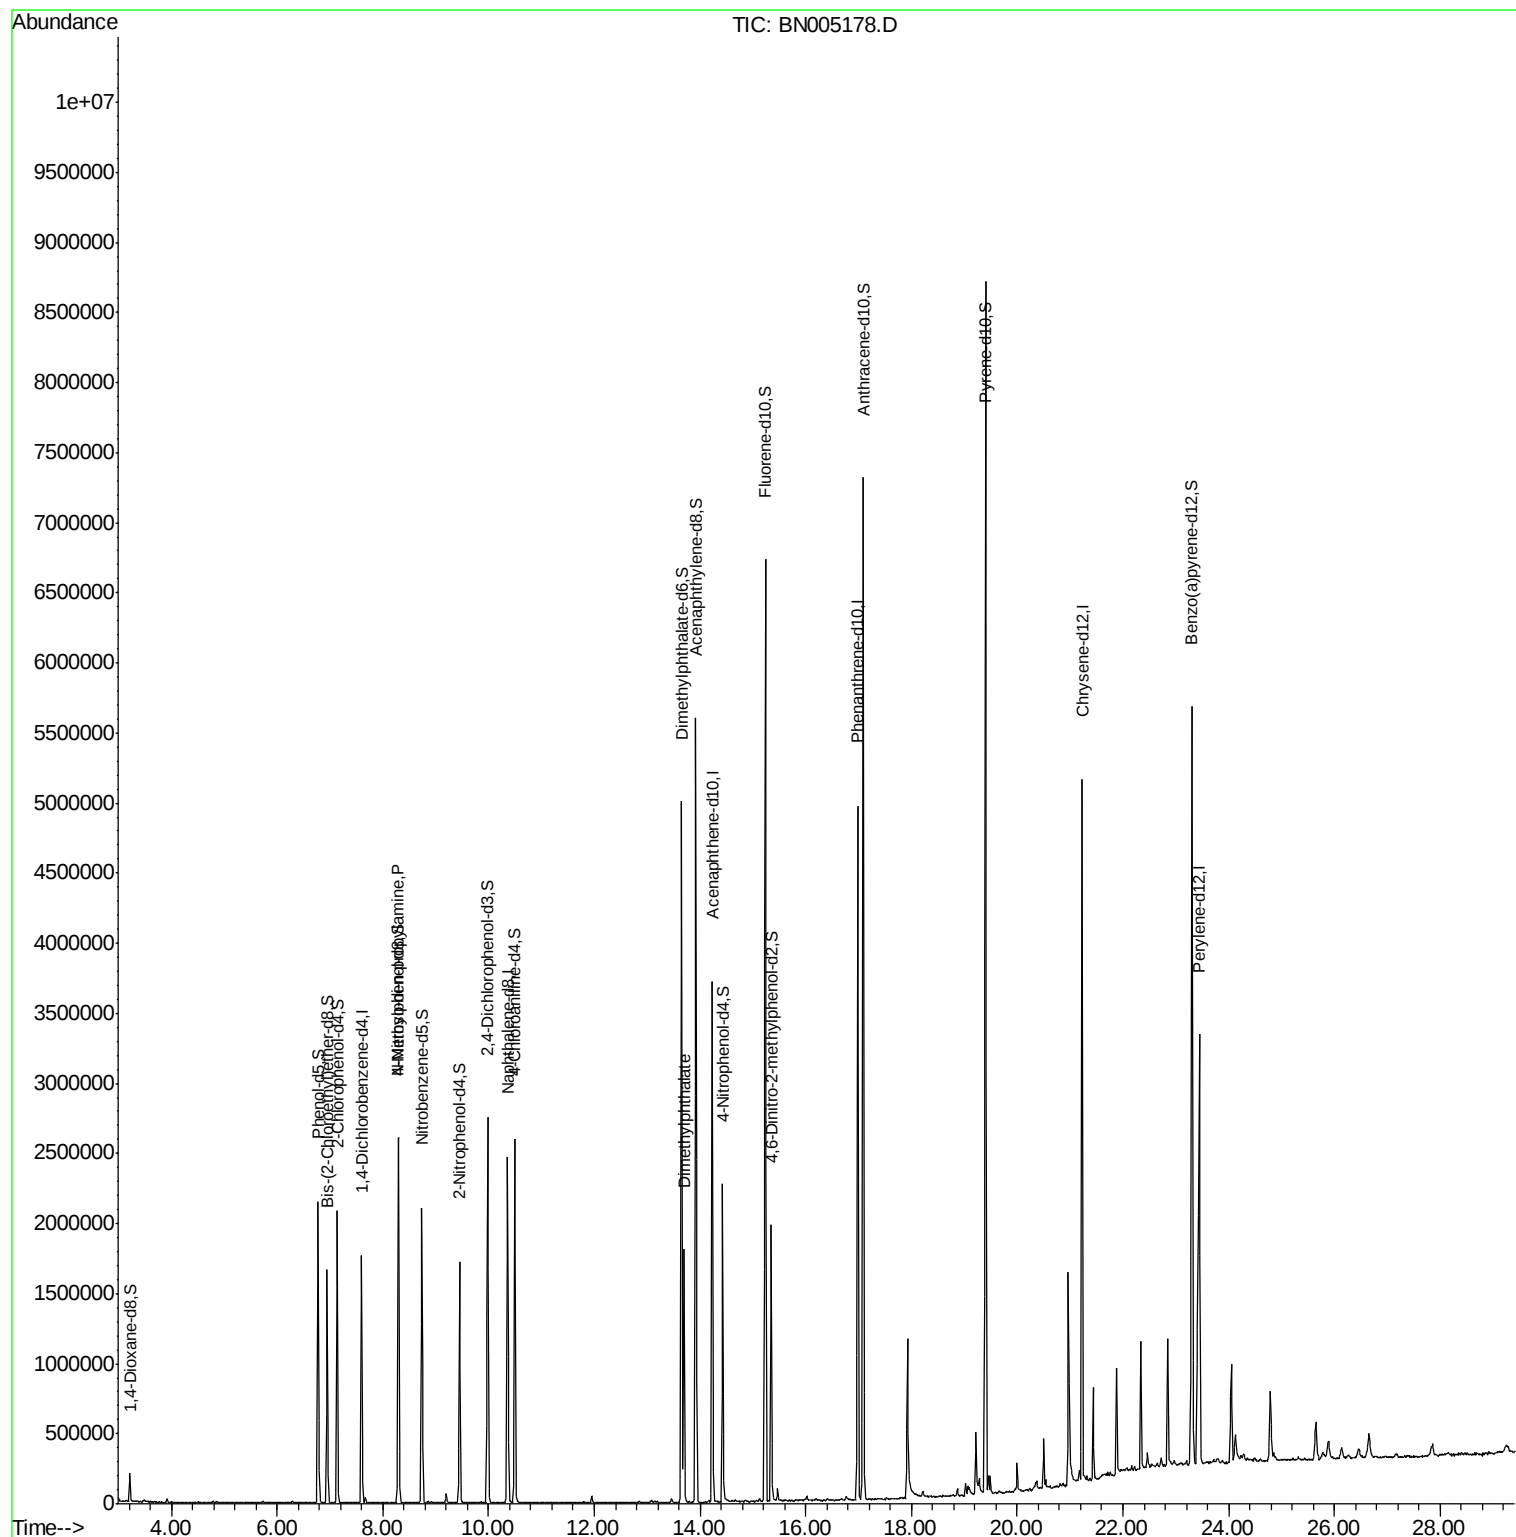

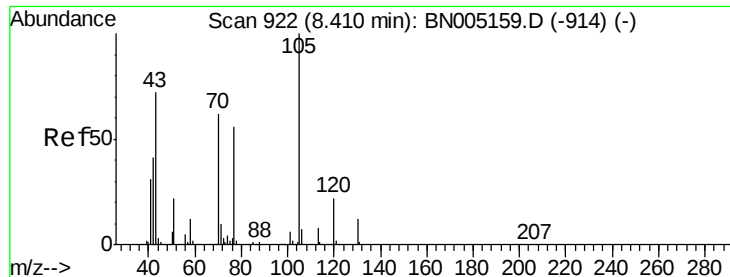

#15

N-Nitroso-di-n-propylamine

Concen: 1.054 ng/ul

RT: 8.29 min Scan# 902

Delta R.T. -0.12 min

Lab File: BN005178.D

Acq: 22 Apr 2019 17:31

Instrument :

BNA_N

ClientSampleId :

GAHJ1

Tgt Ion: 70 Resp: 23958


Ion Ratio Lower Upper

70 100

42 399.2 53.8 80.8#

101 0.0 7.7 11.5#

130 0.0 15.0 22.4#

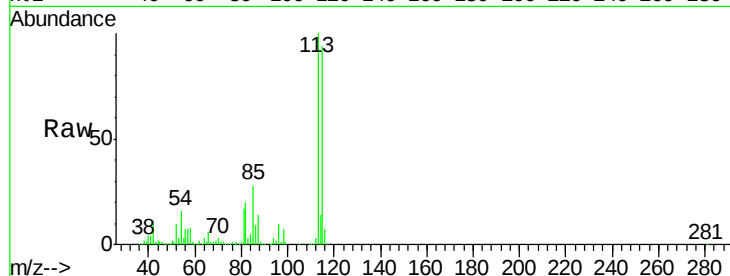


Abundance Ion 70.00 (69.70 to 70.70): BN0


Ion 42.00 (41.70 to 42.70): BN0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

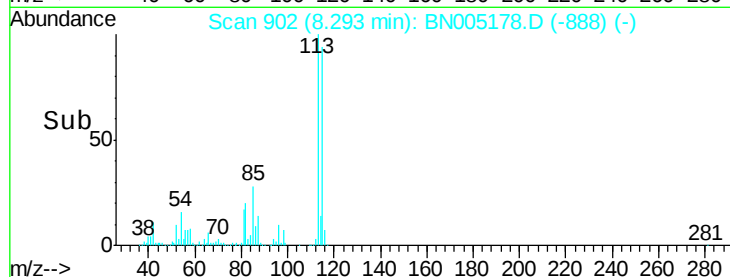

Time-->

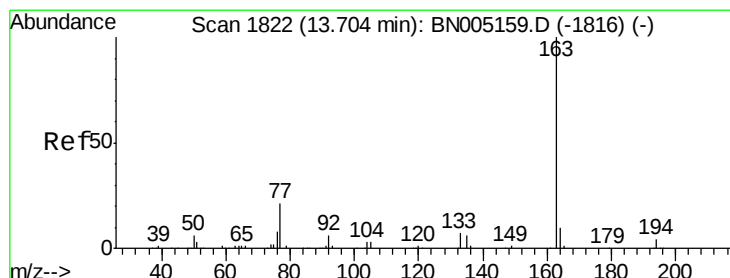

#44

Dimethylphthalate

Concen: 12.263 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BN005178.D

Acq: 22 Apr 2019 17:31


Tgt Ion:163 Resp: 1064302

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0


164 10.1 8.1 12.1

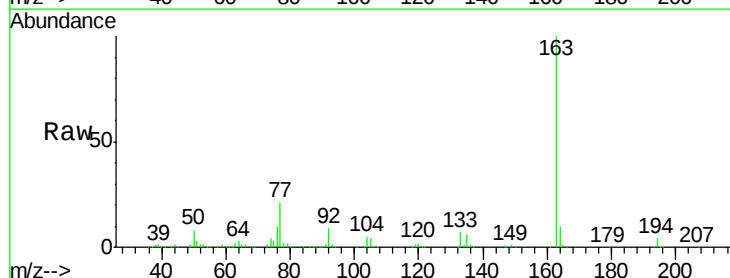

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

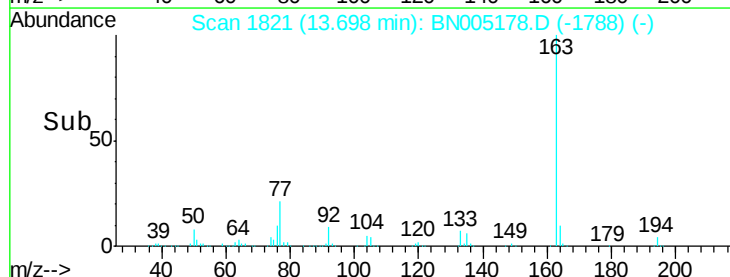

Time-->