

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042219\
 Data File : BN005188.D
 Acq On : 22 Apr 2019 23:18
 Operator : JU/SJ
 Sample : K2455-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHR4

Quant Time: Apr 23 03:43:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 04:25:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	439674	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1903203	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.23	164	1245438	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2828597	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	2441839	20.00	ng/ul	0.00
85) Perylene-d12	23.40	264	2558885	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	121005	13.29	ng/uL	0.00
5) Phenol-d5	6.78	99	1554180	45.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	986936	45.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	1221046	46.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1282994	47.53	ng/ul	-0.01
19) Nitrobenzene-d5	8.74	128	613535	52.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	683096	57.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1258457	46.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	1729200	61.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3831091	42.38	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	4775826	43.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	585923	41.04	ng/ul	0.00
57) Fluorene-d10	15.23	176	3195163	42.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	484362	38.07	ng/ul	0.00
70) Anthracene-d10	17.08	188	4719725	39.80	ng/ul	0.00
78) Pyrene-d10	19.39	212	4884037	39.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	4552960	40.71	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	713818	7.924	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042219\
Data File : BN005188.D
Acq On : 22 Apr 2019 23:18
Operator : JU/SJ
Sample : K2455-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHR4

Quant Time: Apr 23 03:43:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 04:25:06 2019
Response via : Initial Calibration

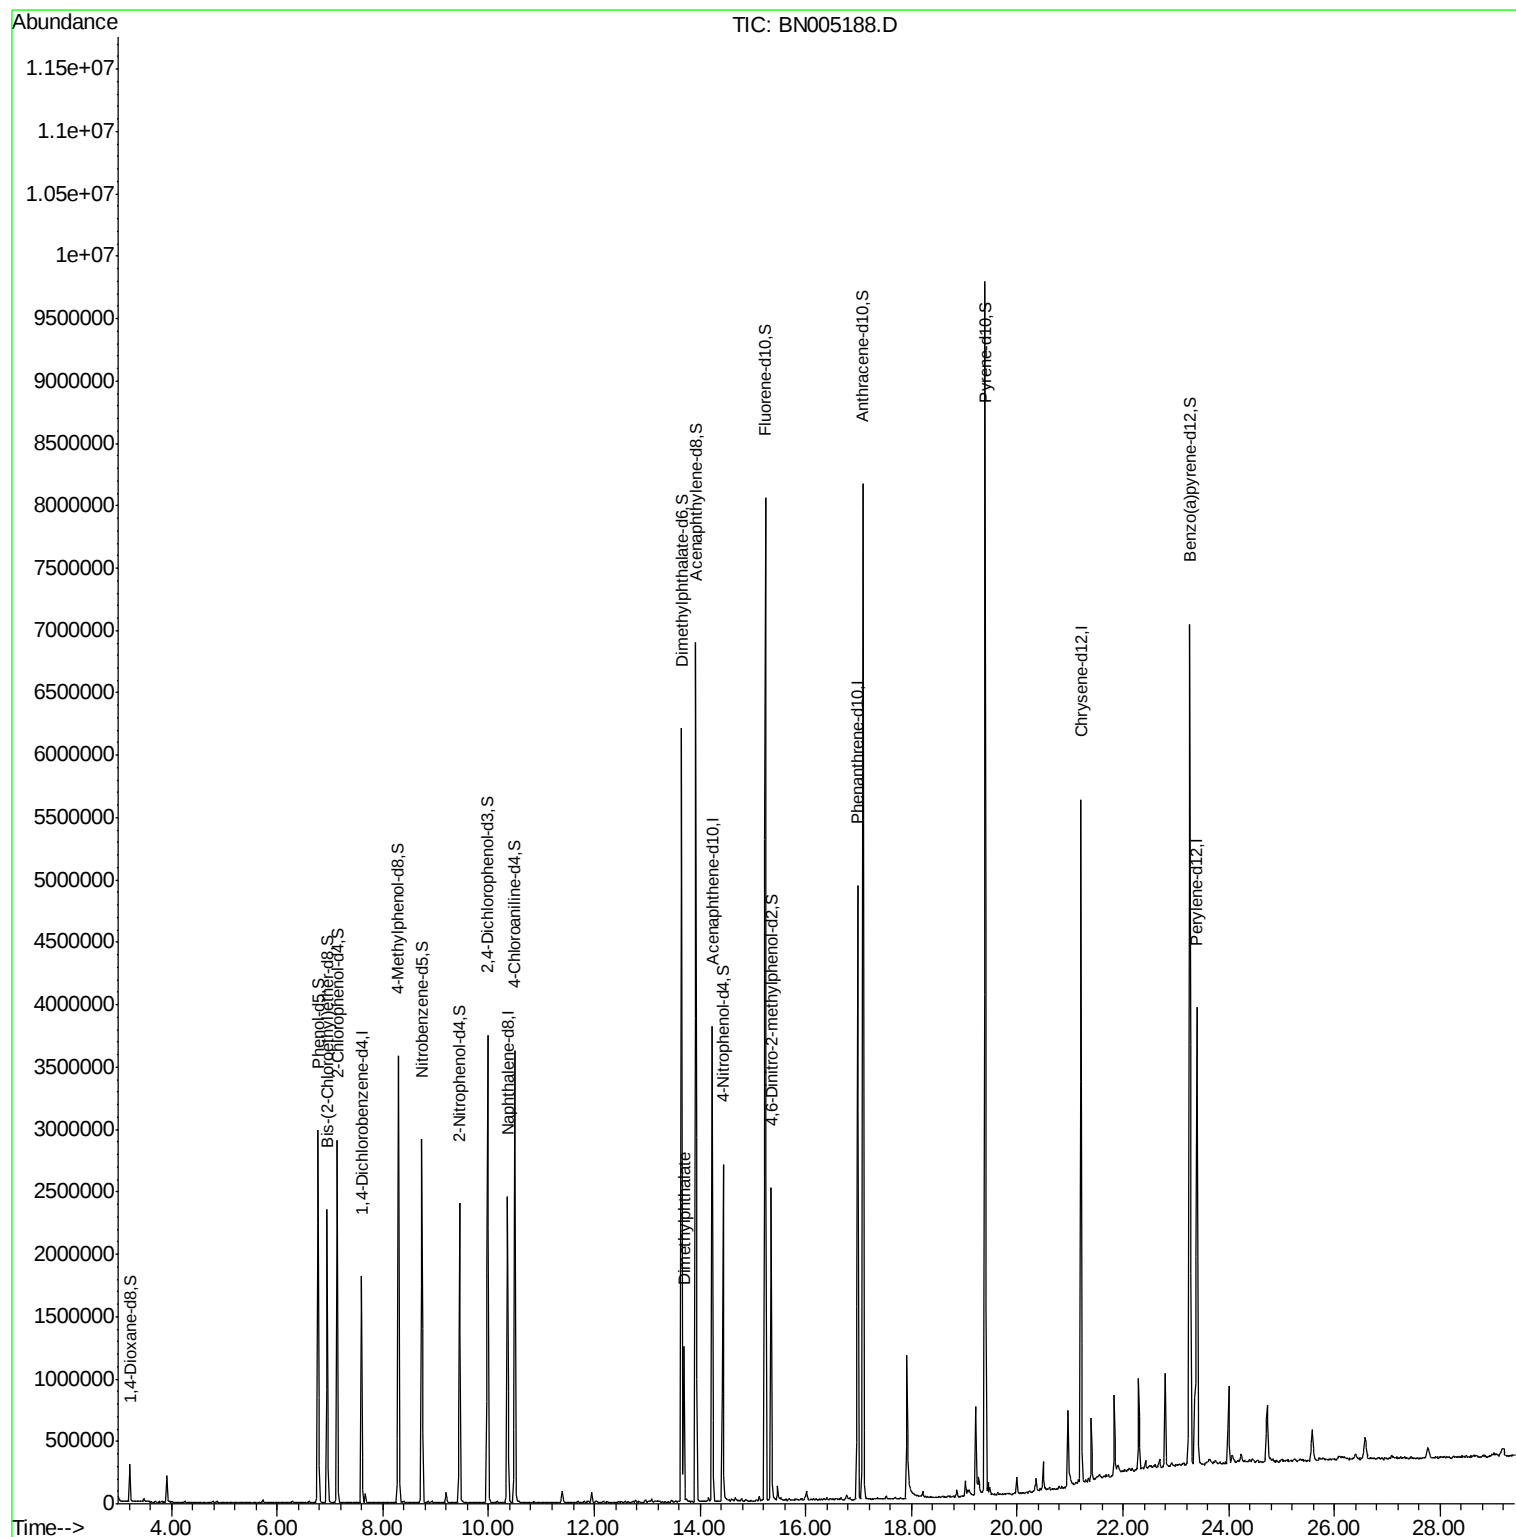


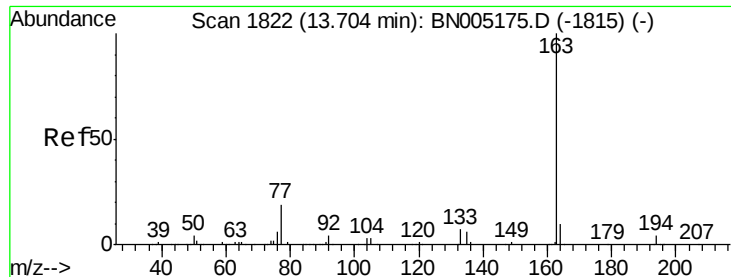

#44
 Dimethylphthalate
 Concen: 7.924 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BN005188.D
 Acq: 22 Apr 2019 23:18

Instrument :
 BNA_N
 ClientSampleId :
 GAHR4

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.0
164	10.6	8.1	12.1

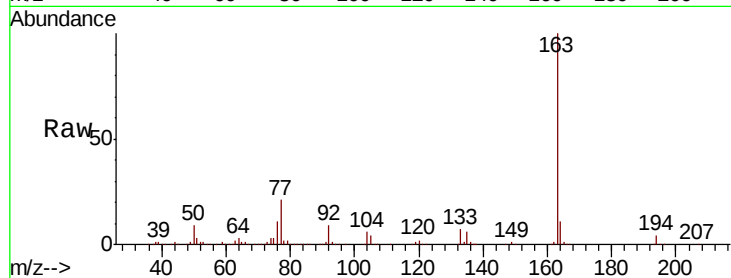

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

