

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042219\
 Data File : BN005205.D
 Acq On : 23 Apr 2019 09:40
 Operator : JU/SJ
 Sample : K2455-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHR2

Quant Time: Apr 23 10:24:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 23 03:50:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	258795	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1215219	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	782795	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	1755264	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	1504163	20.00	ng/ul	0.01
85) Perylene-d12	23.44	264	1619719	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	71641	13.37	ng/uL	0.00
5) Phenol-d5	6.78	99	857393	42.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	537075	42.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	701854	45.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	677748	42.66	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	331522	44.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	354680	46.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	698139	40.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	706500	39.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	1923816	33.86	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	2595313	37.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	281651	31.39	ng/ul	0.00
57) Fluorene-d10	15.23	176	1752302	36.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	76907	9.74	ng/ul	0.00
70) Anthracene-d10	17.09	188	2663809	36.20	ng/ul	0.00
78) Pyrene-d10	19.40	212	2692366	34.99	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.31	264	2576300	36.40	ng/ul	0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	366771	6.478	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042219\
Data File : BN005205.D
Acq On : 23 Apr 2019 09:40
Operator : JU/SJ
Sample : K2455-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHR2

Quant Time: Apr 23 10:24:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 23 03:50:45 2019
Response via : Initial Calibration

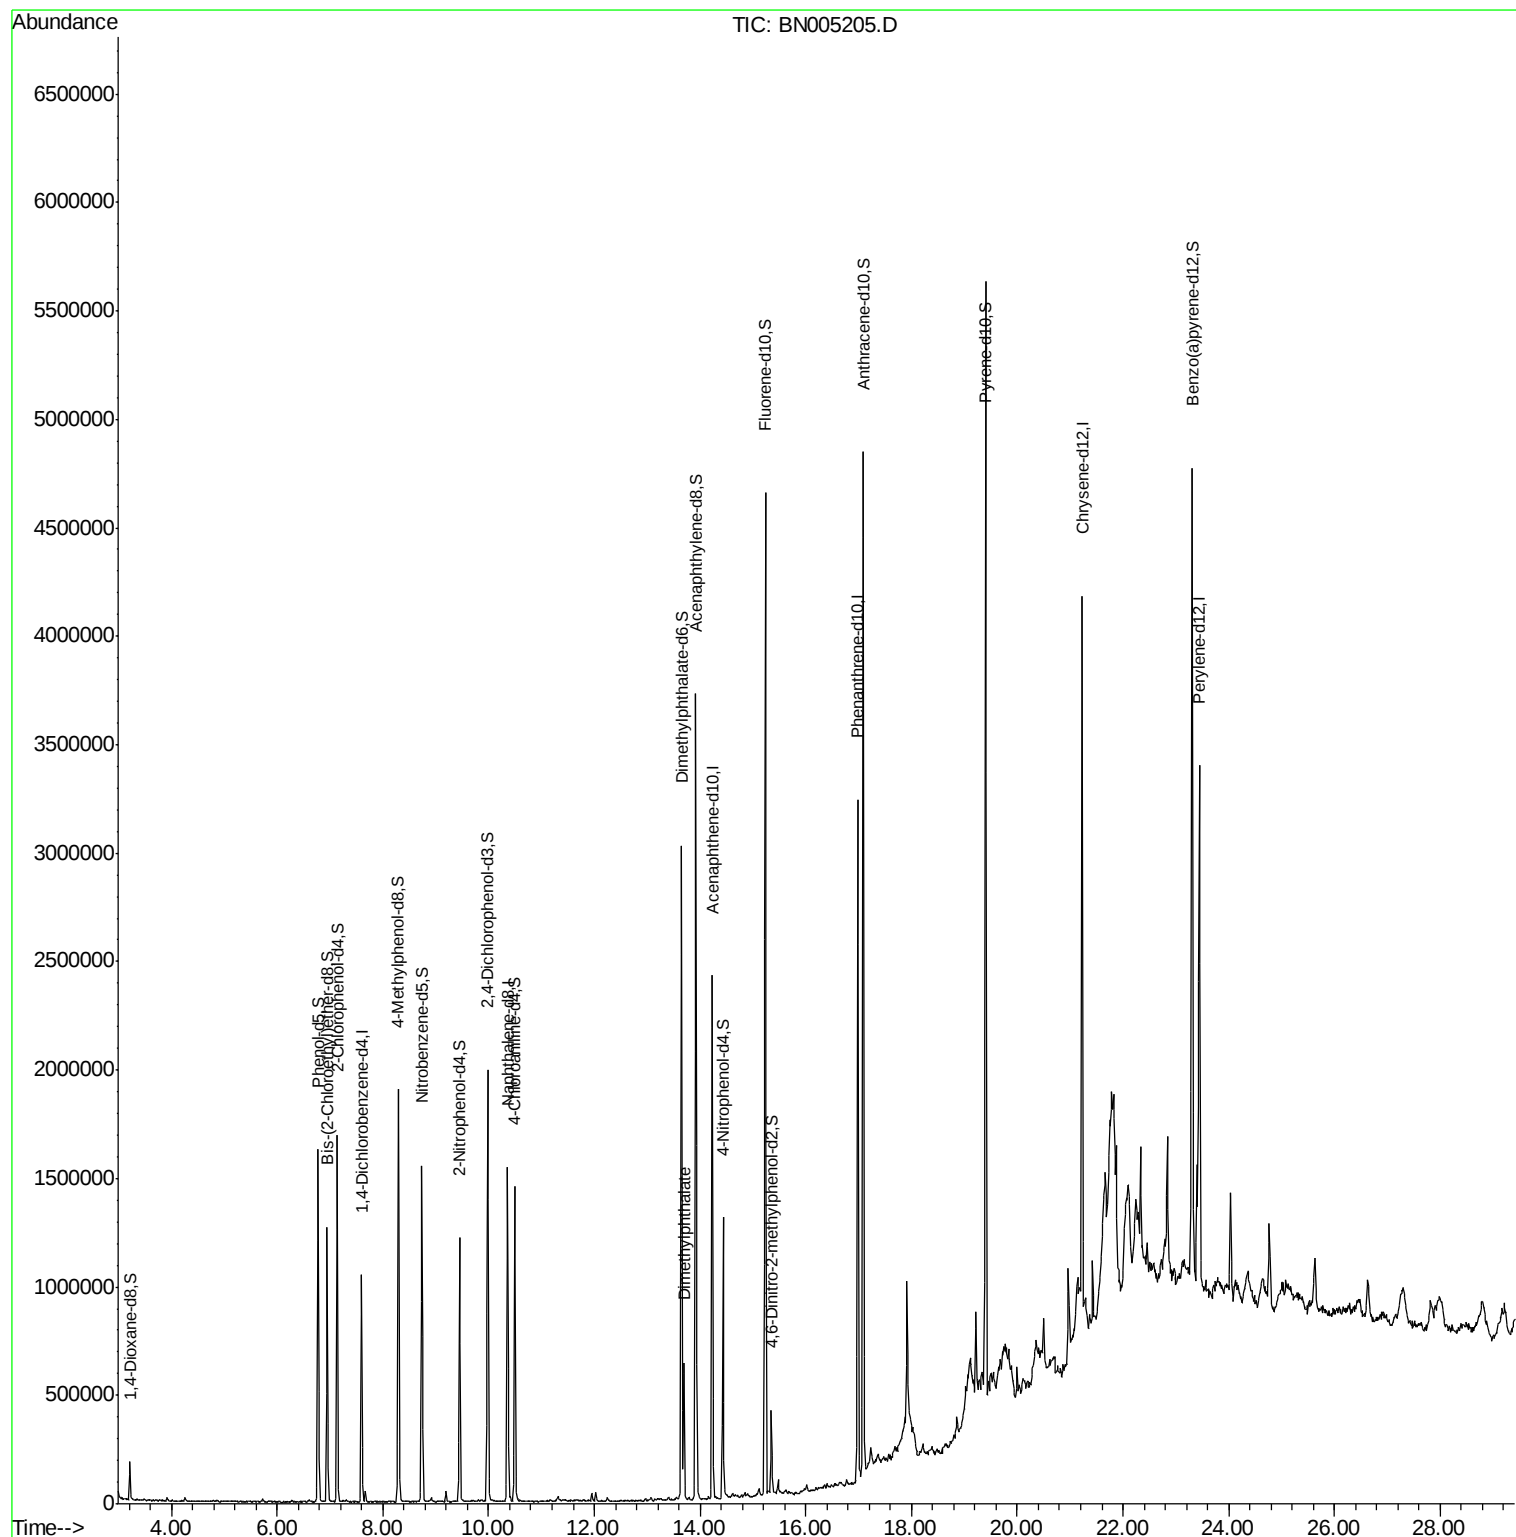

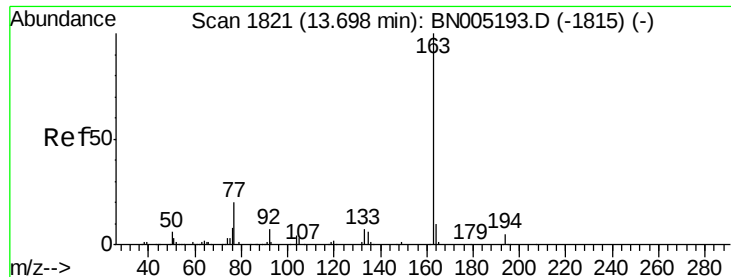

#44

Dimethylphthalate

Concen: 6.478 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BN005205.D

Acq: 23 Apr 2019 09:40

Instrument :

BNA_N

ClientSampleId :

GAHR2


Tot Ion:163 Resp: 366771

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.3 8.1 12.1

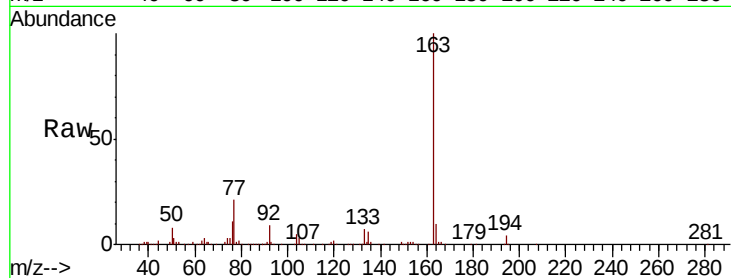

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

